

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
 Data File : FF008604.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jun 2021 12:54
 Operator : DD\AJ
 Sample : M2639-01 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 14 07:20:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.769	133708	1.269 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.967	198997	1.624 ug/ml
15) N-TETRATRIACONTANE	19.409	11690	0.106 ug/ml
16) N-HEXATRIACONTANE	20.116f	37084	0.334 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
Data File : FF008604.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2021 12:54
Operator : DD\AJ
Sample : M2639-01 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 07:20:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

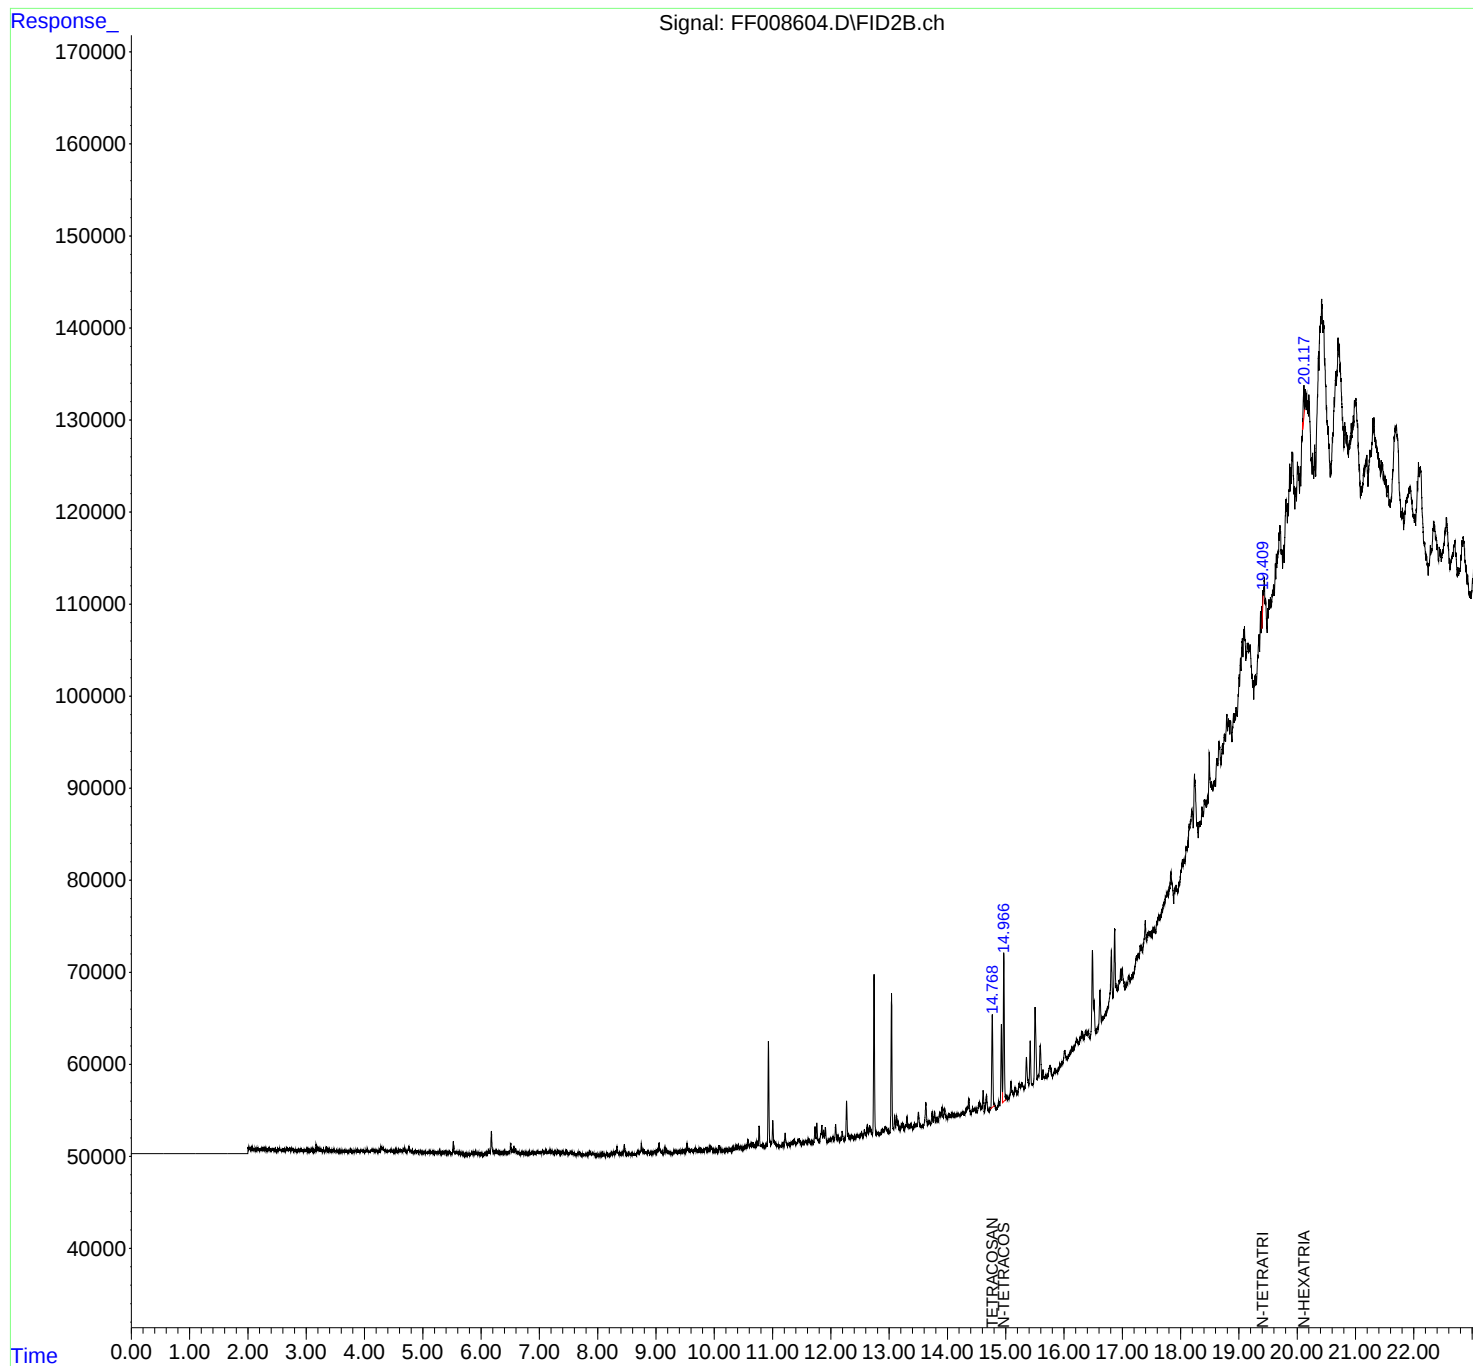


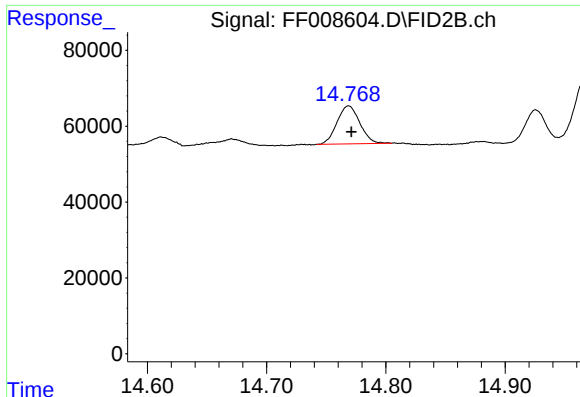

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.769 min
Delta R.T.: -0.002 min
Response: 133708
Conc: 1.27 ug/ml

Instrument :
FID_F
ClientSampleId :

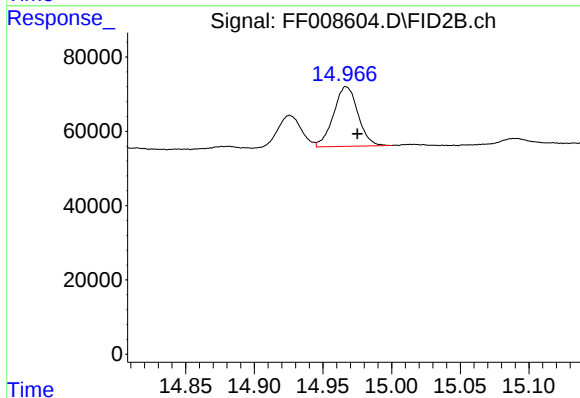


#10 N-TETRACOSANE

R.T.: 14.967 min
Delta R.T.: -0.009 min
Response: 198997
Conc: 1.62 ug/ml

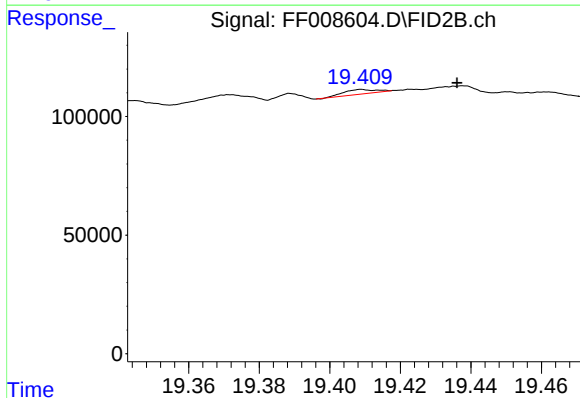

#15 N-TETRATRIACONTANE

R.T.: 19.409 min
Delta R.T.: -0.027 min
Response: 11690
Conc: 0.11 ug/ml

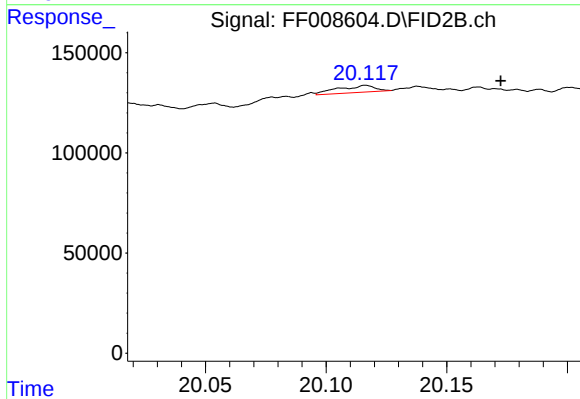

#16 N-HEXATRIACONTANE

R.T.: 20.116 min
Delta R.T.: -0.056 min
Response: 37084
Conc: 0.33 ug/ml