

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
 Data File : FF008605.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jun 2021 13:25
 Operator : DD\AJ
 Sample : M2639-03 10X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 14 07:21:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	143824	1.365 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.969	424531	3.464 ug/ml
12) N-OCTACOSANE	16.972	89031	0.751 ug/ml
16) N-HEXATRIACONTANE	20.163	110610	0.998 ug/ml
18) N-TETRACONTANE	21.859	535365	5.068 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
Data File : FF008605.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2021 13:25
Operator : DD\AJ
Sample : M2639-03 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 07:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

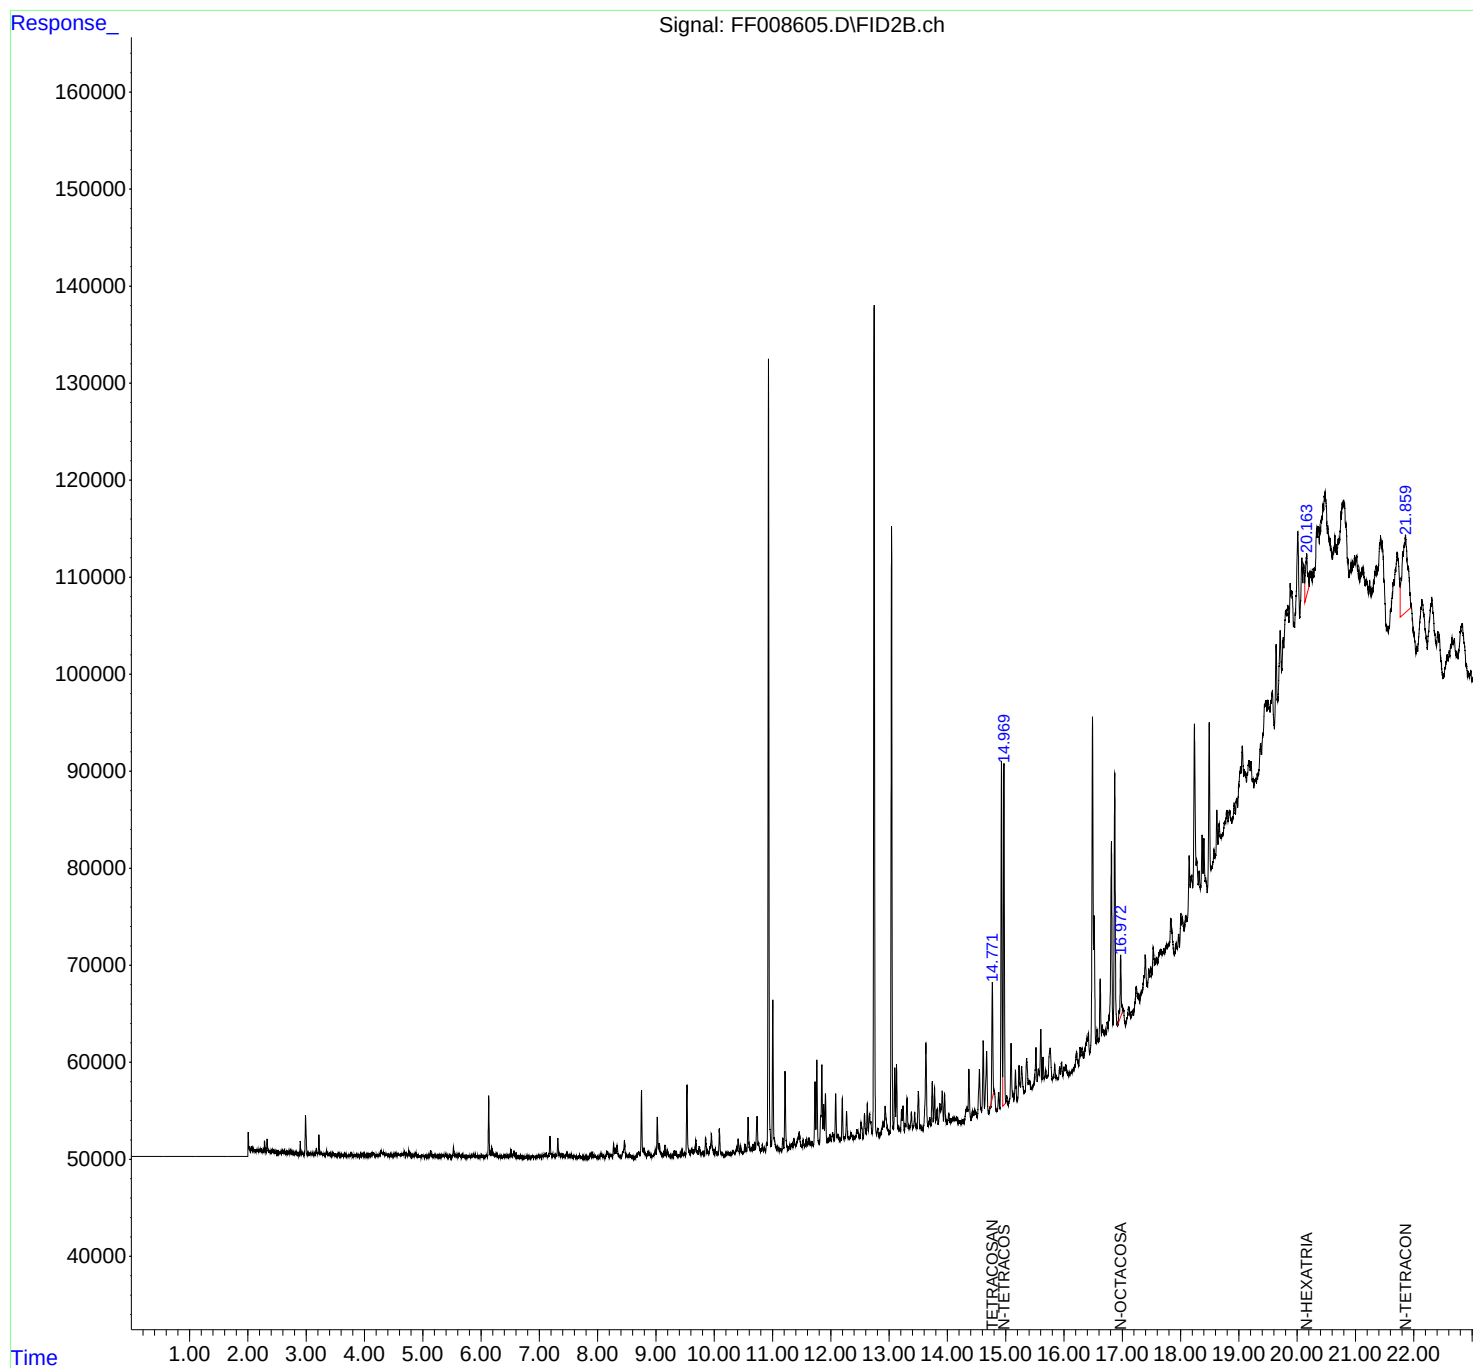


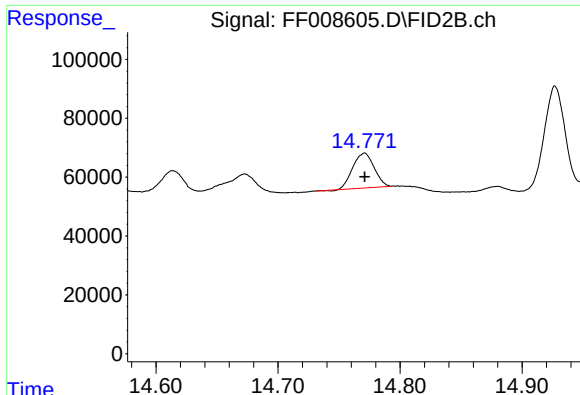

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.771 min
Delta R.T.: 0.000 min
Response: 143824
Conc: 1.36 ug/ml

Instrument :
FID_F
ClientSampleId :

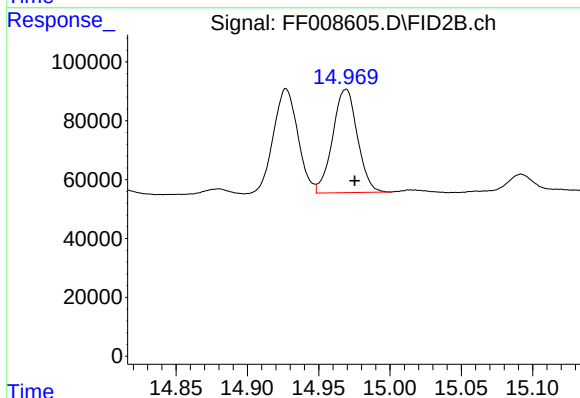


#10 N-TETRACOSANE

R.T.: 14.969 min
Delta R.T.: -0.006 min
Response: 424531
Conc: 3.46 ug/ml

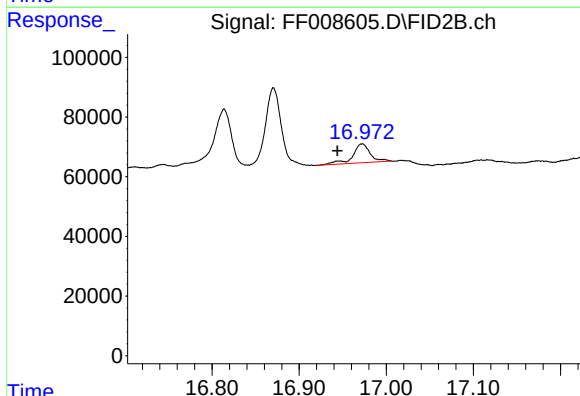


#12 N-OCTACOSANE

R.T.: 16.972 min
Delta R.T.: 0.029 min
Response: 89031
Conc: 0.75 ug/ml

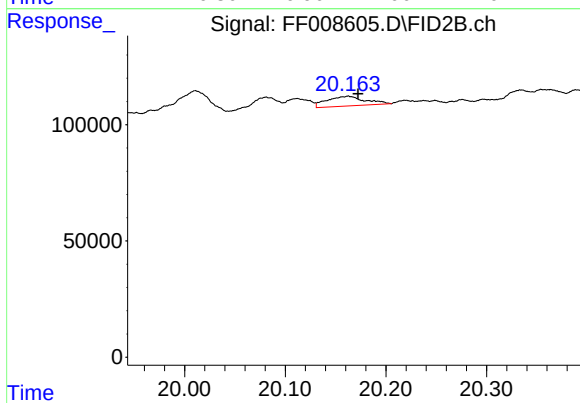

#16 N-HEXATRIACONTANE

R.T.: 20.163 min
Delta R.T.: -0.010 min
Response: 110610
Conc: 1.00 ug/ml

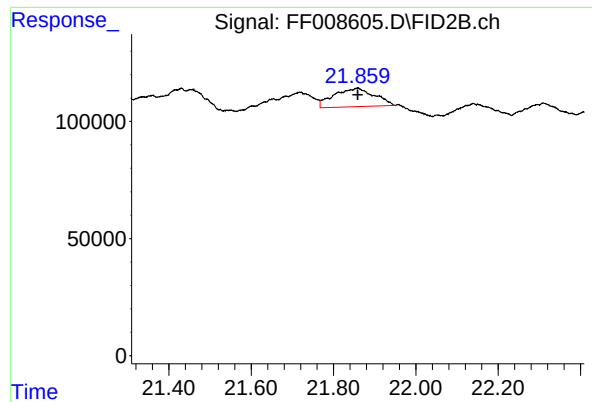

#18 N-TETRACONTANE

R.T.: 21.859 min
Delta R.T.: 0.000 min
Response: 535365
Conc: 5.07 ug/ml

Instrument :
FID_F
ClientSampleId :