

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
Data File : FF008605.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2021 13:25
Operator : DD\AJ
Sample : M2639-03 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
B67

Manual Integrations
APPROVED

Ankita
6/14/2021 2:16:17 PM

Integration File: autoint1.e
Quant Time: Jun 14 07:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	175831	1.669 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061321\
Data File : FF008605.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2021 13:25
Operator : DD\AJ
Sample : M2639-03 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
B67


Manual Integrations
APPROVED

Ankita
6/14/2021 2:16:17 PM

Integration File: autoint1.e
Quant Time: Jun 14 07:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

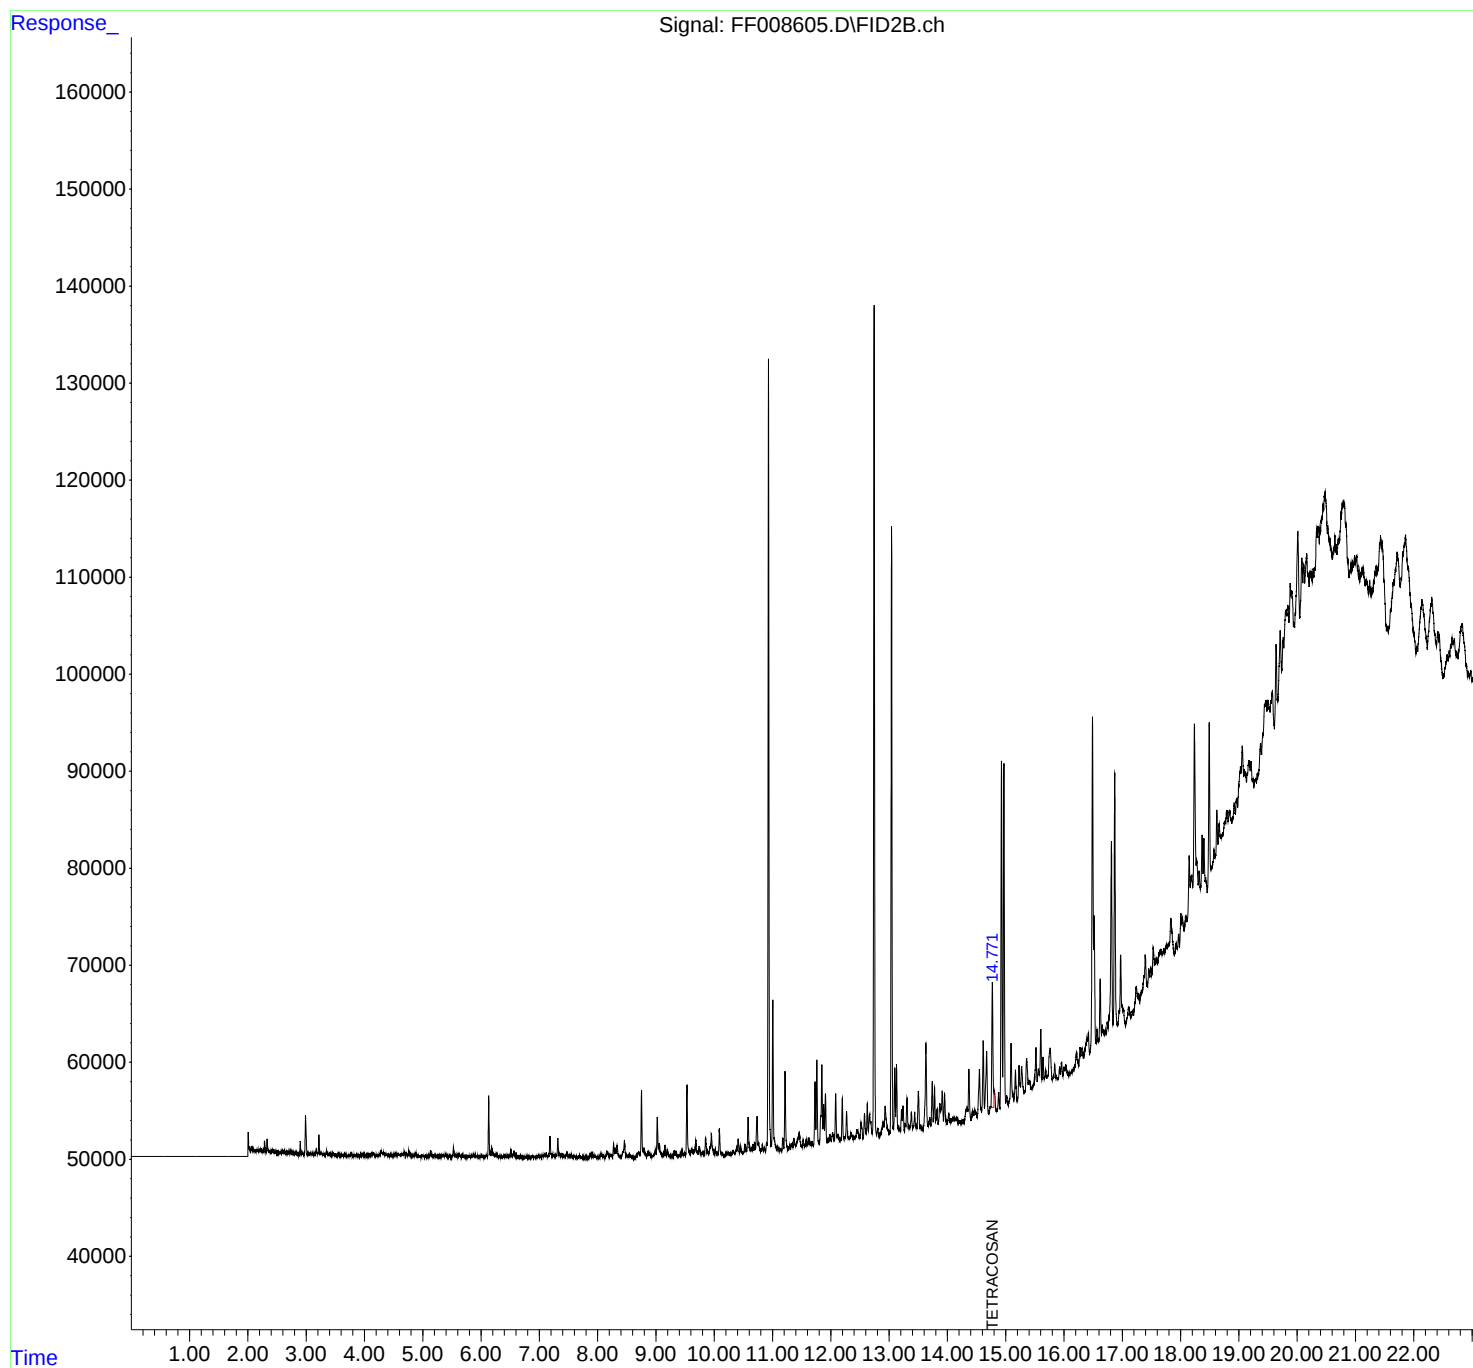

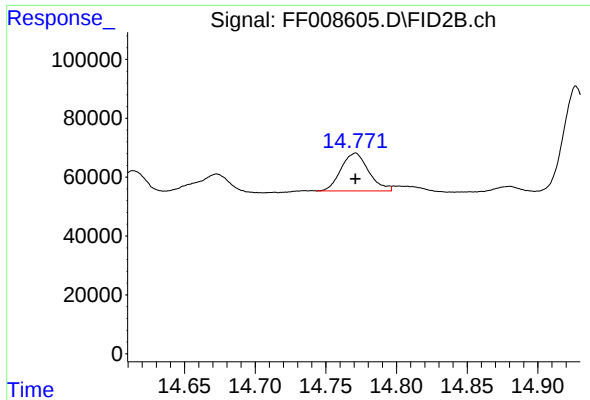

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.771 min
Delta R.T.: 0.000 min
Response: 175831
Conc: 1.67 ug/ml m

Instrument :
FID_F
ClientSampleId :
B67

Manual Integrations
APPROVED

Ankita
6/14/2021 2:16:17 PM