

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010758.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 10:54
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 05:19:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.554	1993141	16.401 ug/ml
12)	N-OCTACOSANE	16.991	1938911	15.888 ug/ml
13)	N-TRIACONTANE	17.875	156908	1.280 ug/ml
14)	N-DOTRIACONTANE	18.706	210638	1.736 ug/ml
15)	N-TETRATRIACONTANE	19.486	159306	1.533 ug/ml
16)	N-HEXATRIACONTANE	20.224	91245	1.061 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010758.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 10:54
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 05:19:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

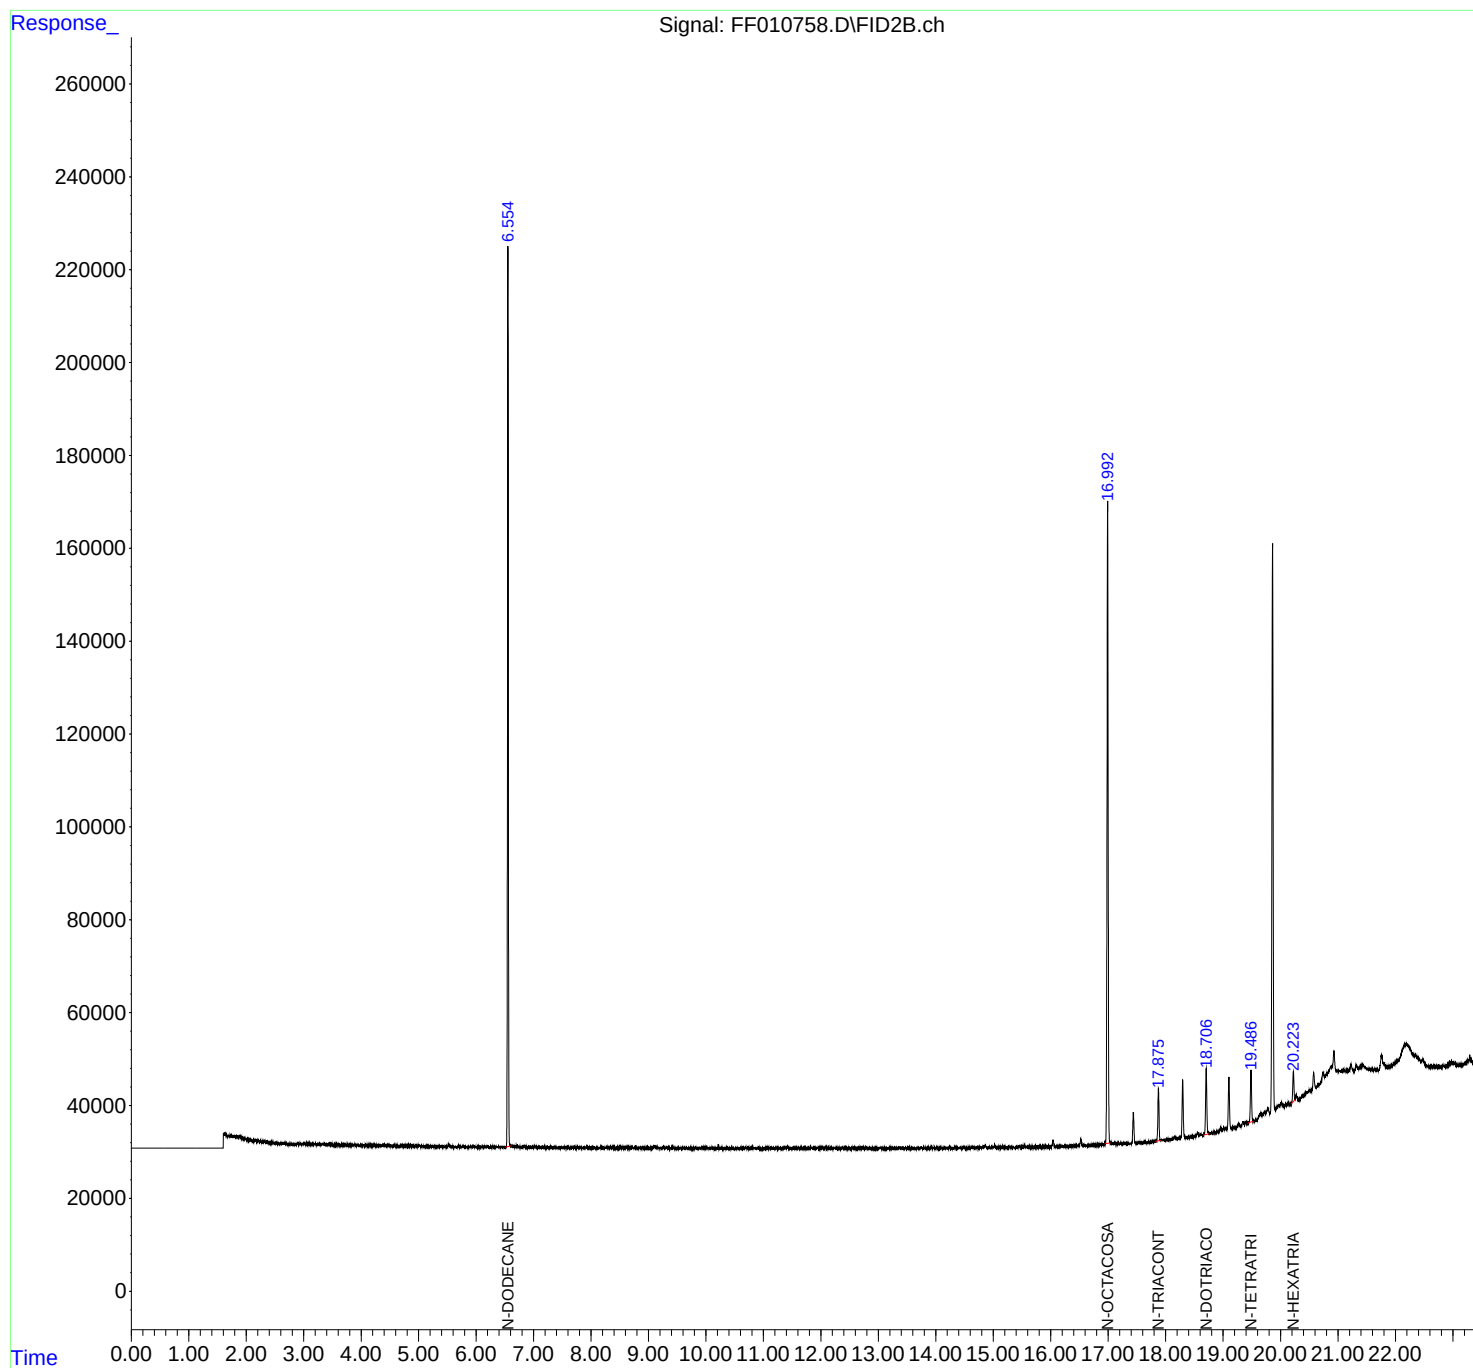


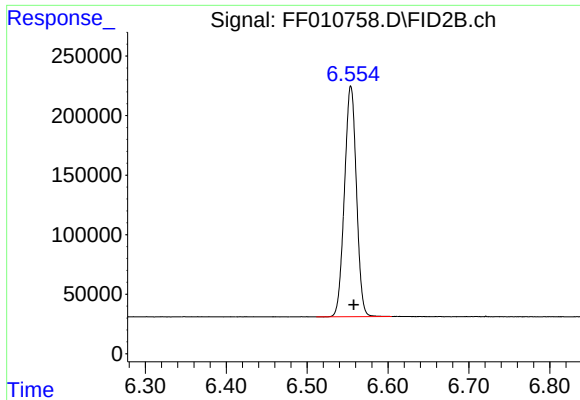

#3 N-DODECANE


R.T.: 6.554 min
Delta R.T.: -0.004 min
Response: 1993141
Conc: 16.40 ug/ml

Instrument :
FID_F
ClientSampleId :

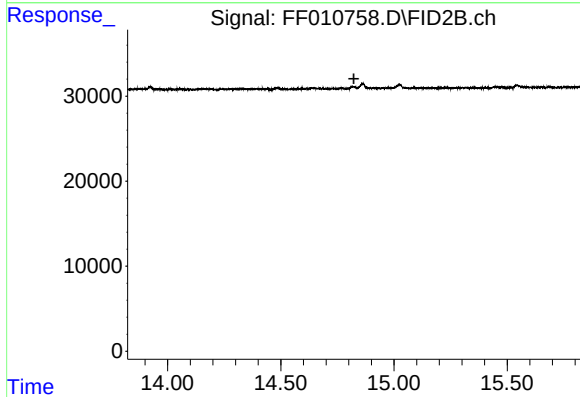


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

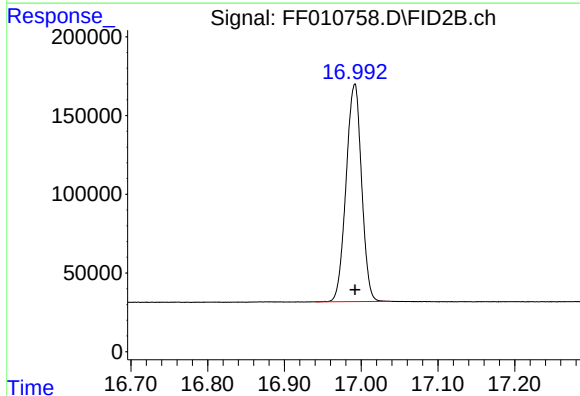


#12 N-OCTACOSANE

R.T.: 16.991 min
Delta R.T.: 0.000 min
Response: 1938911
Conc: 15.89 ug/ml

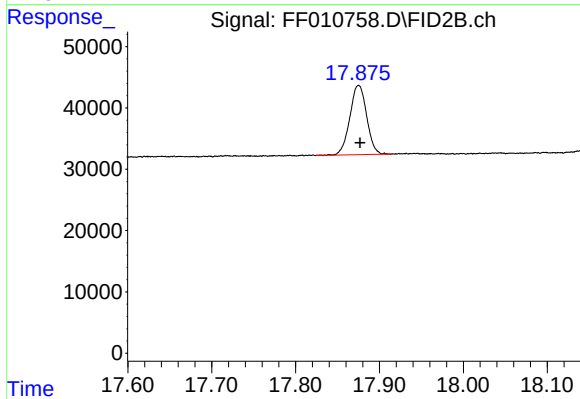

#13 N-TRIACONTANE


R.T.: 17.875 min
Delta R.T.: -0.002 min
Response: 156908
Conc: 1.28 ug/ml

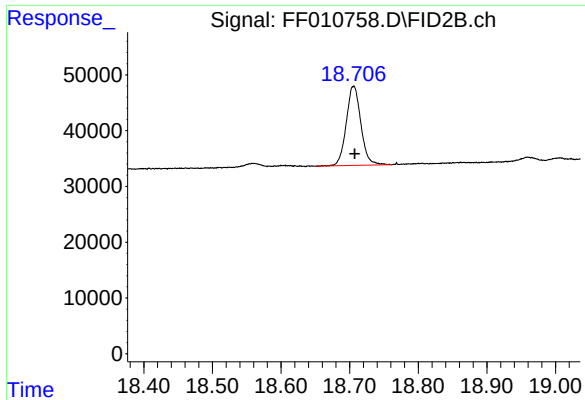

#14 N-DOTRIACONTANE


R.T.: 18.706 min
Delta R.T.: -0.002 min
Response: 210638
Conc: 1.74 ug/ml

Instrument :
FID_F
ClientSampleId :

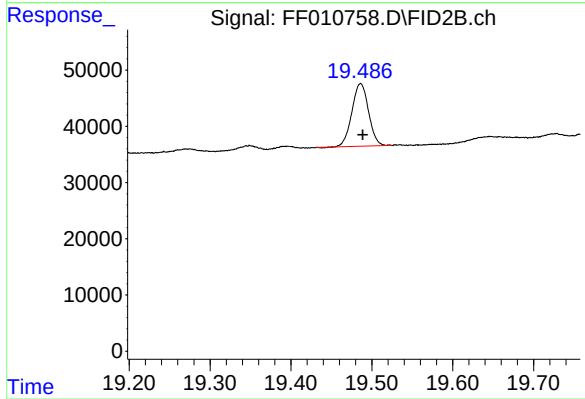

#15 N-TETRATRIACONTANE

R.T.: 19.486 min
Delta R.T.: -0.002 min
Response: 159306
Conc: 1.53 ug/ml

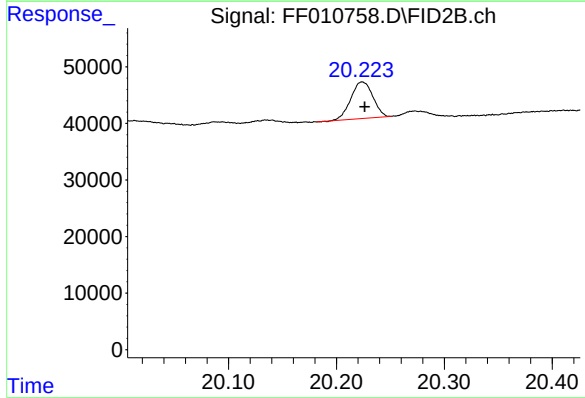

#16 N-HEXATRIACONTANE

R.T.: 20.224 min
Delta R.T.: -0.002 min
Response: 91245
Conc: 1.06 ug/ml