

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010760.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 12:08
Operator : AJ\MA
Sample : PB143242BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 05:20:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.821	3580077	31.672 ug/ml
Target Compounds				
18)	N-TETRACONTANE	21.802	192850	2.468 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010760.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 12:08
Operator : AJ\MA
Sample : PB143242BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 05:20:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

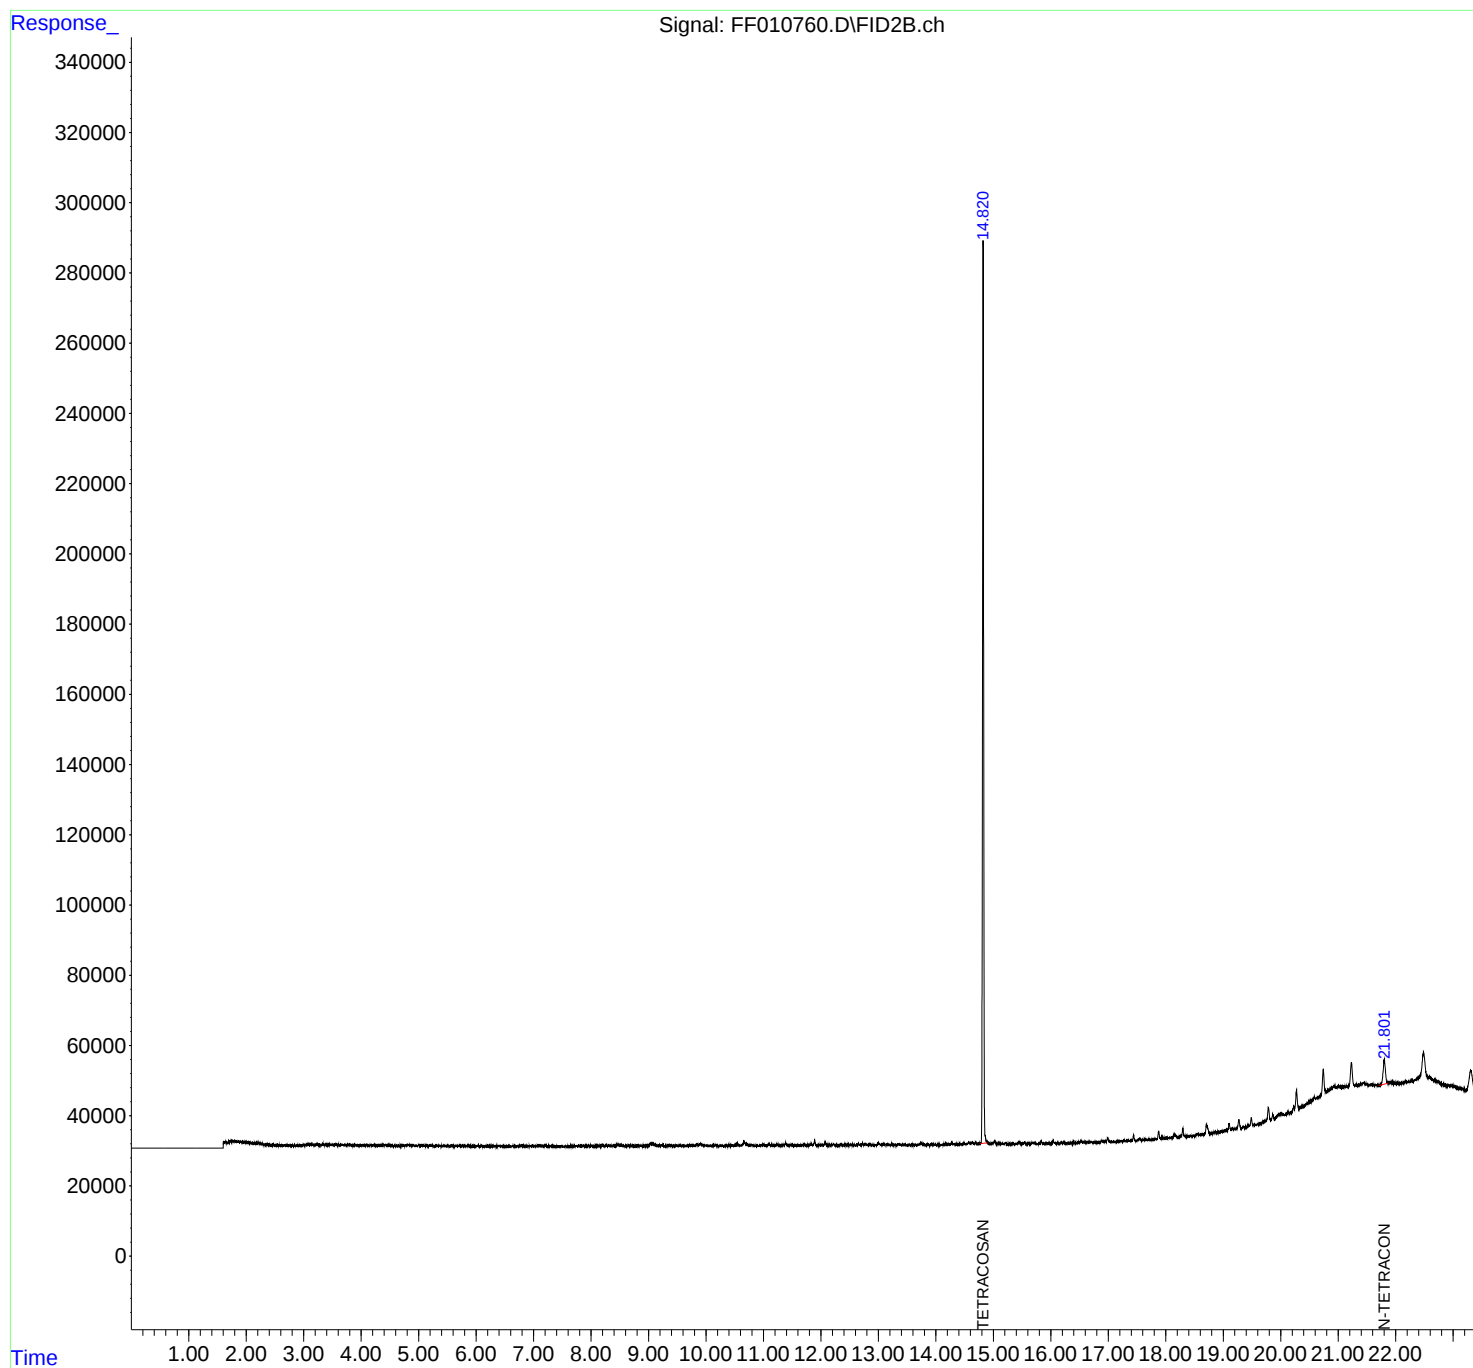


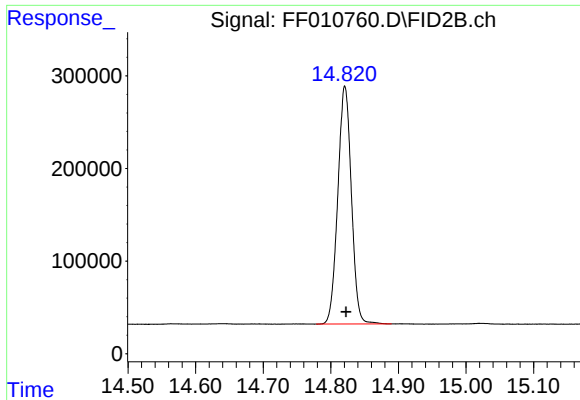

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.821 min
Delta R.T.: -0.002 min
Response: 3580077
Conc: 31.67 ug/ml

Instrument :
FID_F
ClientSampleId :

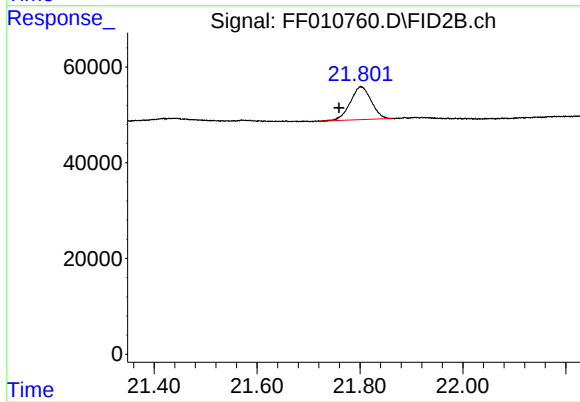

#18 N-TETRACONTANE

R.T.: 21.802 min
Delta R.T.: 0.043 min
Response: 192850
Conc: 2.47 ug/ml