

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010759.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 11:23
Operator : AJ\MA
Sample : PB143273BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB143273BL

Integration File: autoint1.e
Quant Time: Jun 14 05:20:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.821	1935132	17.120 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010759.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 11:23
Operator : AJ\MA
Sample : PB143273BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB143273BL

Integration File: autoint1.e
Quant Time: Jun 14 05:20:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

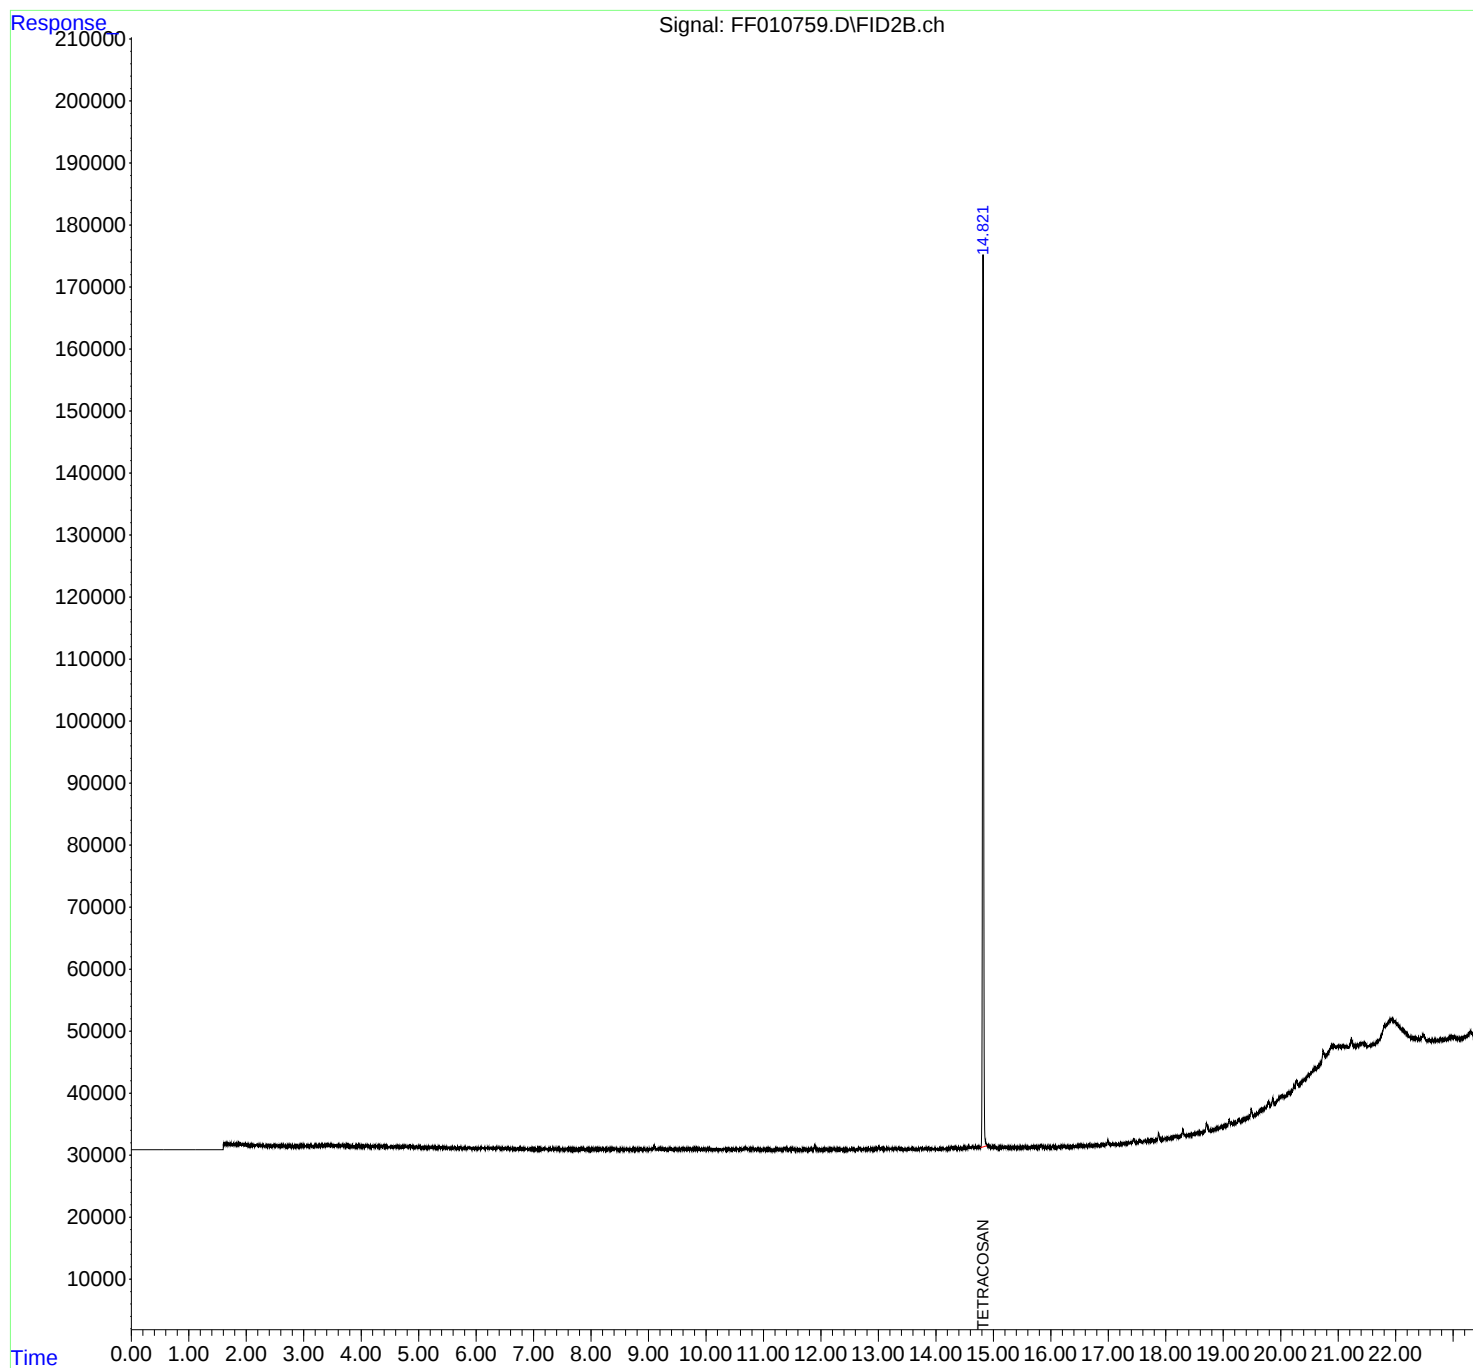

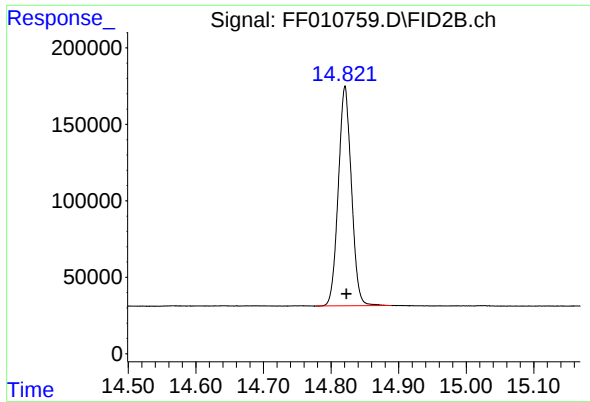

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.821 min
Delta R.T.: -0.002 min
Response: 1935132
Conc: 17.12 ug/ml

Instrument :
FID_F
ClientSampleId :
PB143273BL