

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
 Data File : FF010767.D
 Signal(s) : FID2B.ch
 Acq On : 13 Jun 2022 16:30
 Operator : AJ\MA
 Sample : PB145479BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB145479BS

Integration File: autoint1.e
 Quant Time: Jun 14 05:24:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.820	2329699	20.610 ug/ml
Target Compounds			
2) N-DECANE	4.386	2635764	22.048 ug/ml
3) N-DODECANE	6.552	2735632	22.510 ug/ml
4) N-TETRADECANE	8.375	2814658	22.703 ug/ml
5) N-HEXADECANE	9.978	2840872	22.720 ug/ml
6) N-OCTADECANE	11.418	2917212	22.798 ug/ml
7) N-EICOSANE	12.726	2894865	22.891 ug/ml
8) N-DOCOSANE	13.922	2853032	22.590 ug/ml
10) N-TETRACOSANE	15.023	2844172	22.691 ug/ml
11) N-HEXACOSANE	16.042	2794407	22.061 ug/ml
12) N-OCTACOSANE	16.990	2730424	22.373 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061322\
Data File : FF010767.D
Signal(s) : FID2B.ch
Acq On : 13 Jun 2022 16:30
Operator : AJ\MA
Sample : PB145479BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB145479BS

Integration File: autoint1.e
Quant Time: Jun 14 05:24:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

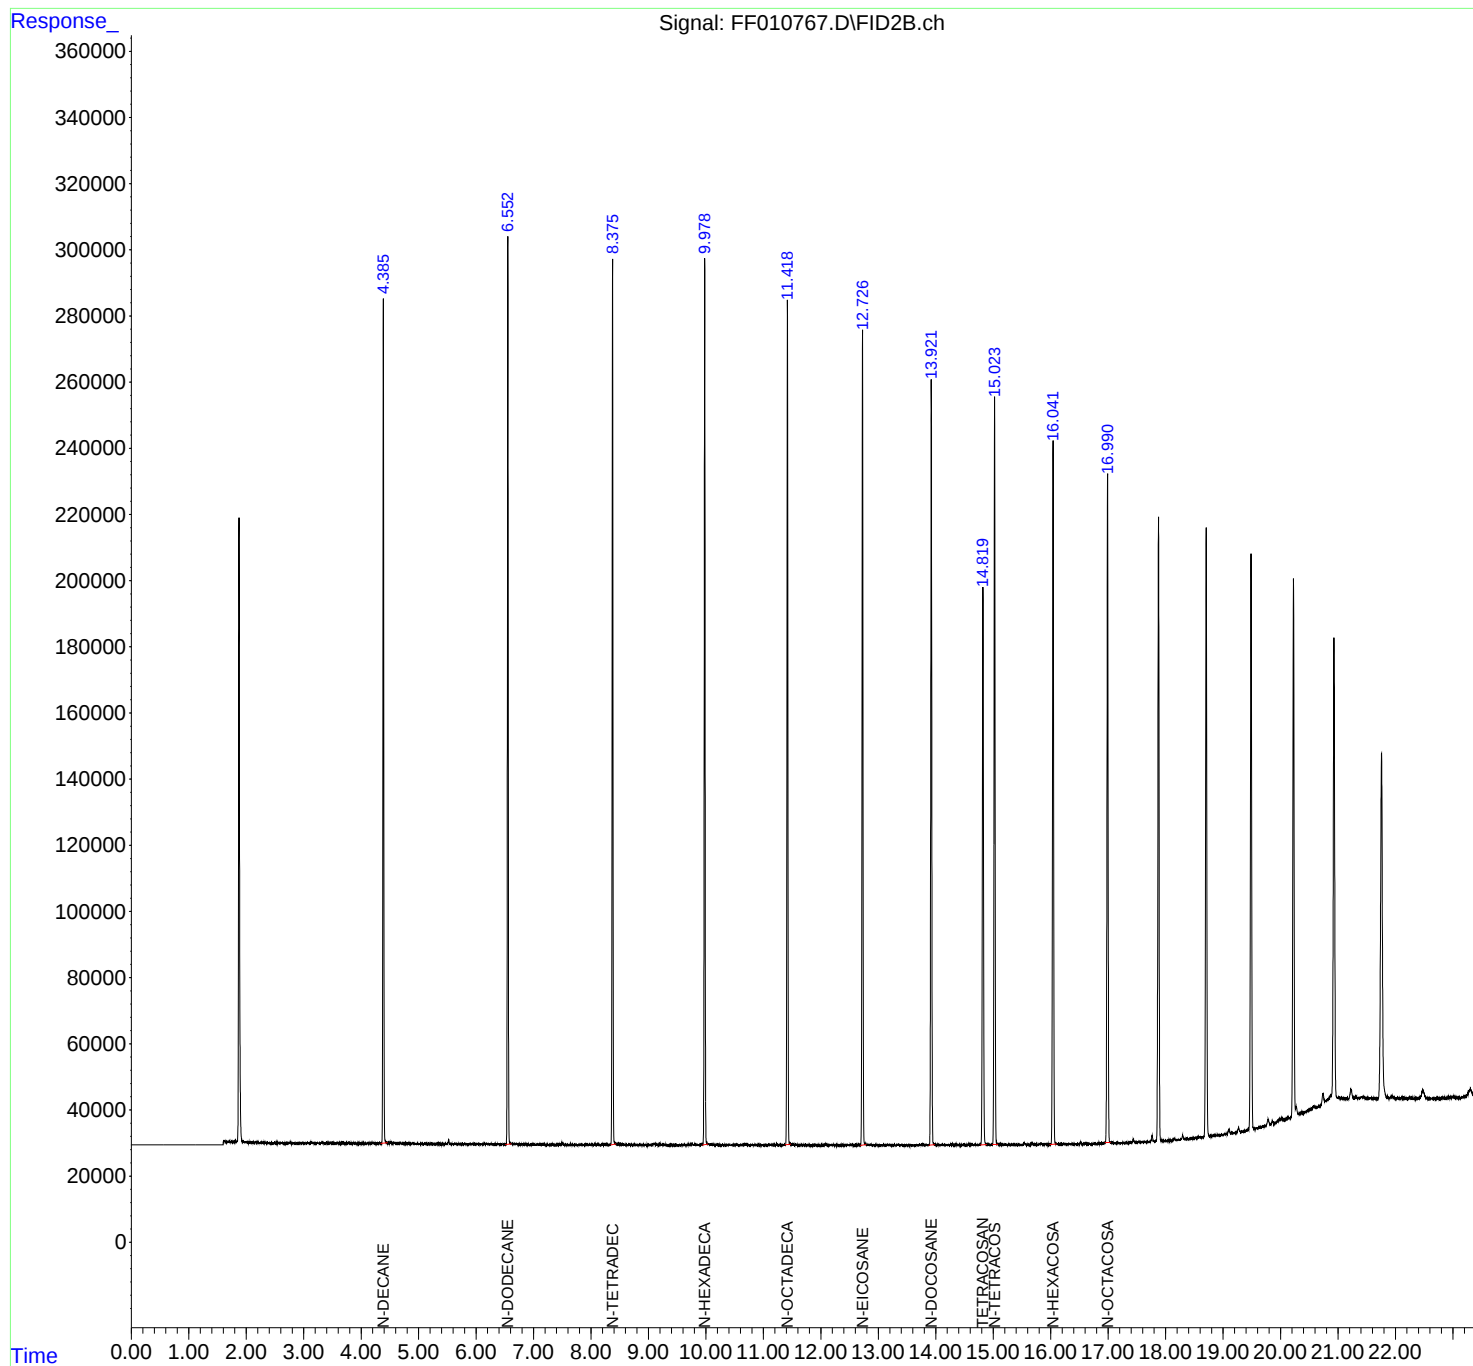


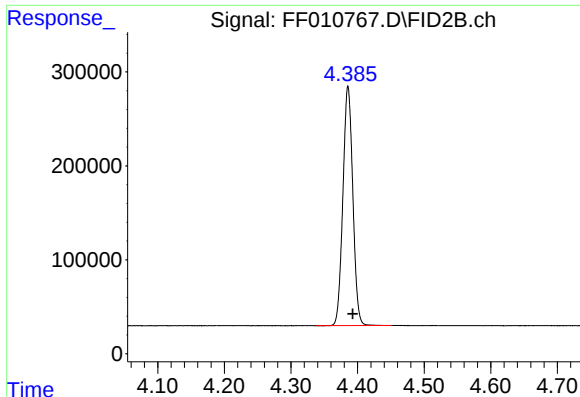

#2 N-DECANE


R.T.: 4.386 min
Delta R.T.: -0.007 min
Response: 2635764
Conc: 22.05 ug/ml

Instrument :
FID_F
ClientSampleId :
PB145479BS

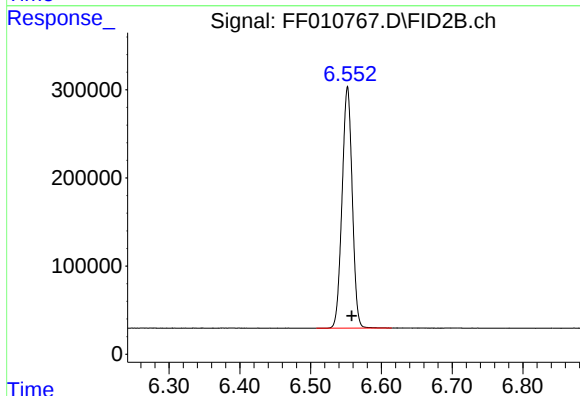


#3 N-DODECANE

R.T.: 6.552 min
Delta R.T.: -0.006 min
Response: 2735632
Conc: 22.51 ug/ml

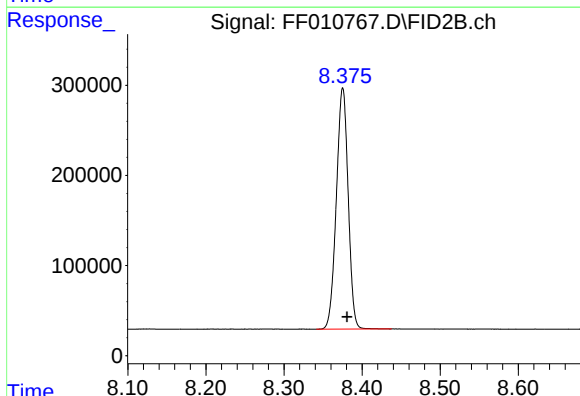


#4 N-TETRADECANE

R.T.: 8.375 min
Delta R.T.: -0.006 min
Response: 2814658
Conc: 22.70 ug/ml

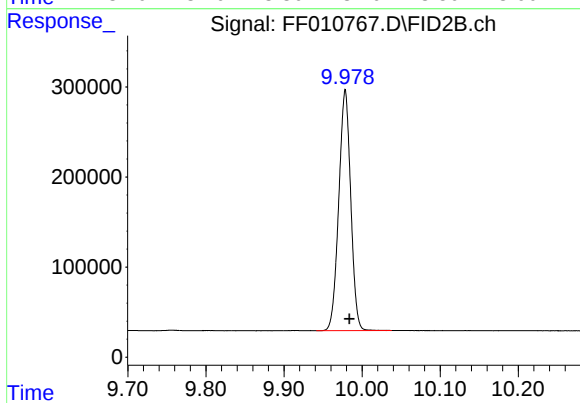

#5 N-HEXADECANE


R.T.: 9.978 min
Delta R.T.: -0.005 min
Response: 2840872
Conc: 22.72 ug/ml

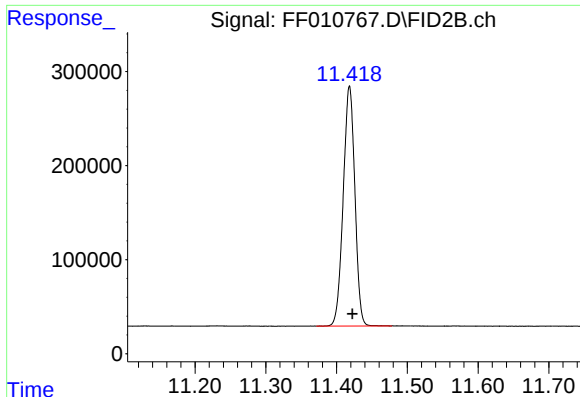

#6 N-OCTADECANE


R.T.: 11.418 min
Delta R.T.: -0.004 min
Response: 2917212
Conc: 22.80 ug/ml

Instrument :
FID_F
ClientSampleId :
PB145479BS

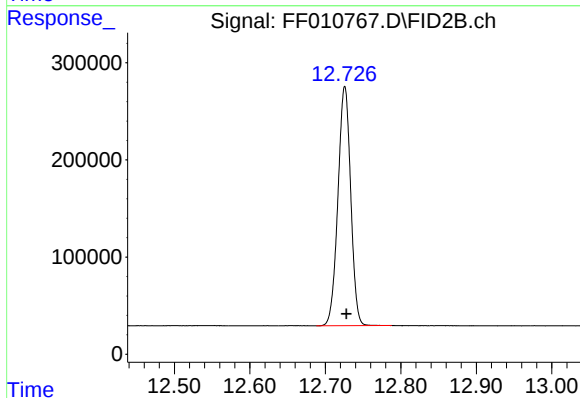


#7 N-EICOSANE

R.T.: 12.726 min
Delta R.T.: -0.002 min
Response: 2894865
Conc: 22.89 ug/ml

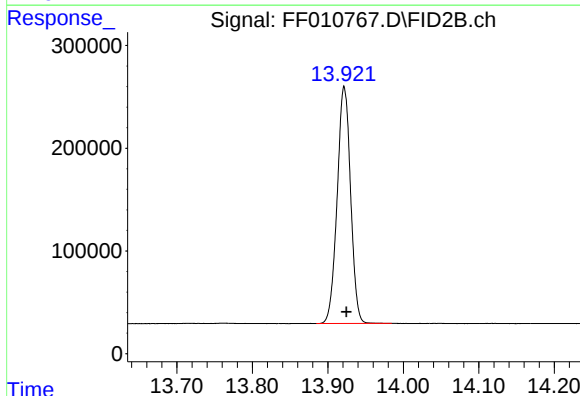


#8 N-DOCOSANE

R.T.: 13.922 min
Delta R.T.: -0.003 min
Response: 2853032
Conc: 22.59 ug/ml

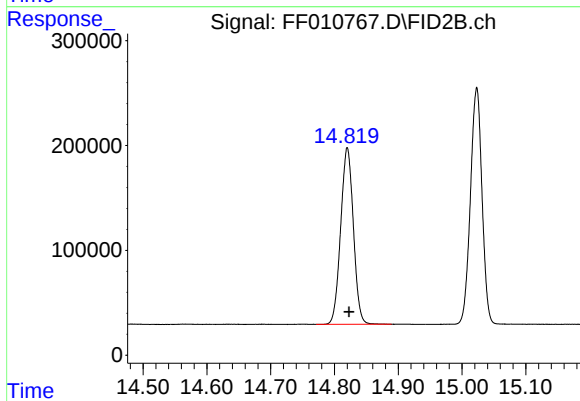

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.820 min
Delta R.T.: -0.003 min
Response: 2329699
Conc: 20.61 ug/ml

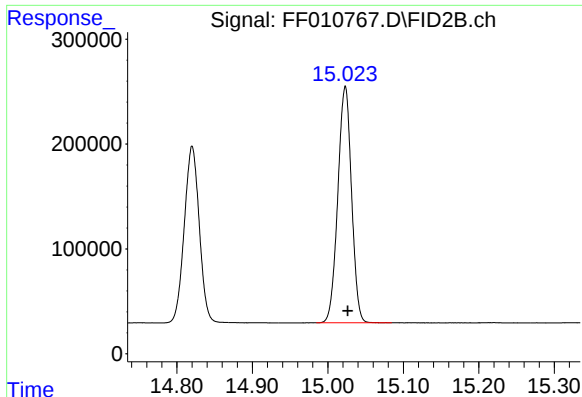

#10 N-TETRACOSANE


R.T.: 15.023 min
Delta R.T.: -0.003 min
Response: 2844172
Conc: 22.69 ug/ml

Instrument :
FID_F
ClientSampleId :
PB145479BS

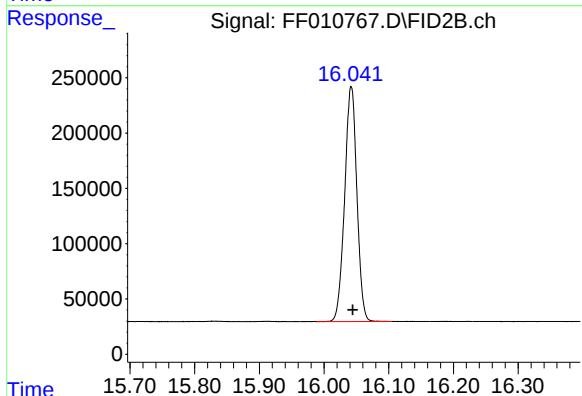

#11 N-HEXACOSANE

R.T.: 16.042 min
Delta R.T.: -0.002 min
Response: 2794407
Conc: 22.06 ug/ml

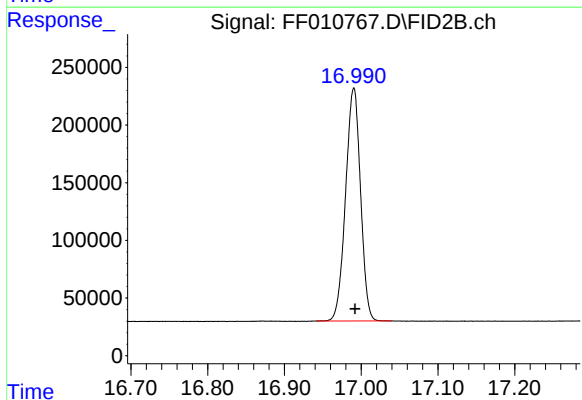

#12 N-OCTACOSANE

R.T.: 16.990 min
Delta R.T.: -0.002 min
Response: 2730424
Conc: 22.37 ug/ml