

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061421\
 Data File : FF008618.D
 Signal(s) : FID2B.ch
 Acq On : 14 Jun 2021 15:13
 Operator : DD\AJ
 Sample : M2674-03 100X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 01:43:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.573	134441	1.108 ug/ml
3) N-DODECANE	6.473f	159237	1.276 ug/ml
4) N-TETRADECANE	8.329	134866	1.060 ug/ml
5) N-HEXADECANE	9.916	213688	1.690 ug/ml
6) N-OCTADECANE	11.359	118952	0.938 ug/ml
7) N-EICOSANE	12.665	72820	0.570 ug/ml
8) N-DOCOSANE	13.864	138157	1.099 ug/ml
10) N-TETRACOSANE	14.972	128029	1.045 ug/ml
11) N-HEXACOSANE	15.962	80697	0.673 ug/ml
13) N-TRIACONTANE	17.834	130533	1.102 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061421\
Data File : FF008618.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2021 15:13
Operator : DD\AJ
Sample : M2674-03 100X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 01:43:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

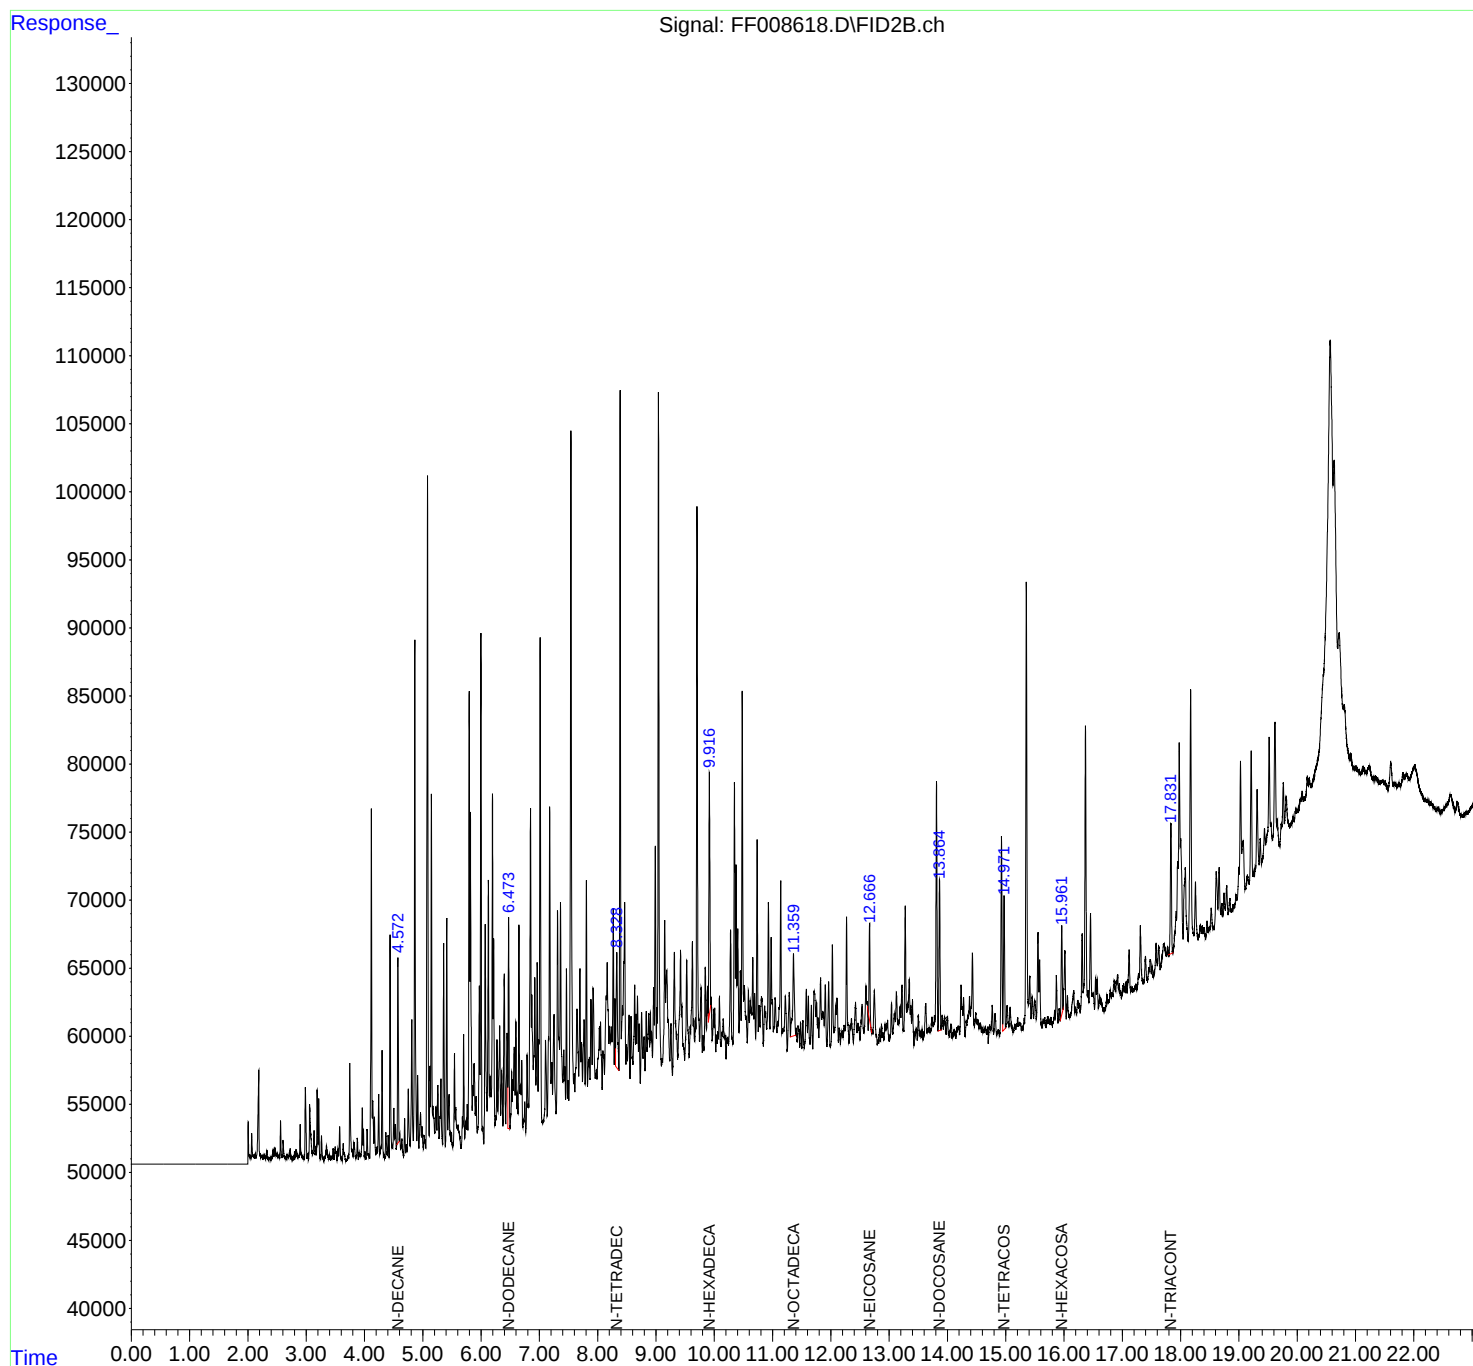


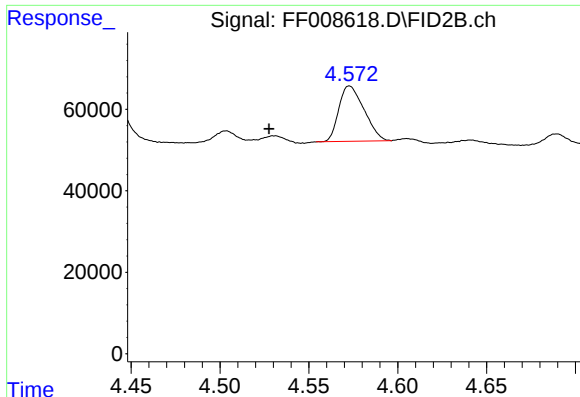

#2 N-DECANE


R.T.: 4.573 min
Delta R.T.: 0.045 min
Response: 134441
Conc: 1.11 ug/ml

Instrument :
FID_F
ClientSampleId :

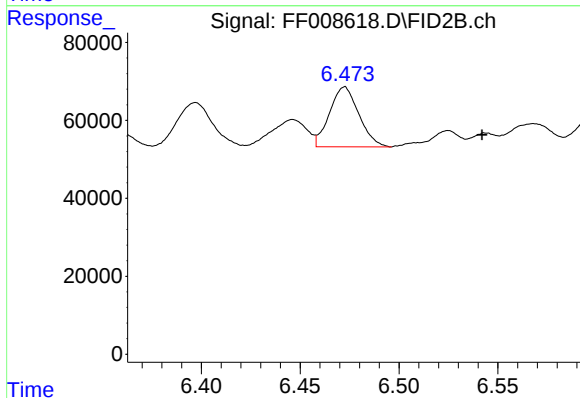


#3 N-DODECANE

R.T.: 6.473 min
Delta R.T.: -0.069 min
Response: 159237
Conc: 1.28 ug/ml

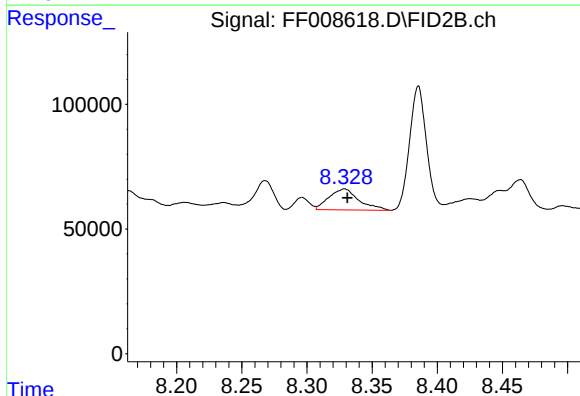


#4 N-TETRADECANE

R.T.: 8.329 min
Delta R.T.: -0.002 min
Response: 134866
Conc: 1.06 ug/ml

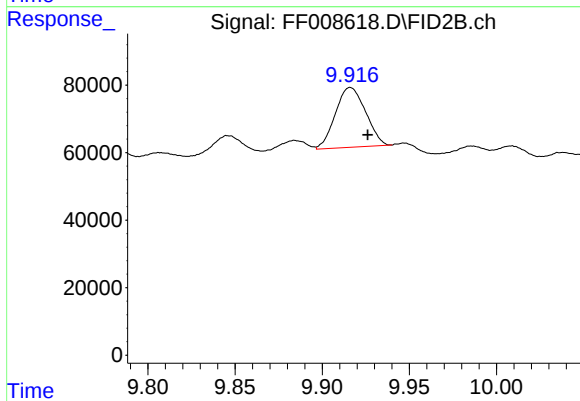

#5 N-HEXADECANE


R.T.: 9.916 min
Delta R.T.: -0.010 min
Response: 213688
Conc: 1.69 ug/ml

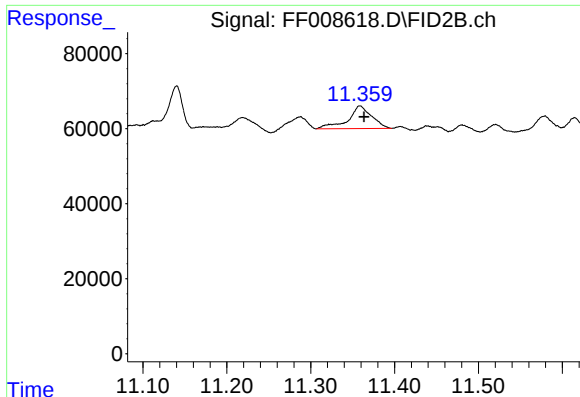

#6 N-OCTADECANE


R.T.: 11.359 min
Delta R.T.: -0.005 min
Response: 118952
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

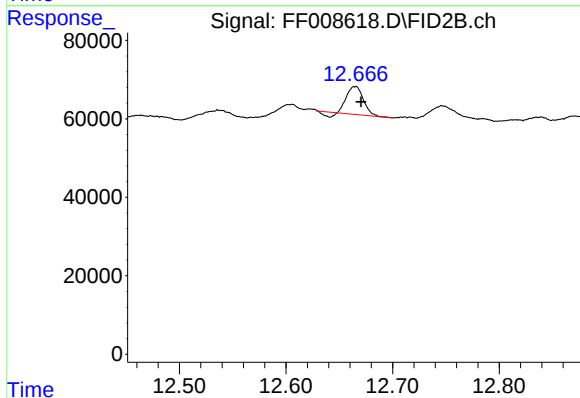


#7 N-EICOSANE

R.T.: 12.665 min
Delta R.T.: -0.005 min
Response: 72820
Conc: 0.57 ug/ml

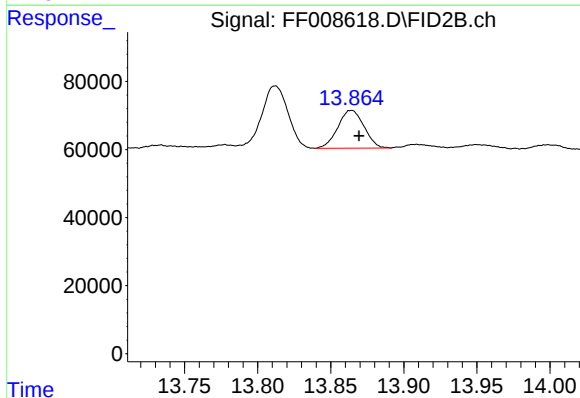


#8 N-DOCOSANE

R.T.: 13.864 min
Delta R.T.: -0.005 min
Response: 138157
Conc: 1.10 ug/ml

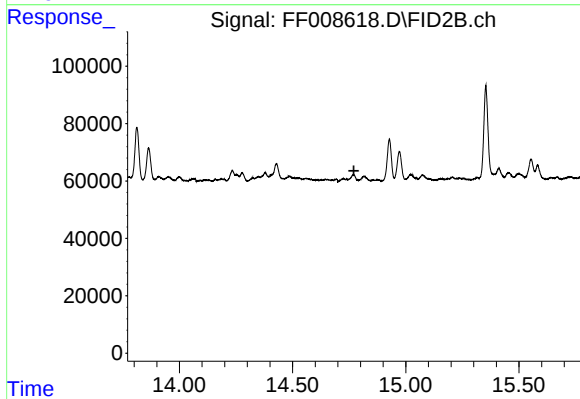

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.771 min
Response: 0
Conc: N.D.

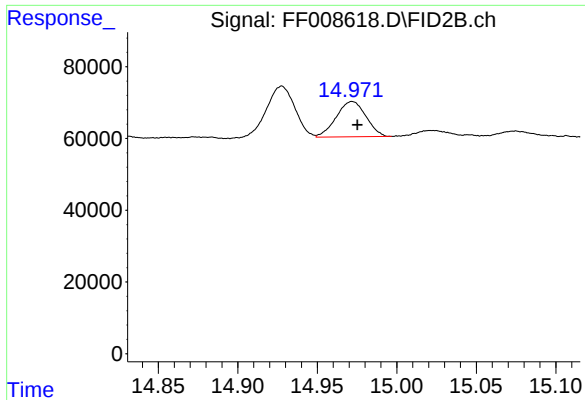

#10 N-TETRACOSANE


R.T.: 14.972 min
Delta R.T.: -0.003 min
Response: 128029
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :

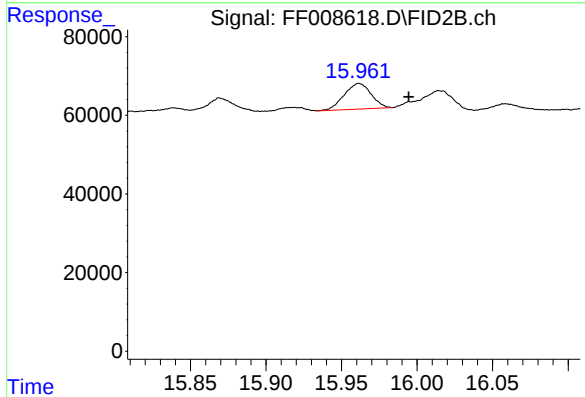

#11 N-HEXACOSANE

R.T.: 15.962 min
Delta R.T.: -0.033 min
Response: 80697
Conc: 0.67 ug/ml

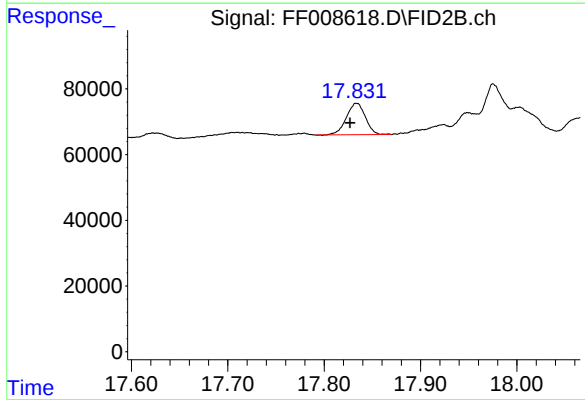

#13 N-TRIACONTANE

R.T.: 17.834 min
Delta R.T.: 0.007 min
Response: 130533
Conc: 1.10 ug/ml