

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061421\
 Data File : FF008614.D
 Signal(s) : FID2B.ch
 Acq On : 14 Jun 2021 12:45
 Operator : DD\AJ
 Sample : M2674-01 10X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Manual Integrations
 APPROVED

Ankita
 6/15/2021 2:37:46 PM

Integration File: autoint1.e
 Quant Time: Jun 15 01:42:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.774	706139	6.702 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061421\
Data File : FF008614.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2021 12:45
Operator : DD\AJ
Sample : M2674-01 10X
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :


Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:46 PM

Integration File: autoint1.e
Quant Time: Jun 15 01:42:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

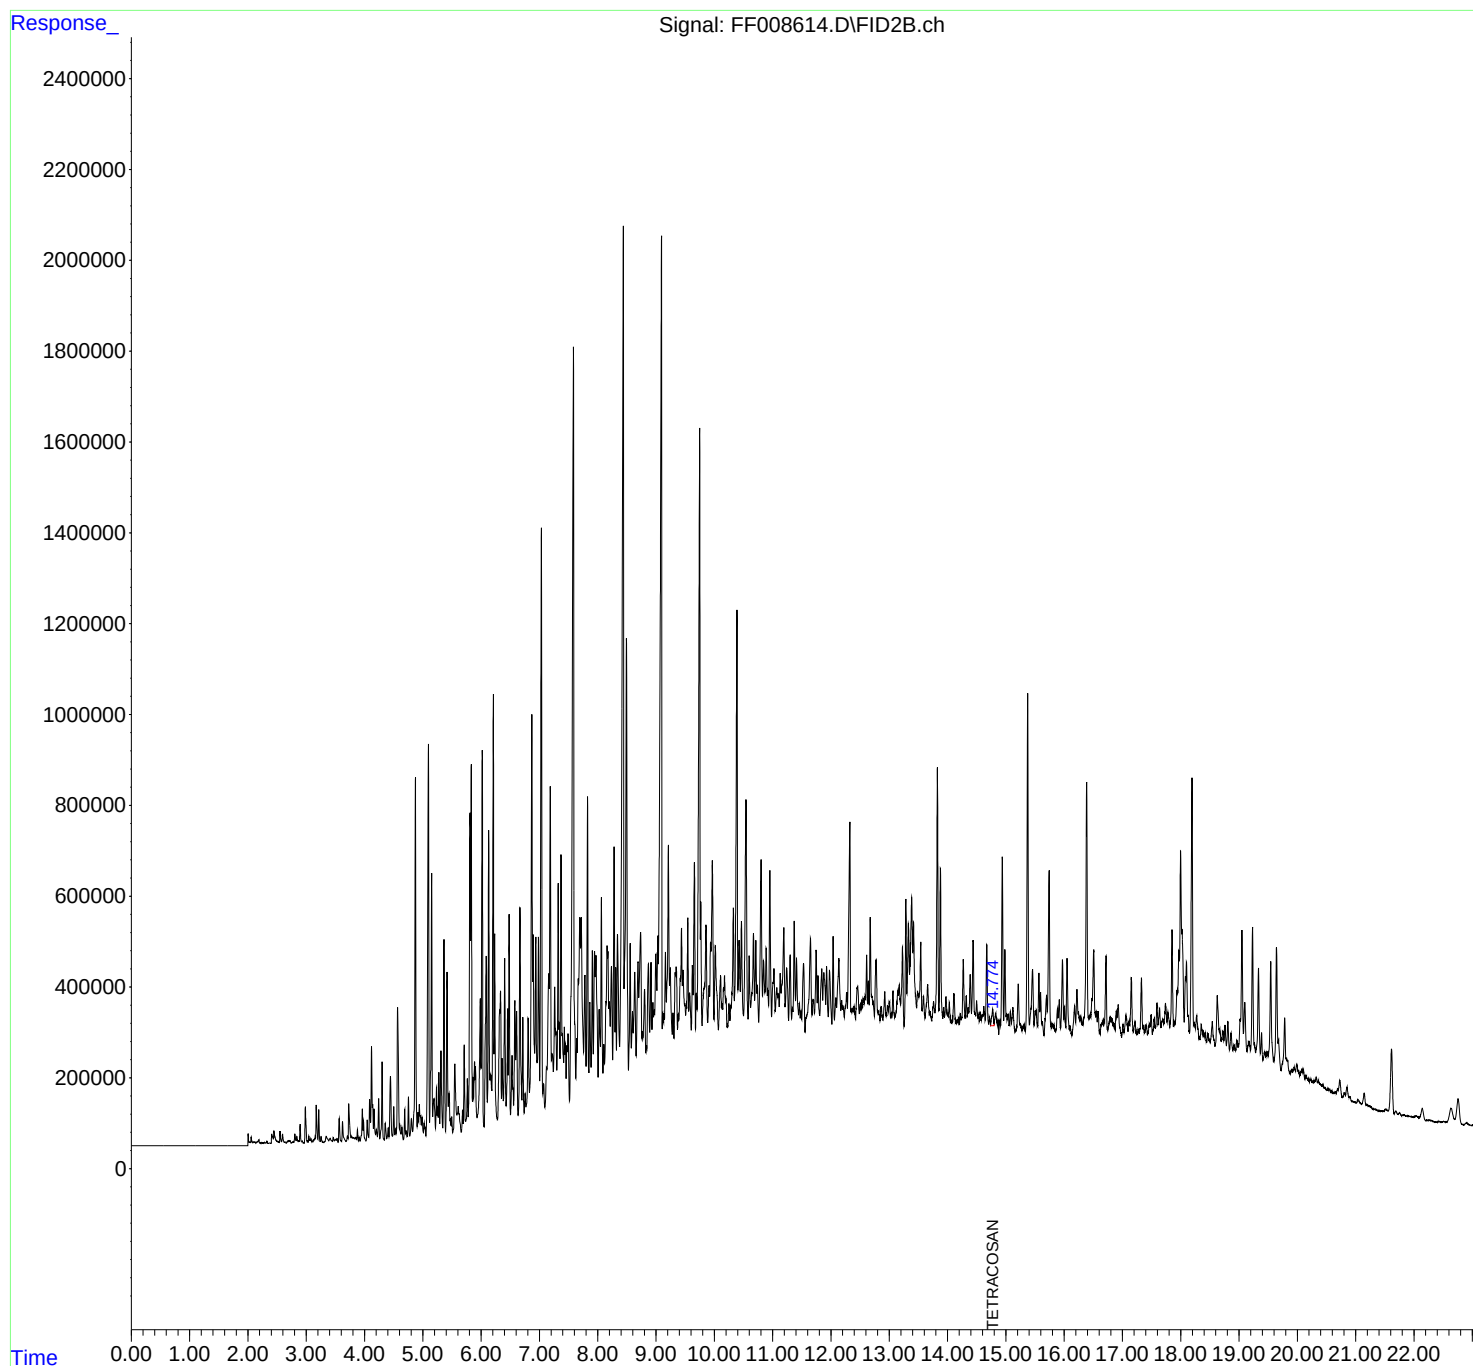

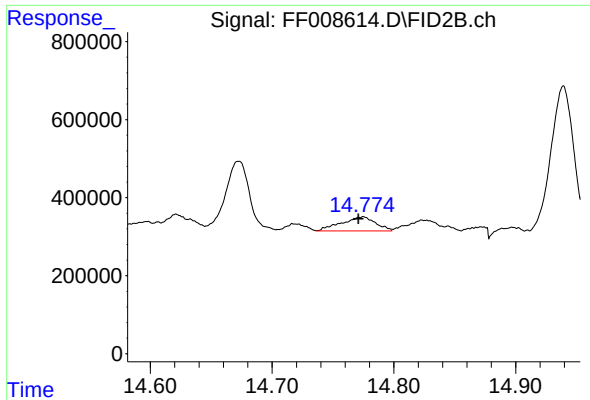

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.774 min
Delta R.T.: 0.003 min
Response: 706139
Conc: 6.70 ug/ml m

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:46 PM