

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061421\
Data File : FF008616.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2021 13:48
Operator : DD\AJ
Sample : M2674-04 20X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TMR-DS-04-060921

Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:50 PM

Integration File: autoint1.e
Quant Time: Jun 15 08:47:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.766	116301	1.104 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061421\
Data File : FF008616.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2021 13:48
Operator : DD\AJ
Sample : M2674-04 20X
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
TMR-DS-04-060921


Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:50 PM

Integration File: autoint1.e
Quant Time: Jun 15 08:47:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

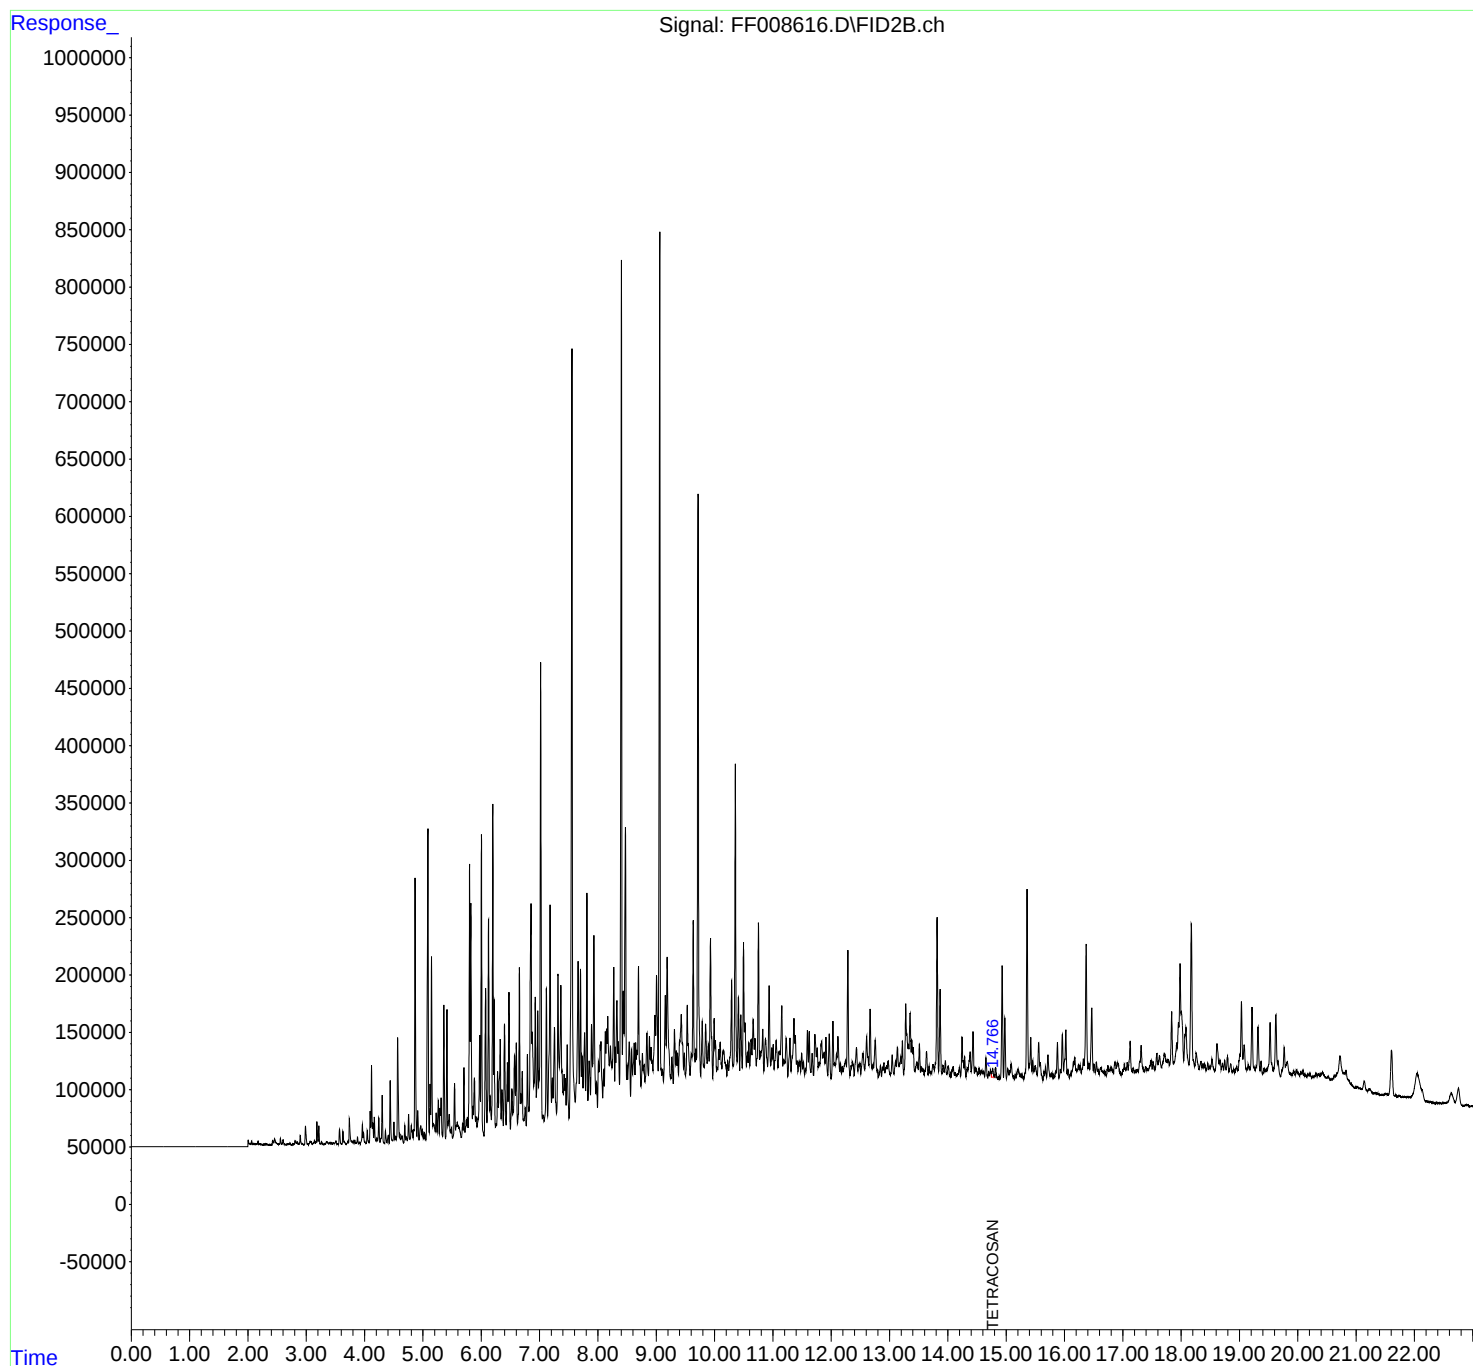

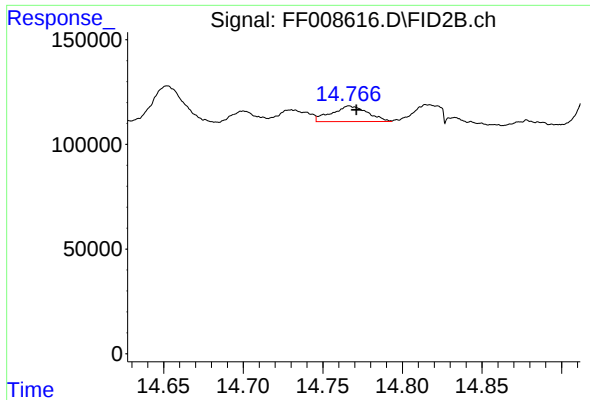

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.766 min
Delta R.T.: -0.005 min
Response: 116301
Conc: 1.10 ug/ml m

Instrument :
FID_F
ClientSampleId :
TMR-DS-04-060921

Manual Integrations
APPROVED

Ankita
6/15/2021 2:37:50 PM