

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061422\
 Data File : FF010780.D
 Signal(s) : FID2B.ch
 Acq On : 14 Jun 2022 09:06
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 01:34:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.824	2795055	24.727 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.879	183579	1.498 ug/ml
14) N-DOTRIACONTANE	18.710	277947	2.291 ug/ml
15) N-TETRATRIACONTANE	19.492	175077	1.685 ug/ml
16) N-HEXATRIACONTANE	20.231	146358	1.702 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061422\
Data File : FF010780.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2022 09:06
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 01:34:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

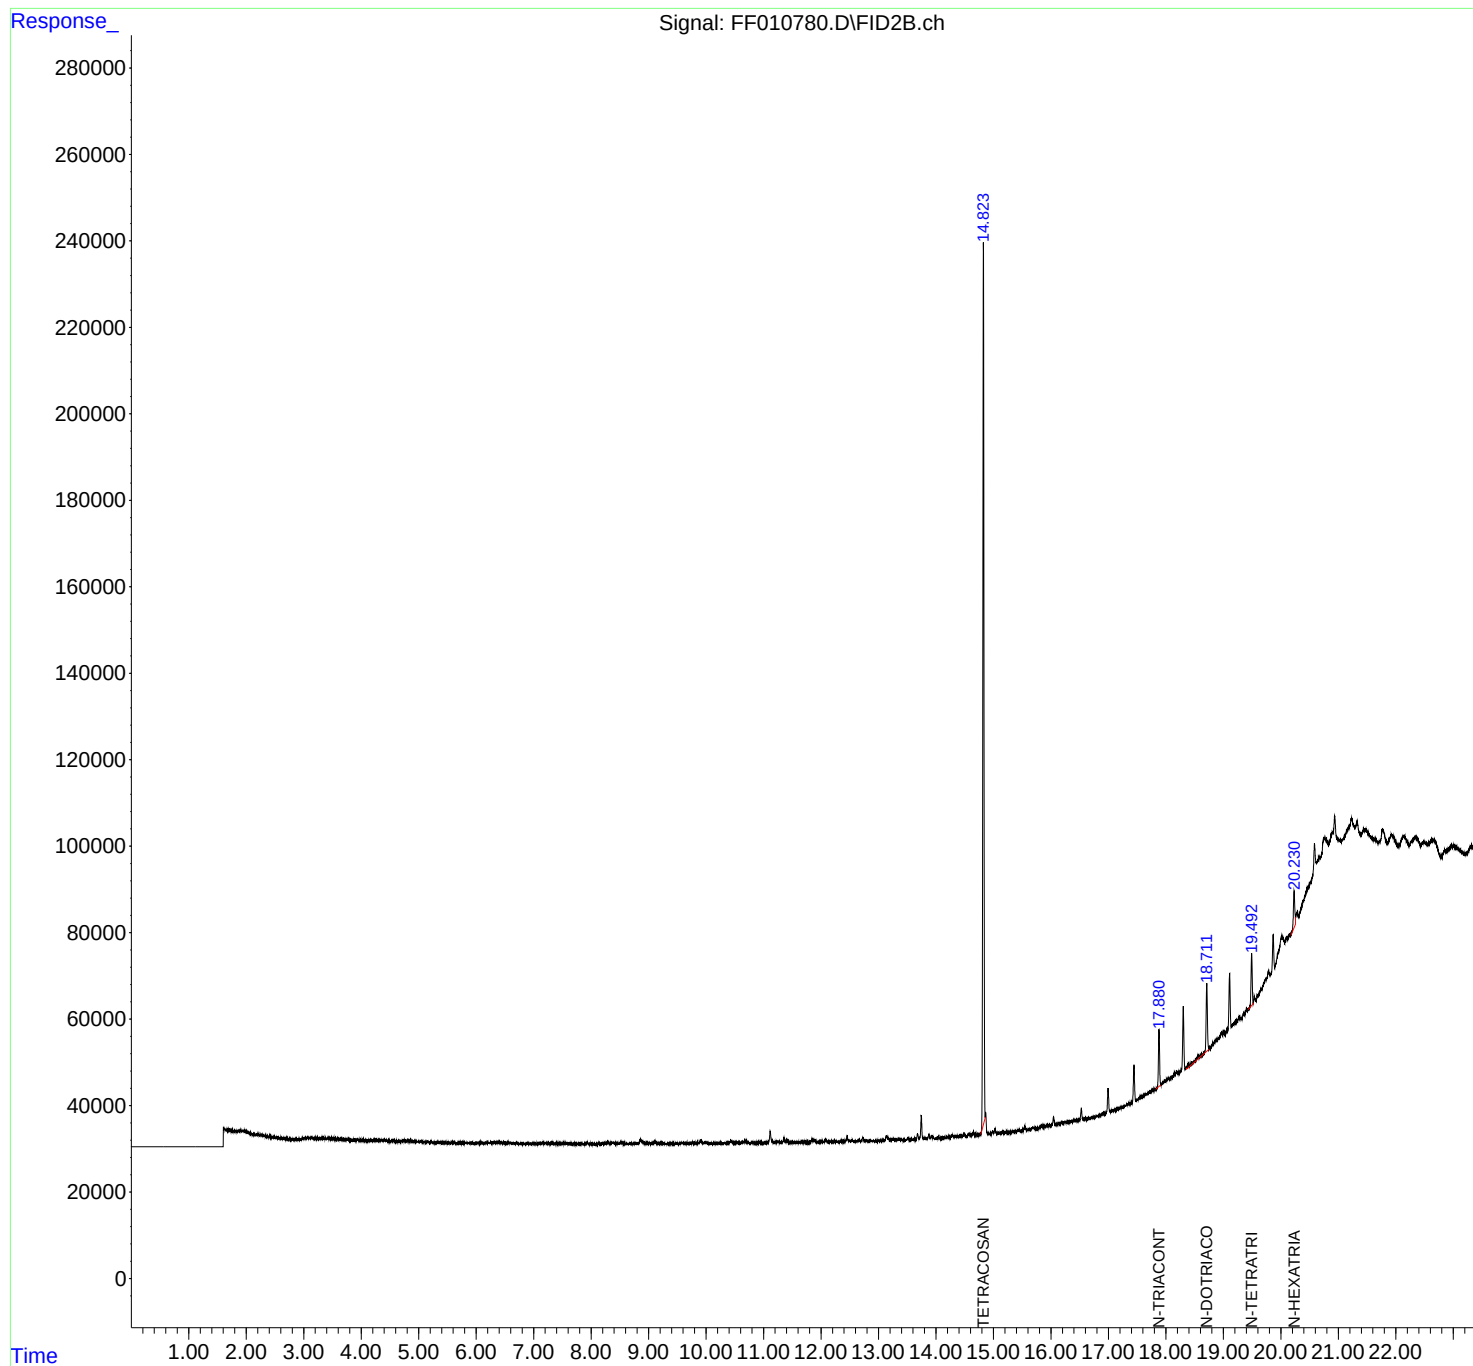


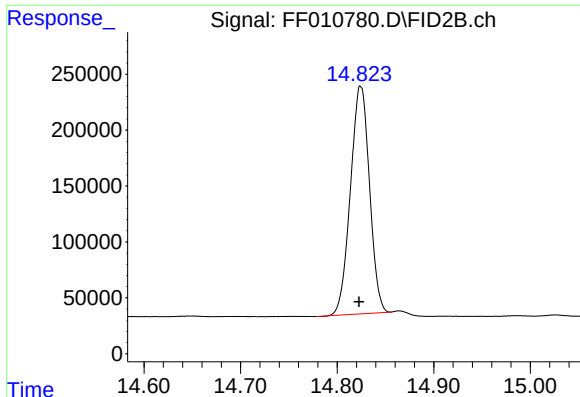

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.824 min
Delta R.T.: 0.001 min
Response: 2795055
Conc: 24.73 ug/ml

Instrument :
FID_F
ClientSampleId :

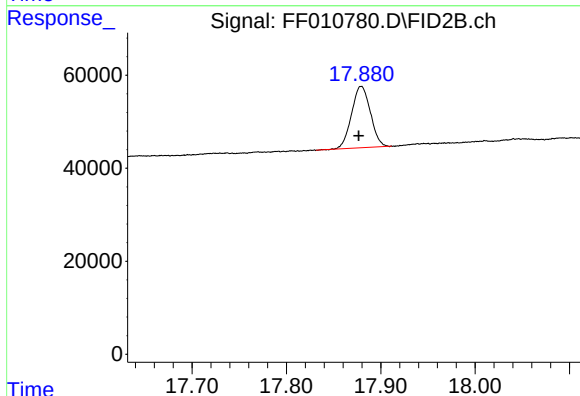


#13 N-TRIACONTANE

R.T.: 17.879 min
Delta R.T.: 0.003 min
Response: 183579
Conc: 1.50 ug/ml

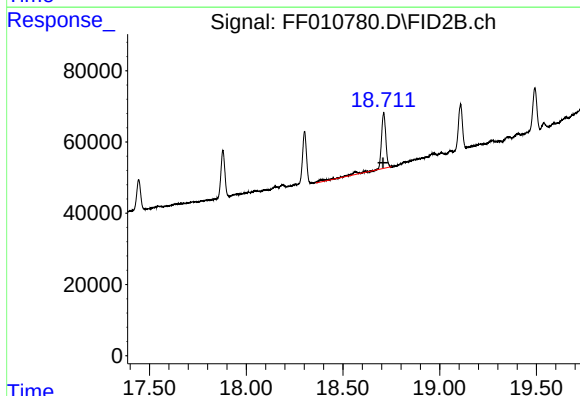


#14 N-DOTRIACONTANE

R.T.: 18.710 min
Delta R.T.: 0.003 min
Response: 277947
Conc: 2.29 ug/ml

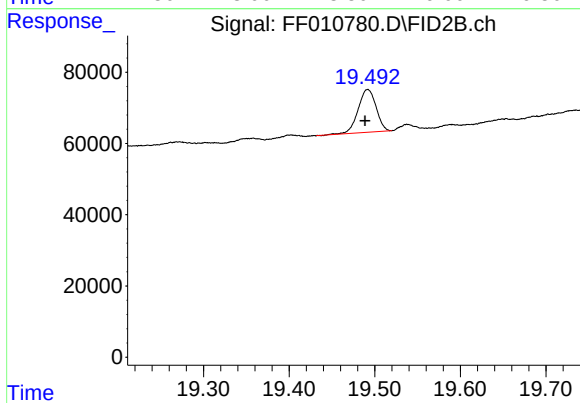

#15 N-TETRATRIACONTANE

R.T.: 19.492 min
Delta R.T.: 0.003 min
Response: 175077
Conc: 1.68 ug/ml

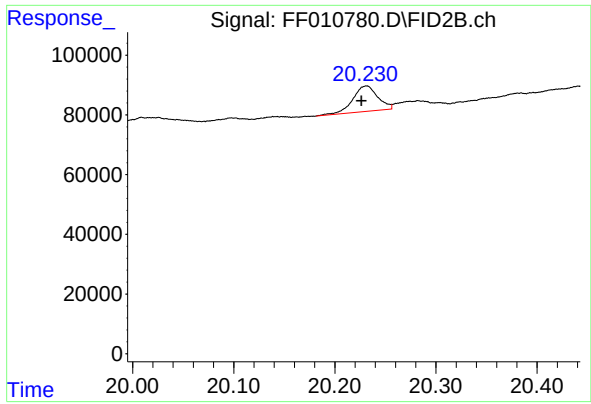

#16 N-HEXATRIACONTANE

R.T.: 20.231 min
Delta R.T.: 0.005 min
Response: 146358
Conc: 1.70 ug/ml

Instrument :

FID_F

ClientSampleId :