

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF061422\  
Data File : FF010784.D  
Signal(s) : FID2B.ch  
Acq On : 14 Jun 2022 11:42  
Operator : AJ\MA  
Sample : N3304-04 500X  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 15 01:36:47 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 6) N-OCTADECANE             | 11.419 | 90447    | 0.707 ug/ml |
| 7) N-EICOSANE               | 12.727 | 143736   | 1.137 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF061422\  
Data File : FF010784.D  
Signal(s) : FID2B.ch  
Acq On : 14 Jun 2022 11:42  
Operator : AJ\MA  
Sample : N3304-04 500X  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 15 01:36:47 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF060622.M  
Quant Title :  
QLast Update : Tue Jun 07 09:12:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

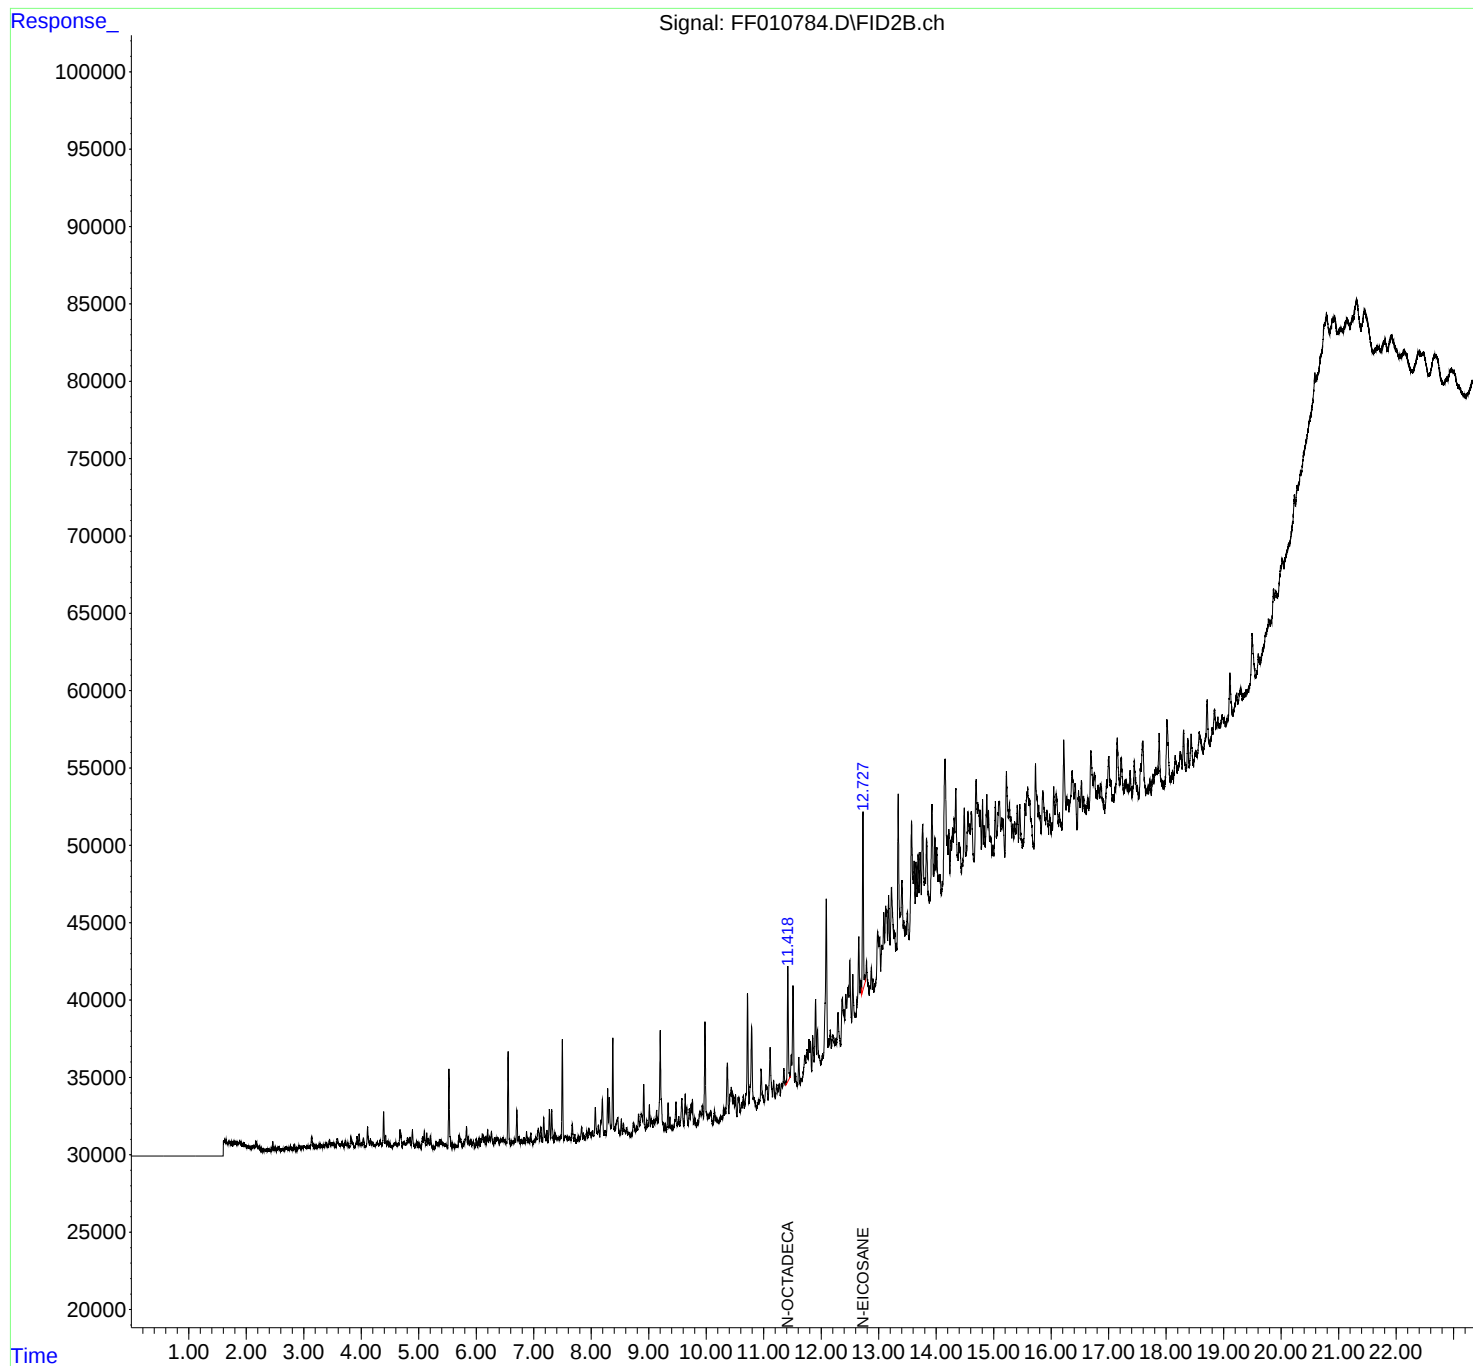


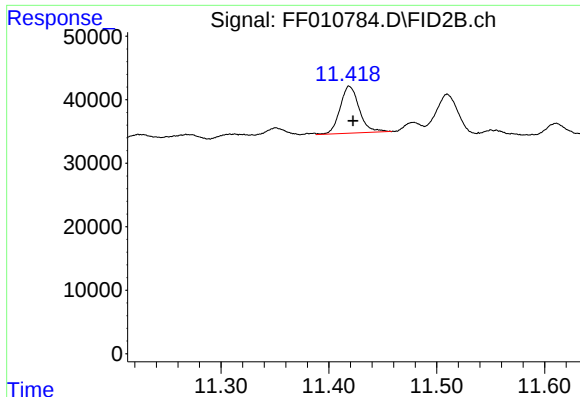

#6 N-OCTADECANE


R.T.: 11.419 min  
Delta R.T.: -0.003 min  
Response: 90447  
Conc: 0.71 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

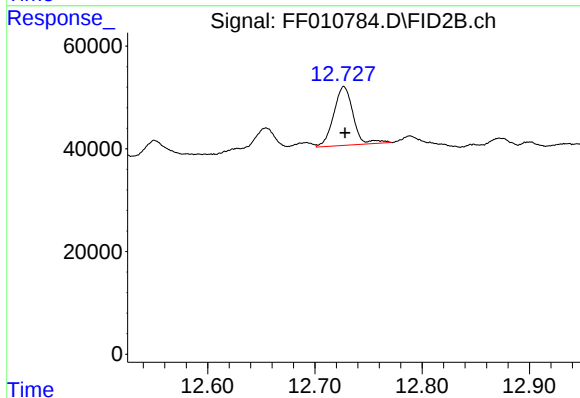

#7 N-EICOSANE

R.T.: 12.727 min  
Delta R.T.: -0.001 min  
Response: 143736  
Conc: 1.14 ug/ml

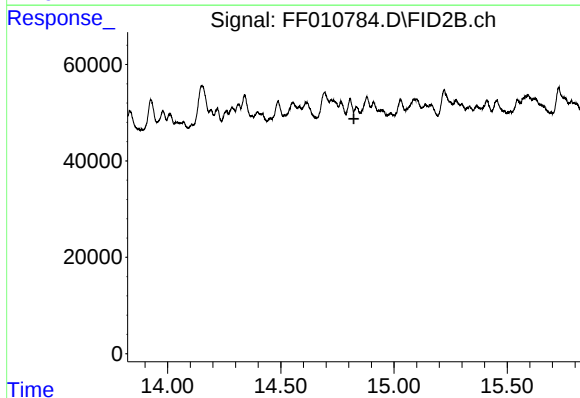

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.823 min  
Response: 0  
Conc: N.D.