

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061422\
Data File : FF010785.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2022 12:11
Operator : AJ\MA
Sample : N3304-06 200X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 01:37:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
12) N-OCTACOSANE	16.998	133001	1.090 ug/ml
13) N-TRIACONTANE	17.879	126152	1.029 ug/ml
14) N-DOTRIACONTANE	18.711	133564	1.101 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061422\
Data File : FF010785.D
Signal(s) : FID2B.ch
Acq On : 14 Jun 2022 12:11
Operator : AJ\MA
Sample : N3304-06 200X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 01:37:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

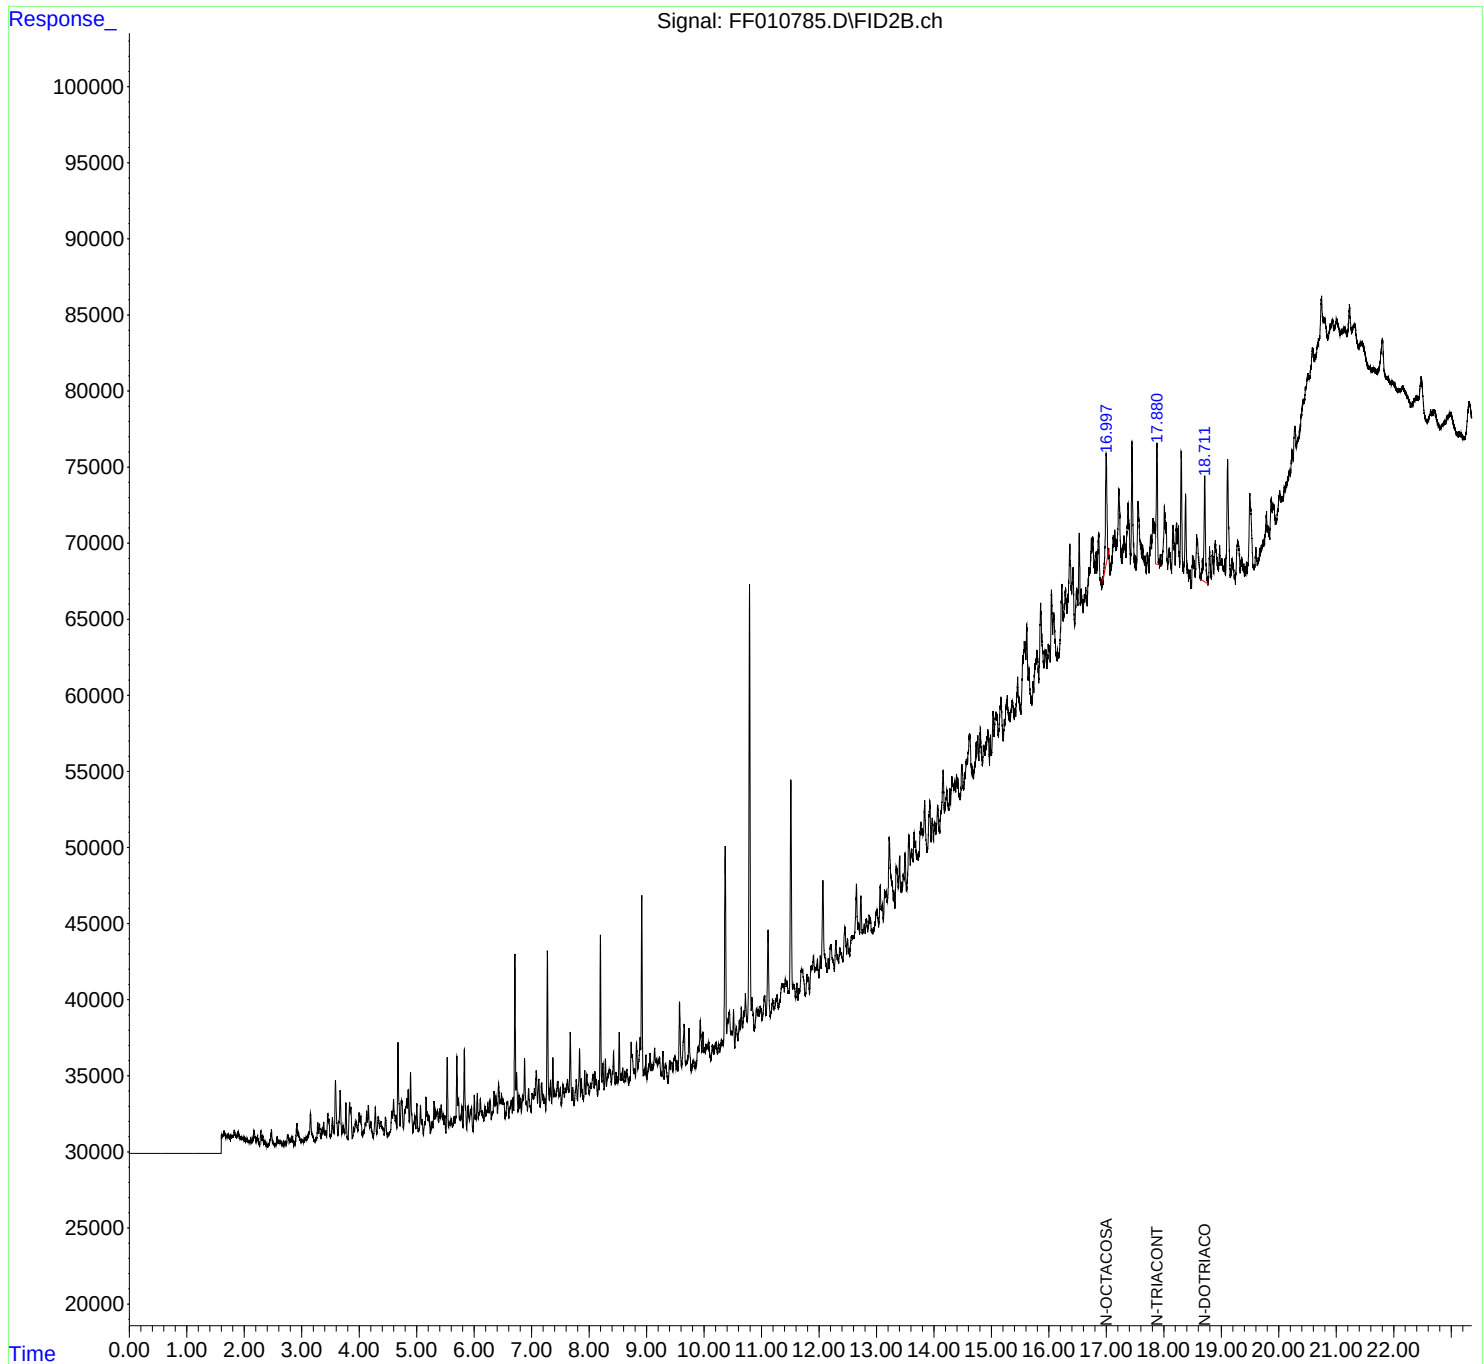


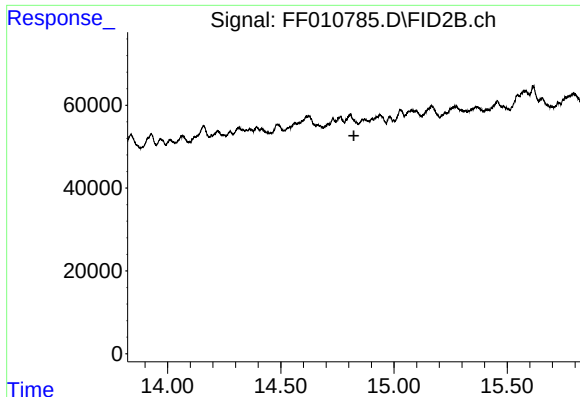

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.823 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

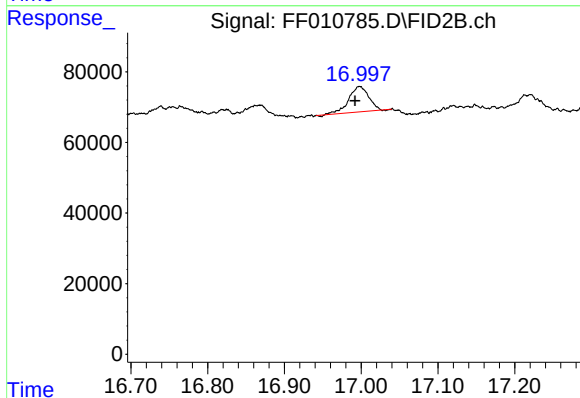


#12 N-OCTACOSANE

R.T.: 16.998 min
Delta R.T.: 0.006 min
Response: 133001
Conc: 1.09 ug/ml

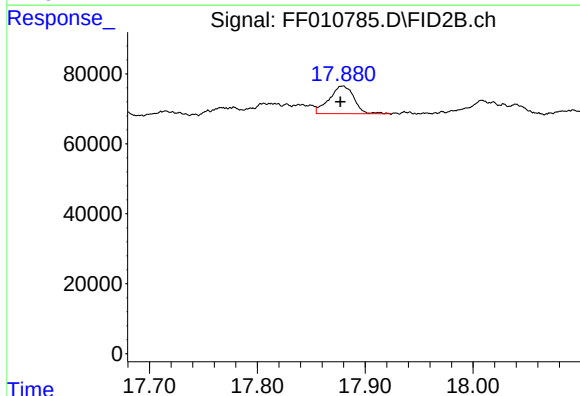

#13 N-TRIACONTANE

R.T.: 17.879 min
Delta R.T.: 0.002 min
Response: 126152
Conc: 1.03 ug/ml

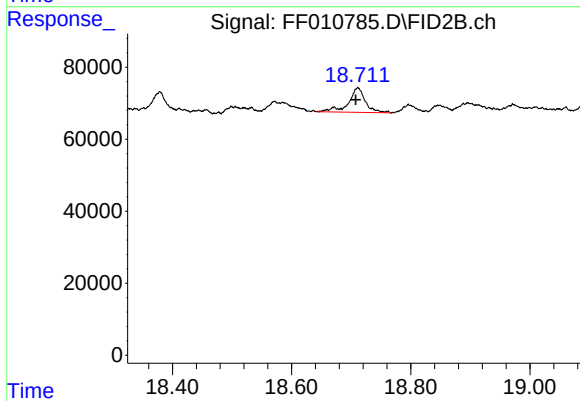

#14 N-DOTRIACONTANE

R.T.: 18.711 min
Delta R.T.: 0.004 min
Response: 133564
Conc: 1.10 ug/ml