

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000951.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 10:38
 Operator : UA\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 23:41:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.259	2681816	19.135 ug/ml
12) N-OCTACOSANE	16.660	2450789	19.273 ug/ml
16) N-HEXATRIACONTANE	19.904	409490	3.586 ug/ml
17) N-OCTATRIACONTANE	20.615	2560634	24.884 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000951.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 10:38
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 23:41:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

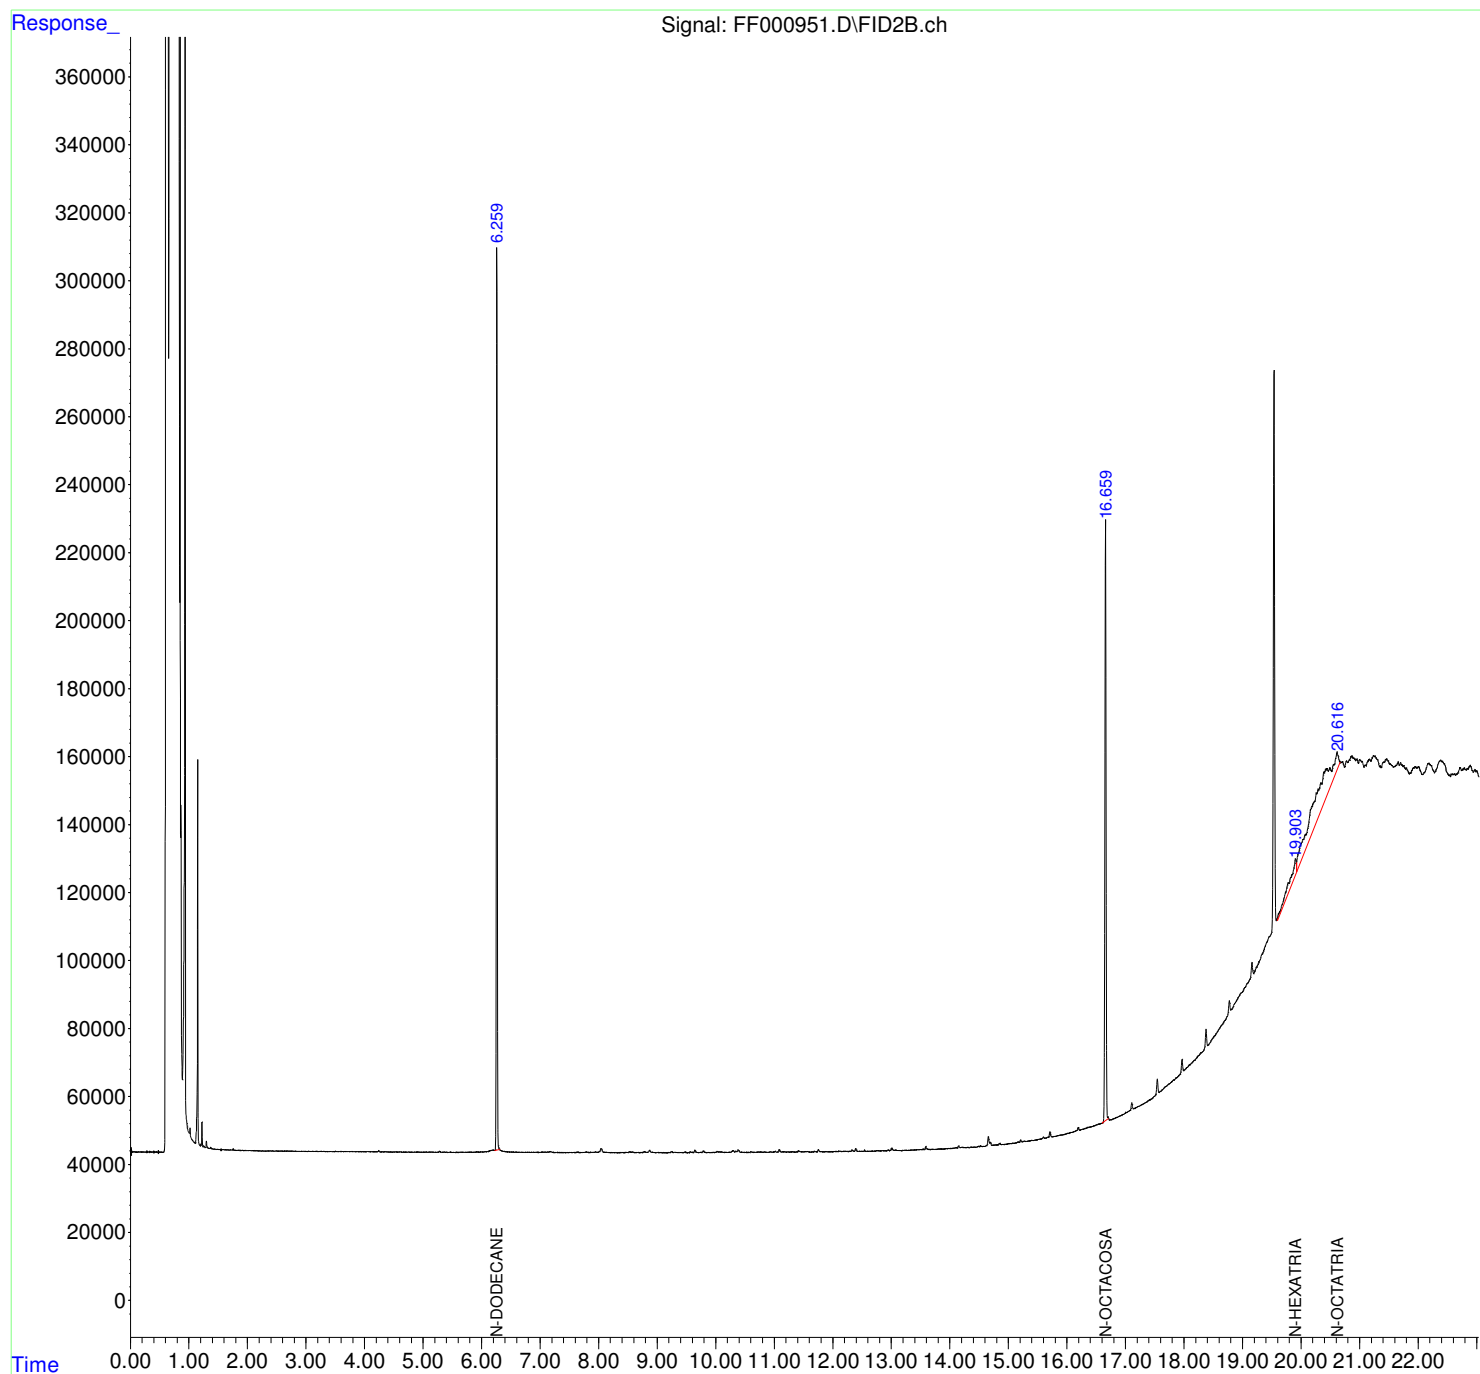


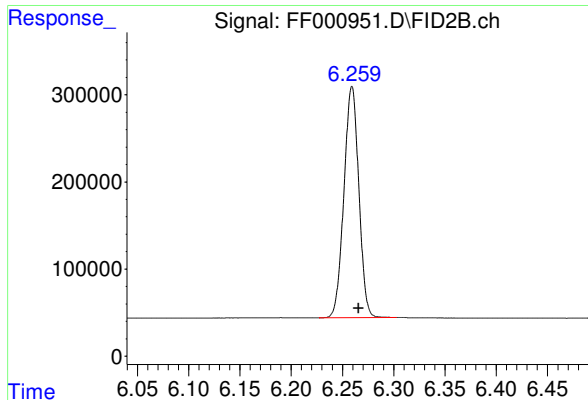

#3 N-DODECANE


R.T.: 6.259 min
Delta R.T.: -0.006 min
Response: 2681816
Conc: 19.14 ug/ml

Instrument :
FID_F
ClientSampleId :

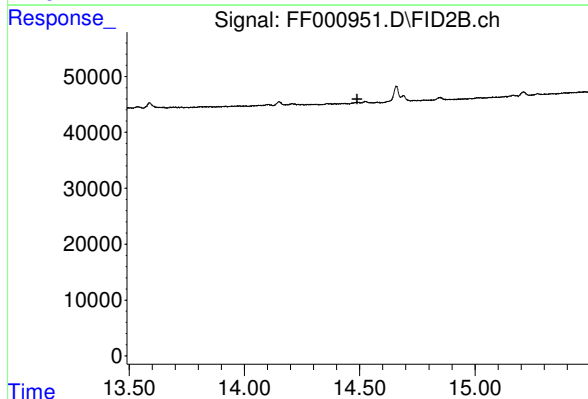


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.490 min
Response: 0
Conc: N.D.

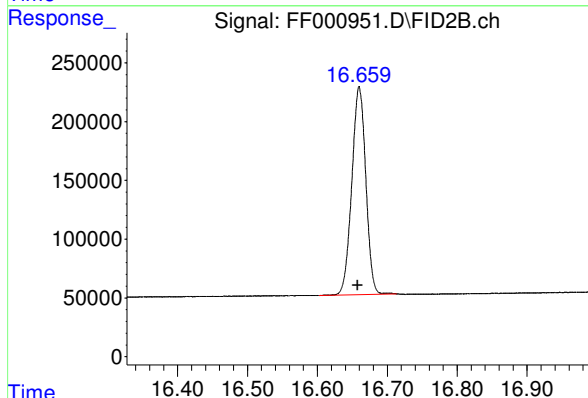


#12 N-OCTACOSANE

R.T.: 16.660 min
Delta R.T.: 0.002 min
Response: 2450789
Conc: 19.27 ug/ml

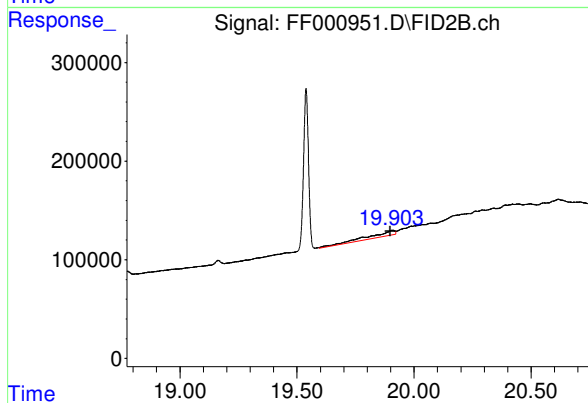

#16 N-HEXATRIACONTANE

R.T.: 19.904 min
Delta R.T.: 0.005 min
Response: 409490
Conc: 3.59 ug/ml

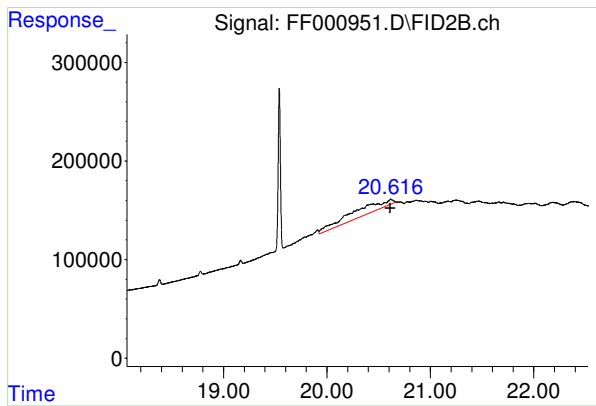

#17 N-OCTATRIACONTANE

R.T.: 20.615 min
Delta R.T.: 0.004 min
Response: 2560634
Conc: 24.88 ug/ml

Instrument :
FID_F
ClientSampleId :