

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000968.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 19:16
 Operator : UA\AJ
 Sample : J3498-10
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 23:42:17 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.485	2147855	18.624 ug/ml
Target Compounds			
1) N-OCTANE	2.164	274629	1.949 ug/ml
4) N-TETRADECANE	8.102	607211	4.361 ug/ml
5) N-HEXADECANE	9.642	233615	1.694 ug/ml
8) N-DOCOSANE	13.585	215028	1.626 ug/ml
10) N-TETRACOSANE	14.688	189848	1.464 ug/ml
11) N-HEXACOSANE	15.709	383261	2.984 ug/ml
12) N-OCTACOSANE	16.660	663427	5.217 ug/ml
13) N-TRIACONTANE	17.543	836624	6.626 ug/ml
14) N-DOTRIACONTANE	18.377	864430	7.048 ug/ml
15) N-TETRATRIACONTANE	19.174	727865	6.065 ug/ml
16) N-HEXATRIACONTANE	19.905	410909	3.599 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000968.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 19:16
Operator : UA\AJ
Sample : J3498-10
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 23:42:17 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

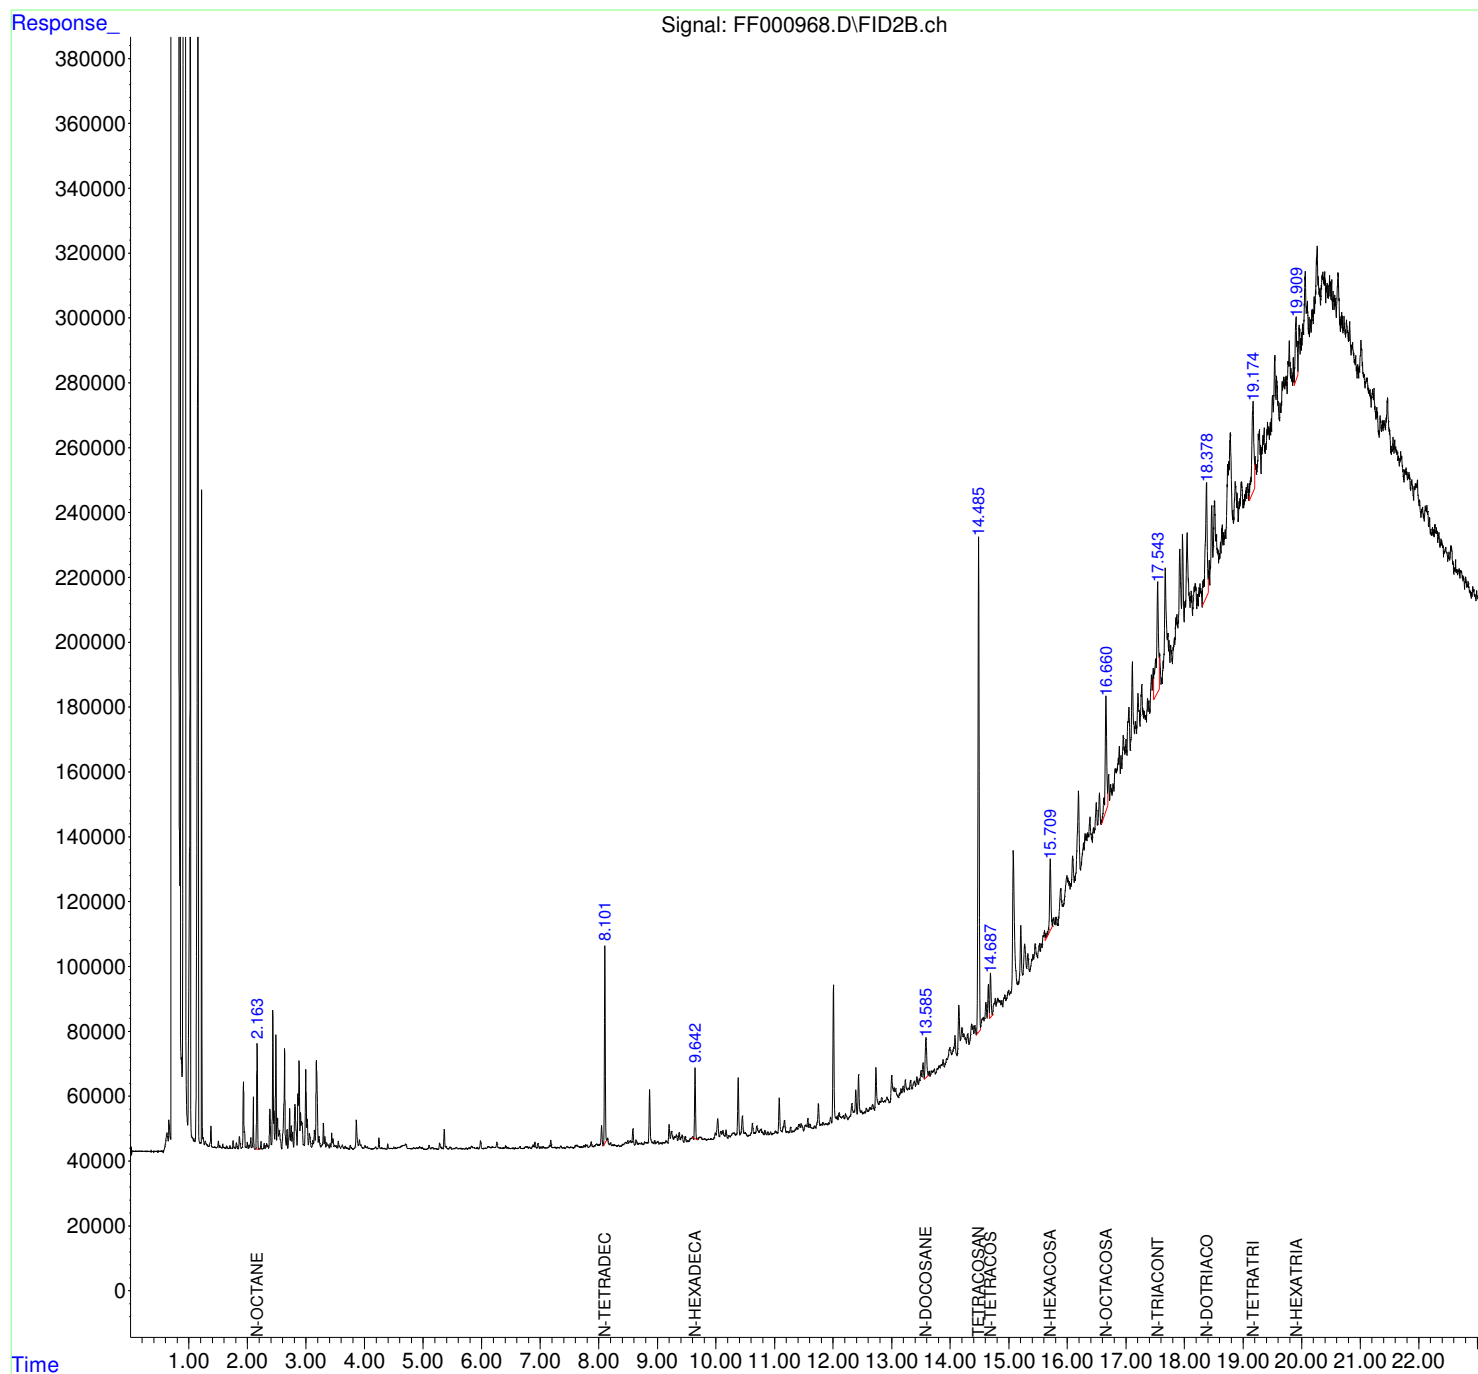


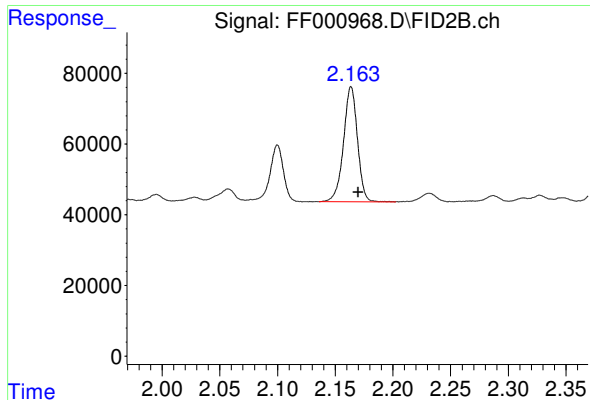

#1 N-OCTANE


R.T.: 2.164 min
Delta R.T.: -0.006 min
Response: 274629
Conc: 1.95 ug/ml

Instrument :
FID_F
ClientSampleId :

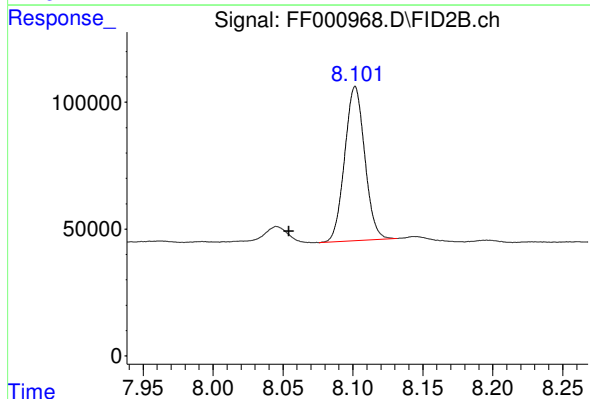


#4 N-TETRADECANE

R.T.: 8.102 min
Delta R.T.: 0.047 min
Response: 607211
Conc: 4.36 ug/ml

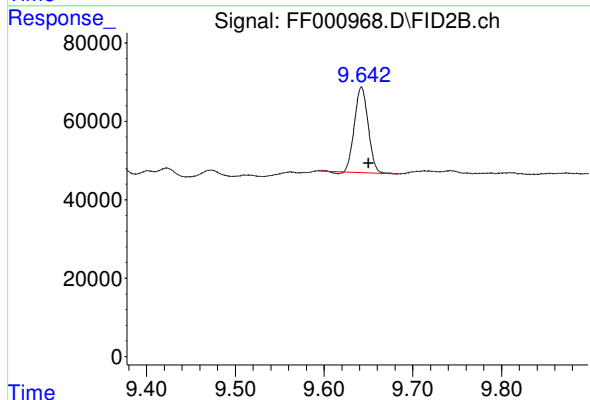


#5 N-HEXADECANE

R.T.: 9.642 min
Delta R.T.: -0.008 min
Response: 233615
Conc: 1.69 ug/ml

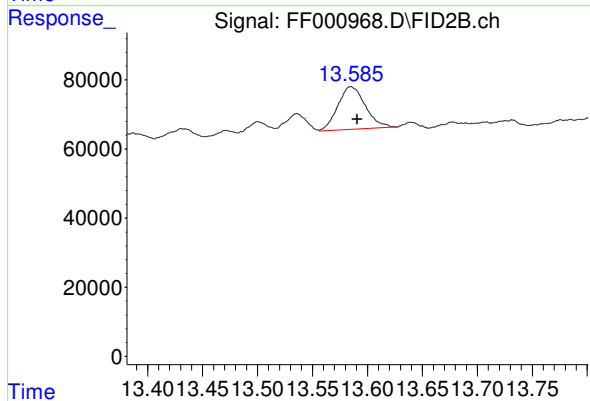

#8 N-DOCOSANE


R.T.: 13.585 min
Delta R.T.: -0.006 min
Response: 215028
Conc: 1.63 ug/ml

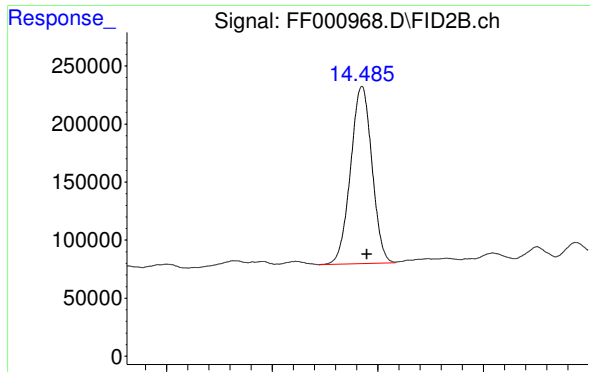

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.485 min
Delta R.T.: -0.005 min
Response: 2147855
Conc: 18.62 ug/ml

Instrument :
FID_F
ClientSampleId :

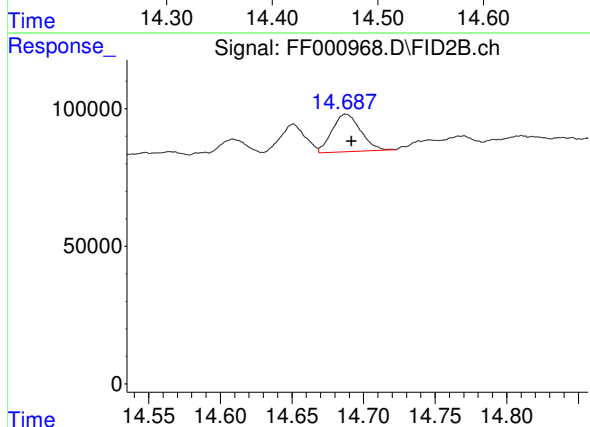


#10 N-TETRACOSANE

R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 189848
Conc: 1.46 ug/ml

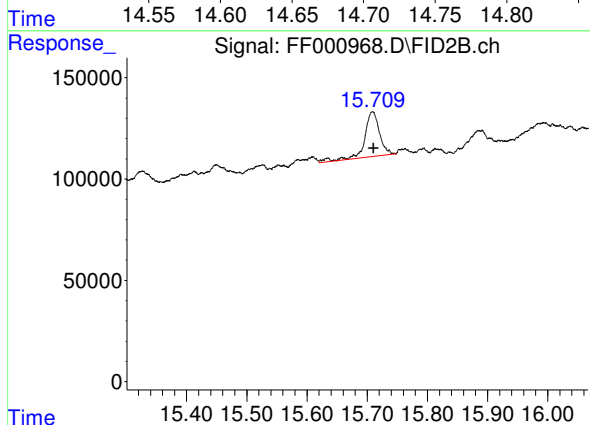


#11 N-HEXACOSANE

R.T.: 15.709 min
Delta R.T.: -0.002 min
Response: 383261
Conc: 2.98 ug/ml

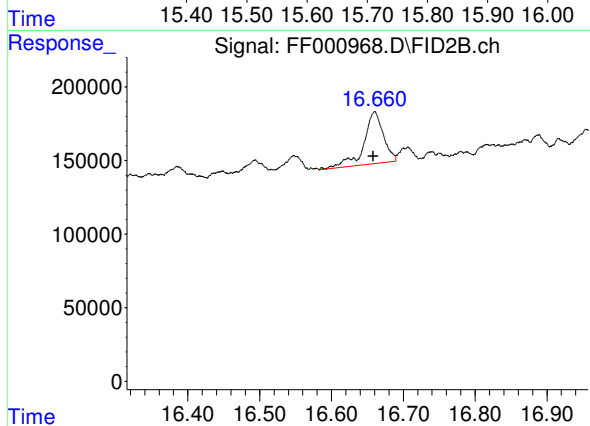

#12 N-OCTACOSANE


R.T.: 16.660 min
Delta R.T.: 0.002 min
Response: 663427
Conc: 5.22 ug/ml

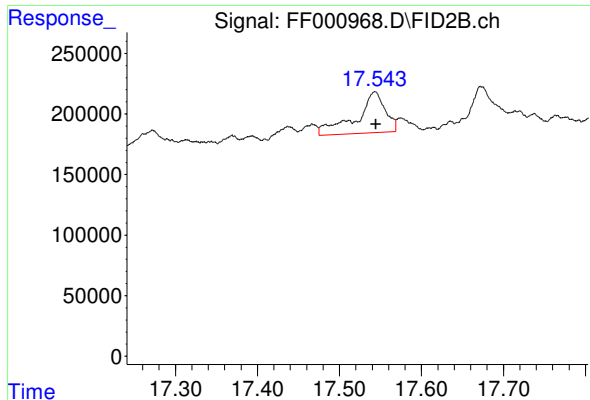

#13 N-TRIACONTANE


R.T.: 17.543 min
Delta R.T.: -0.001 min
Response: 836624
Conc: 6.63 ug/ml

Instrument :
FID_F
ClientSampleId :

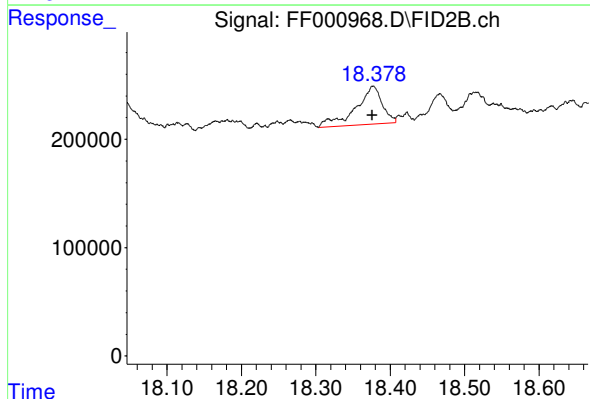


#14 N-DOTRIACONTANE

R.T.: 18.377 min
Delta R.T.: 0.002 min
Response: 864430
Conc: 7.05 ug/ml

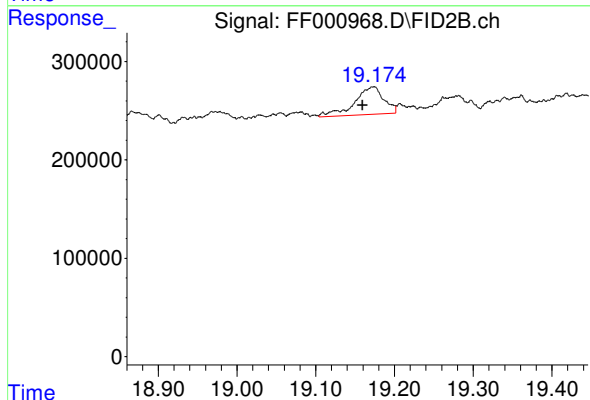

#15 N-TETRATRIACONTANE

R.T.: 19.174 min
Delta R.T.: 0.014 min
Response: 727865
Conc: 6.07 ug/ml

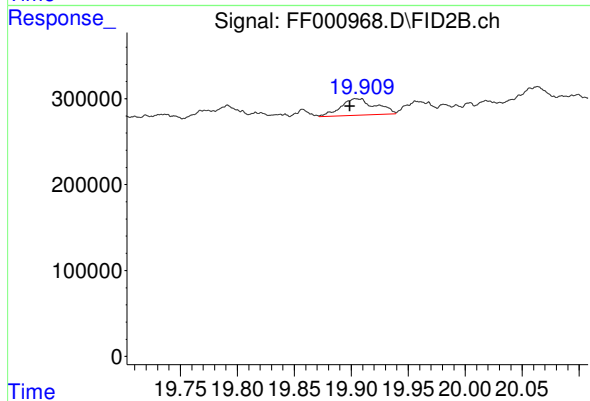

#16 N-HEXATRIACONTANE

R.T.: 19.905 min
Delta R.T.: 0.007 min
Response: 410909
Conc: 3.60 ug/ml