

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000970.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 20:15
 Operator : UA\AJ
 Sample : J3498-14
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 23:42:23 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.485	1644250	14.258 ug/ml
Target Compounds			
4) N-TETRADECANE	8.102	473398	3.400 ug/ml
5) N-HEXADECANE	9.643	185091	1.342 ug/ml
7) N-EICOSANE	12.436	235940	1.761 ug/ml
14) N-DOTRIACONTANE	18.372	175101	1.428 ug/ml
15) N-TETRATRIACONTANE	19.160	26854	0.224 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000970.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 20:15
Operator : UA\AJ
Sample : J3498-14
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 23:42:23 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

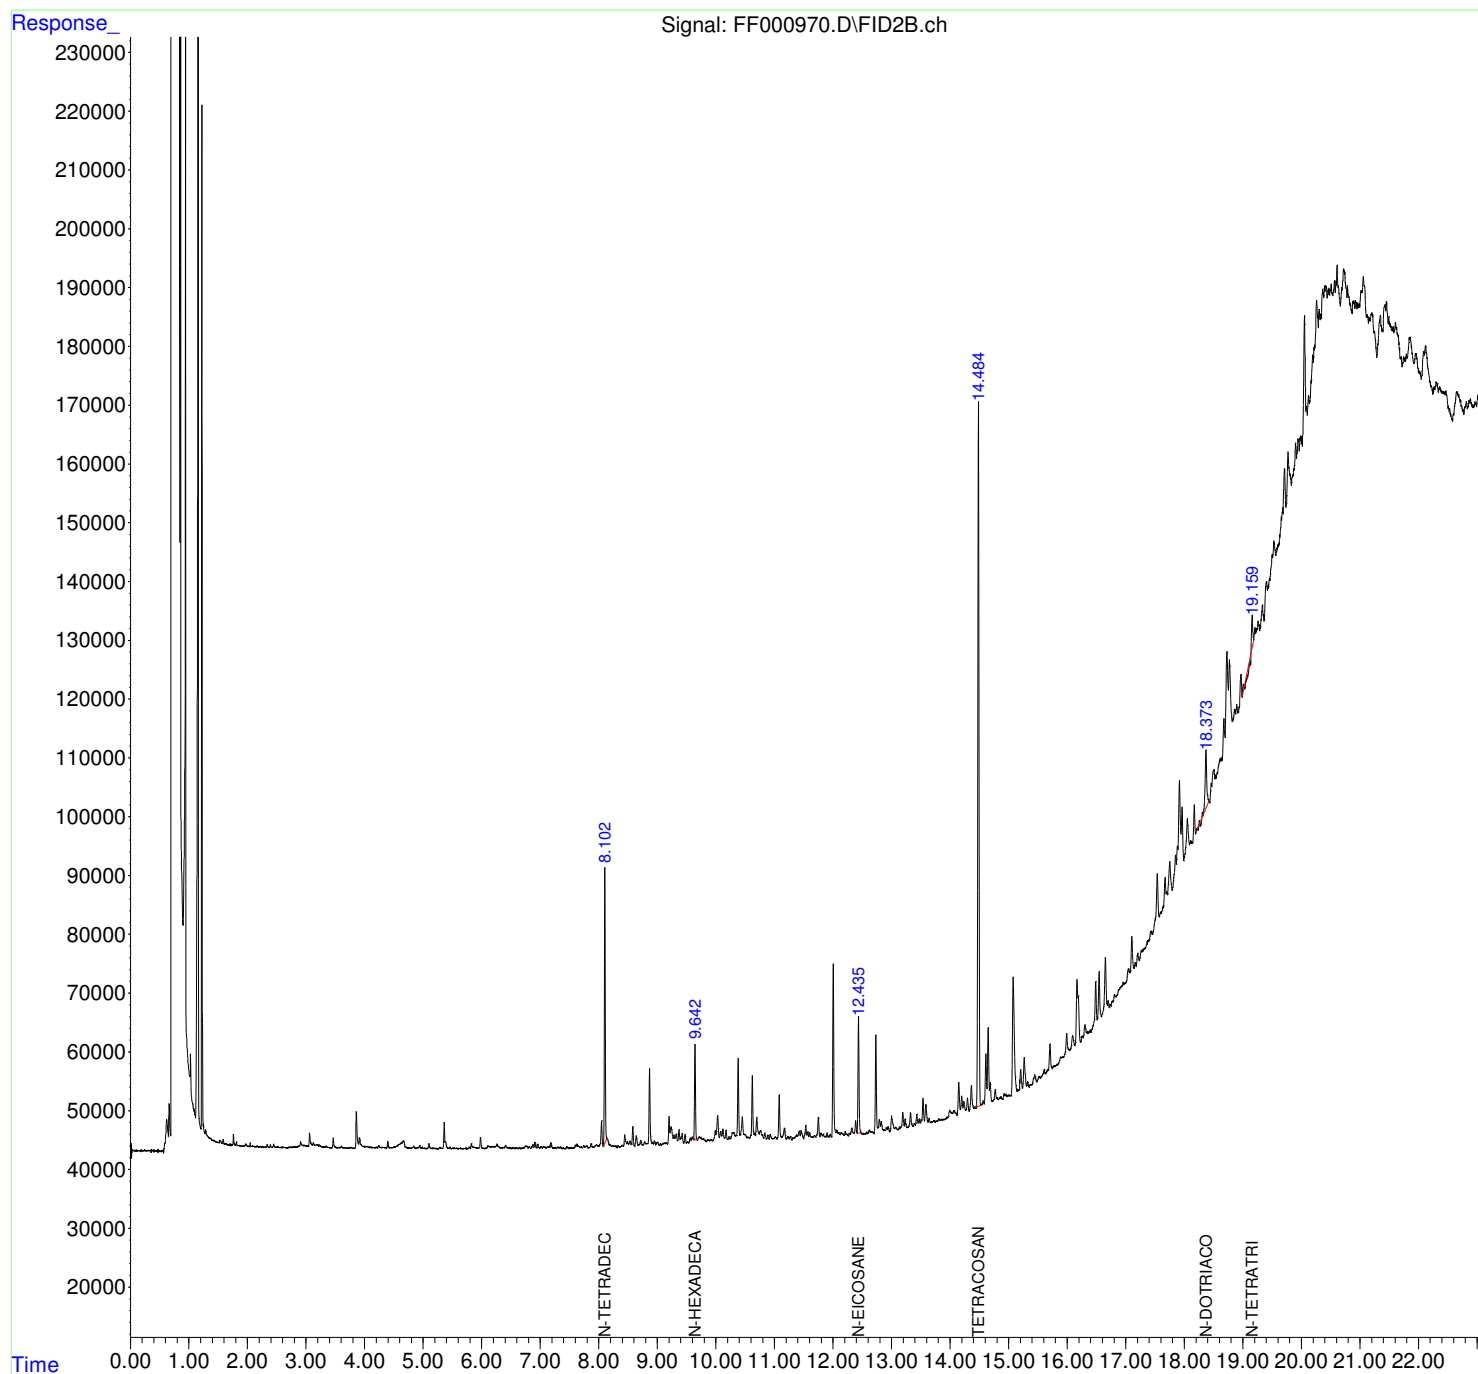


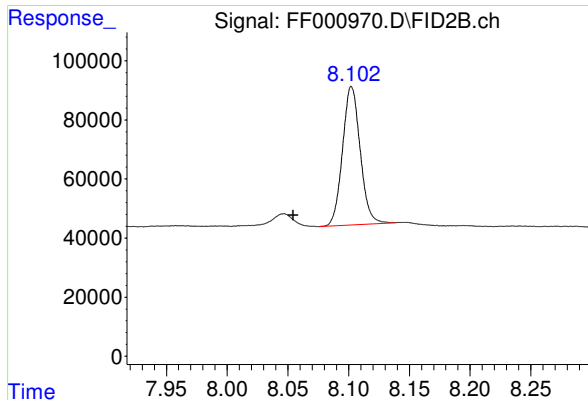

#4 N-TETRADECANE


R.T.: 8.102 min
Delta R.T.: 0.048 min
Response: 473398
Conc: 3.40 ug/ml

Instrument :
FID_F
ClientSampleId :

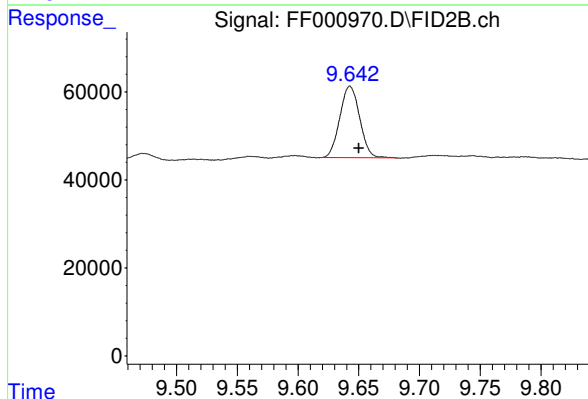


#5 N-HEXADECANE

R.T.: 9.643 min
Delta R.T.: -0.007 min
Response: 185091
Conc: 1.34 ug/ml

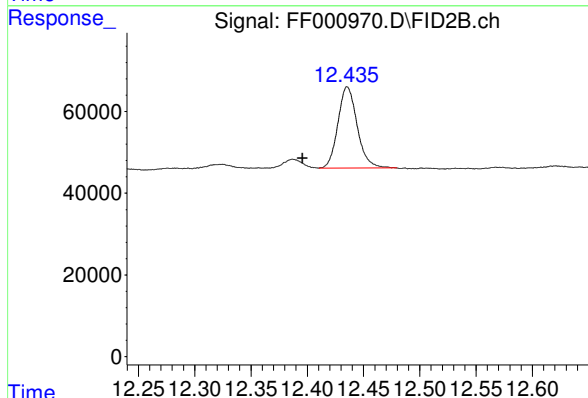


#7 N-EICOSANE

R.T.: 12.436 min
Delta R.T.: 0.040 min
Response: 235940
Conc: 1.76 ug/ml

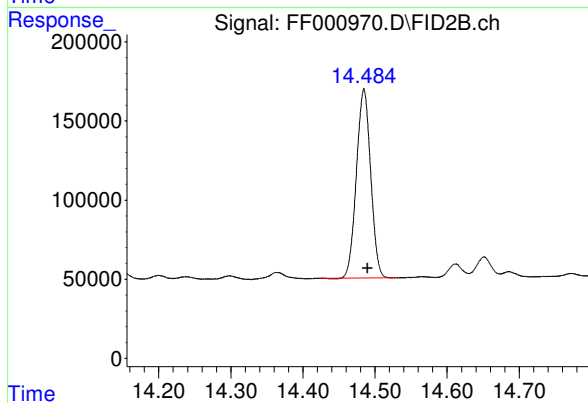

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.485 min
Delta R.T.: -0.005 min
Response: 1644250
Conc: 14.26 ug/ml

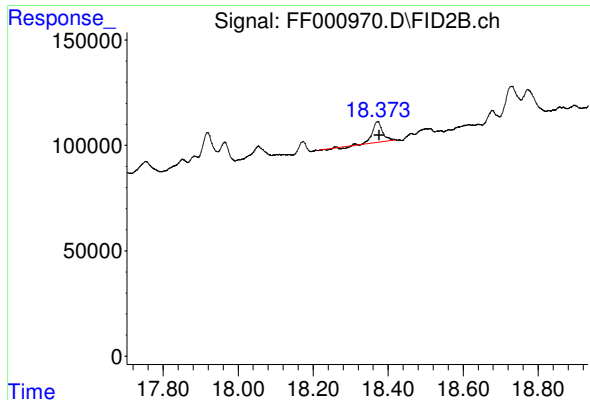

#14 N-DOTRIACONTANE

R.T.: 18.372 min
Delta R.T.: -0.003 min
Response: 175101
Conc: 1.43 ug/ml

Instrument :
FID_F
ClientSampleId :

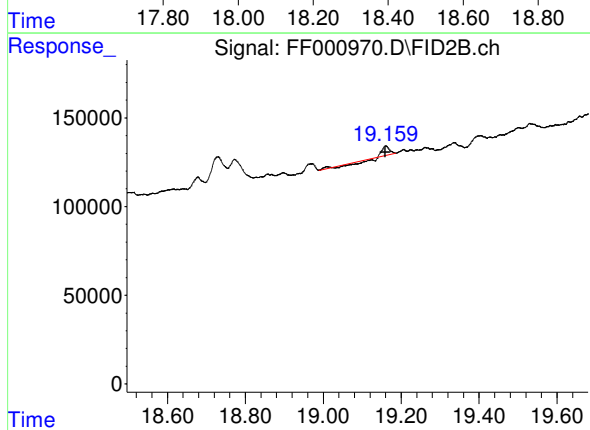

#15 N-TETRATRIACONTANE

R.T.: 19.160 min
Delta R.T.: 0.000 min
Response: 26854
Conc: 0.22 ug/ml