

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000950.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 10:07
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 23:41:15 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.492	5854633	50.767 ug/ml
Target Compounds			
2) N-DECANE	4.249	7661851	54.682 ug/ml
3) N-DODECANE	6.263	7533539	53.753 ug/ml
4) N-TETRADECANE	8.053	7420840	53.299 ug/ml
5) N-HEXADECANE	9.650	7298434	52.934 ug/ml
6) N-OCTADECANE	11.089	7176284	52.553 ug/ml
7) N-EICOSANE	12.397	6990943	52.180 ug/ml
8) N-DOCOSANE	13.593	6848412	51.793 ug/ml
10) N-TETRACOSANE	14.695	6774099	52.225 ug/ml
11) N-HEXACOSANE	15.716	6716607	52.292 ug/ml
12) N-OCTACOSANE	16.665	6780498	53.323 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000950.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 10:07
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 23:41:15 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

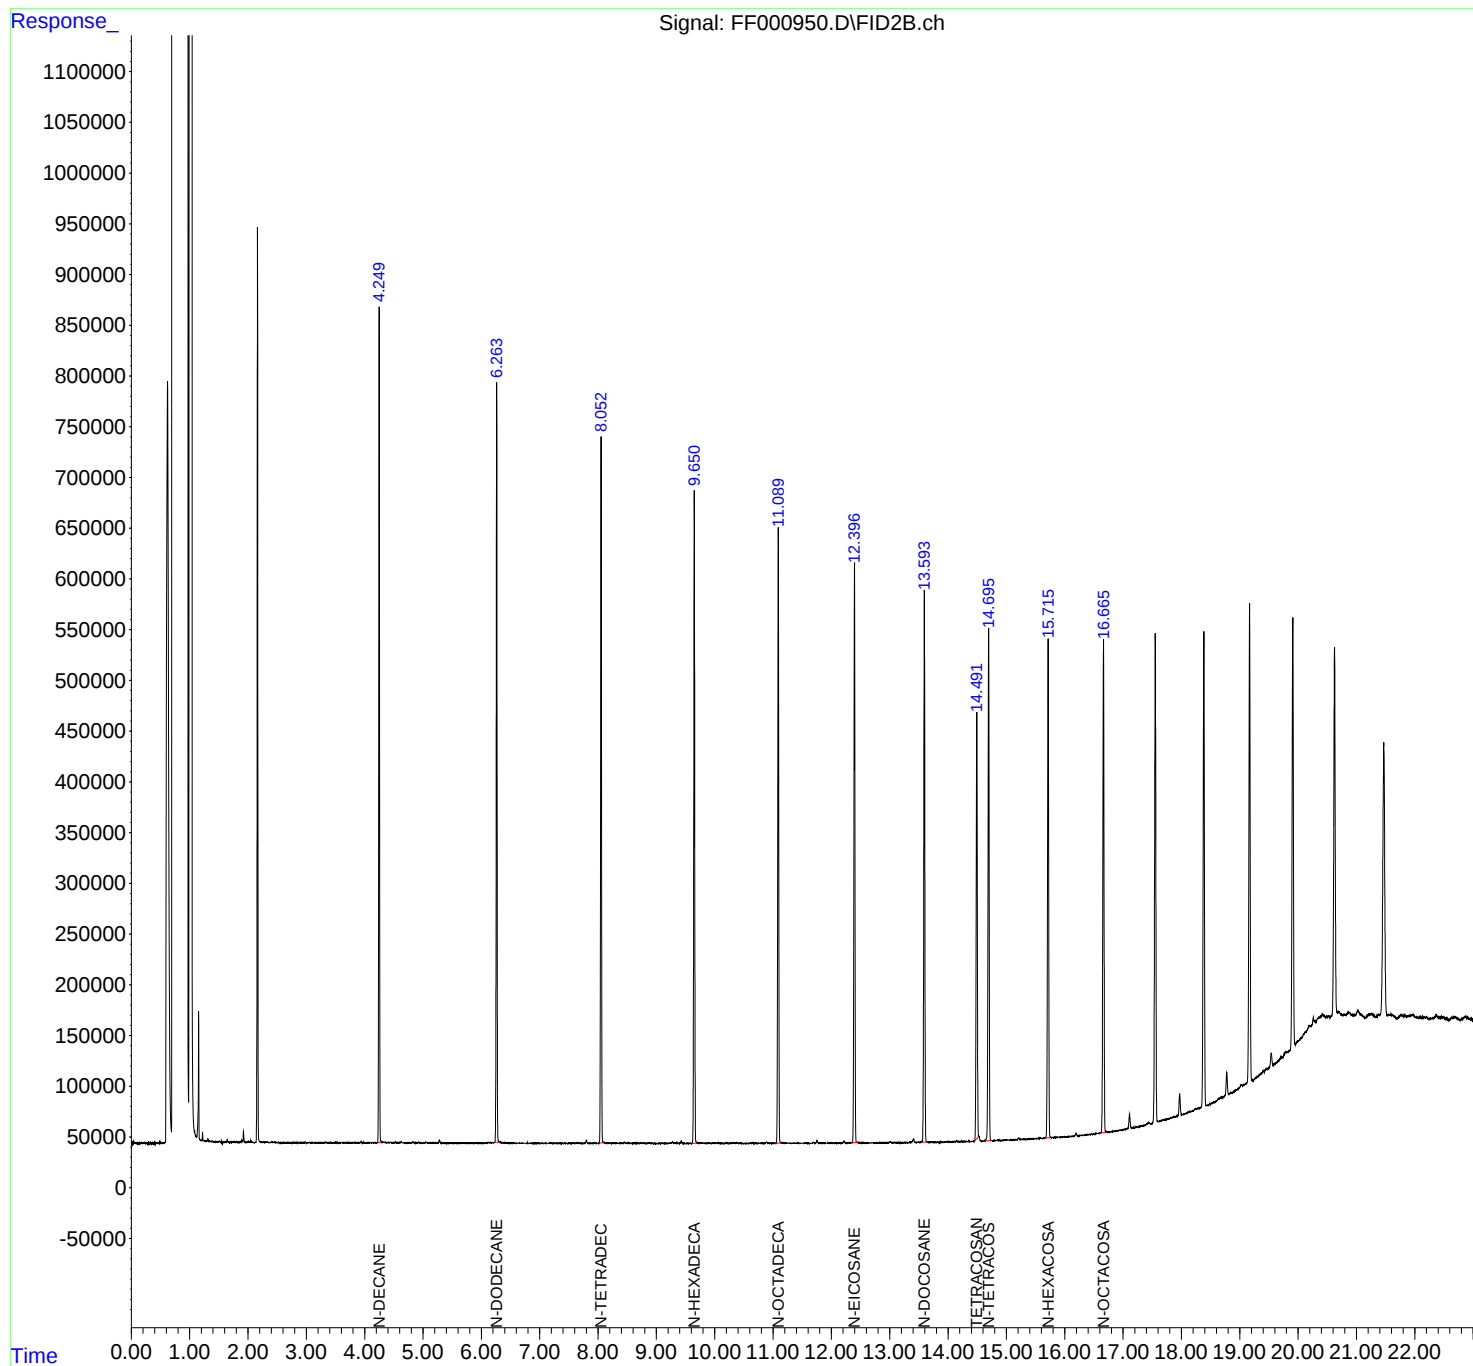


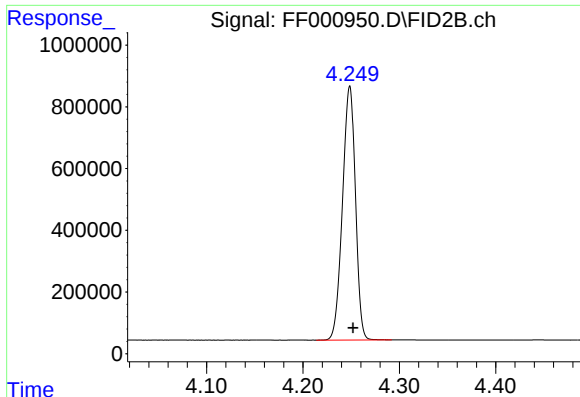

#2 N-DECANE


R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 7661851
Conc: 54.68 ug/ml

Instrument :
FID_F
ClientSampleId :

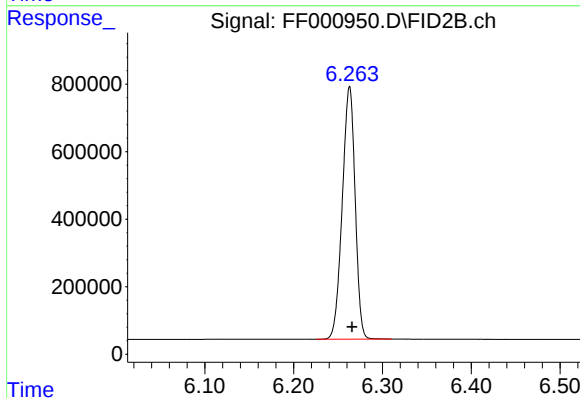


#3 N-DODECANE

R.T.: 6.263 min
Delta R.T.: -0.003 min
Response: 7533539
Conc: 53.75 ug/ml

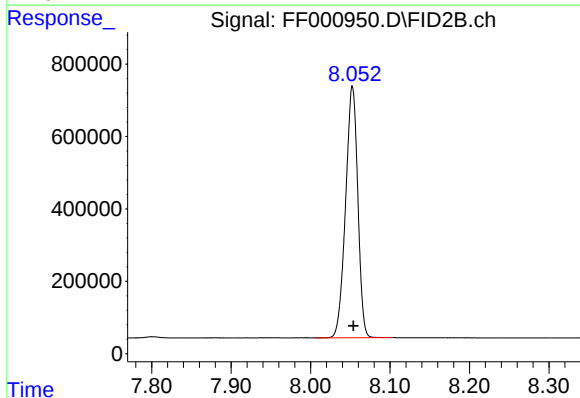


#4 N-TETRADECANE

R.T.: 8.053 min
Delta R.T.: -0.001 min
Response: 7420840
Conc: 53.30 ug/ml

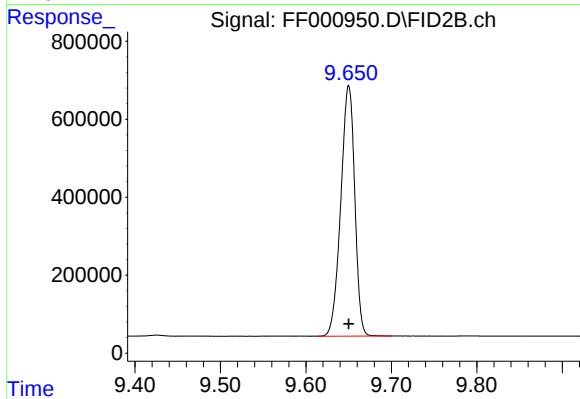

#5 N-HEXADECANE


R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 7298434
Conc: 52.93 ug/ml

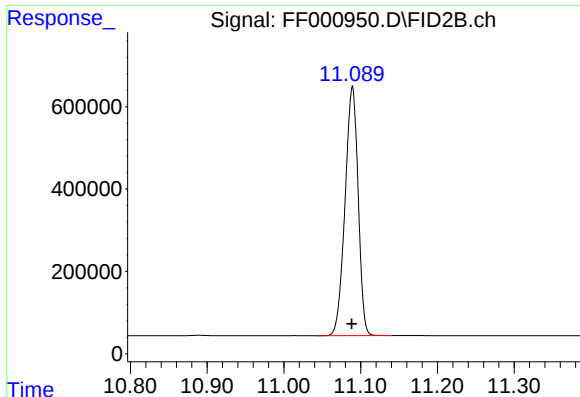

#6 N-OCTADECANE


R.T.: 11.089 min
Delta R.T.: 0.000 min
Response: 7176284
Conc: 52.55 ug/ml

Instrument :
FID_F
ClientSampleId :

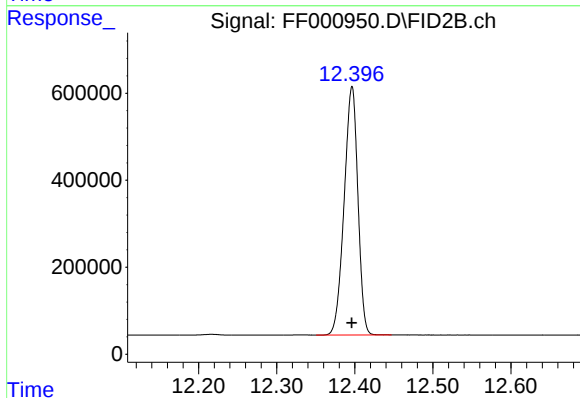


#7 N-EICOSANE

R.T.: 12.397 min
Delta R.T.: 0.000 min
Response: 6990943
Conc: 52.18 ug/ml

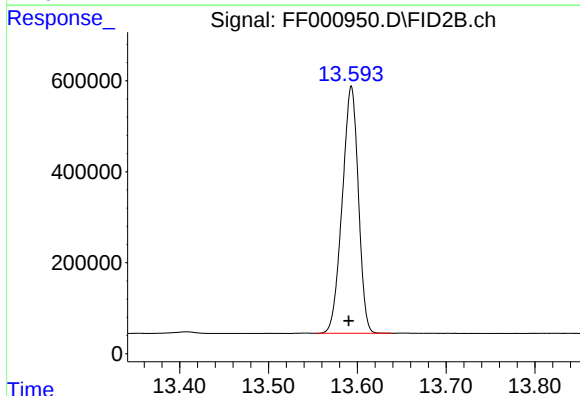


#8 N-DOCOSANE

R.T.: 13.593 min
Delta R.T.: 0.003 min
Response: 6848412
Conc: 51.79 ug/ml

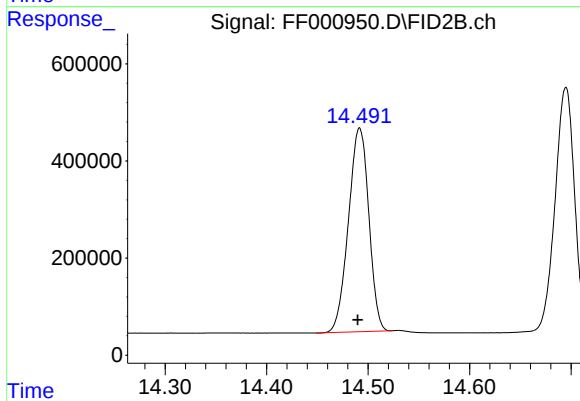

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.492 min
Delta R.T.: 0.002 min
Response: 5854633
Conc: 50.77 ug/ml

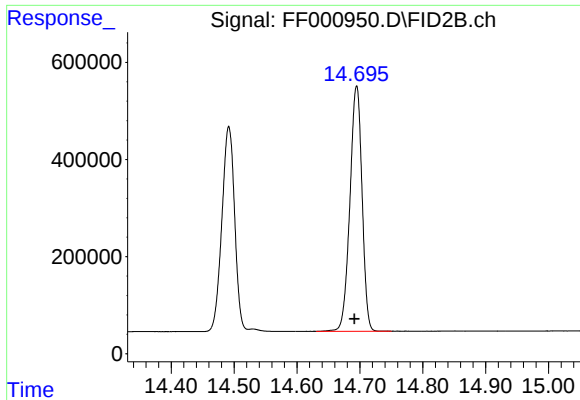

#10 N-TETRACOSANE


R.T.: 14.695 min
Delta R.T.: 0.003 min
Response: 6774099
Conc: 52.23 ug/ml

Instrument :
FID_F
ClientSampleId :

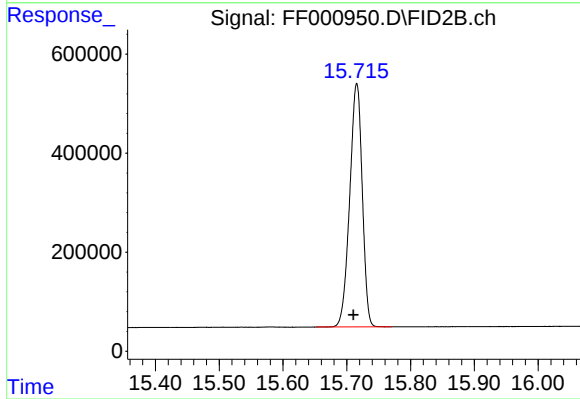

#11 N-HEXACOSANE

R.T.: 15.716 min
Delta R.T.: 0.005 min
Response: 6716607
Conc: 52.29 ug/ml

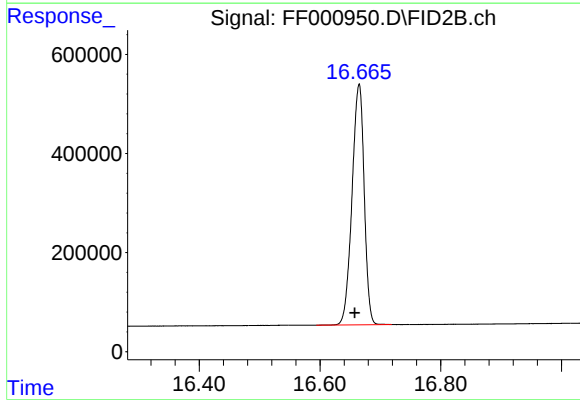

#12 N-OCTACOSANE

R.T.: 16.665 min
Delta R.T.: 0.007 min
Response: 6780498
Conc: 53.32 ug/ml