

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000961.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 15:46
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 23:41:52 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.488	5456885	47.318 ug/ml
Target Compounds			
2) N-DECANE	4.248	7133130	50.908 ug/ml
3) N-DODECANE	6.263	7032201	50.175 ug/ml
4) N-TETRADECANE	8.051	6939757	49.844 ug/ml
5) N-HEXADECANE	9.647	6814298	49.423 ug/ml
6) N-OCTADECANE	11.086	6694574	49.025 ug/ml
7) N-EICOSANE	12.394	6524787	48.701 ug/ml
8) N-DOCOSANE	13.590	6391696	48.339 ug/ml
10) N-TETRACOSANE	14.692	6329508	48.798 ug/ml
11) N-HEXACOSANE	15.713	6281842	48.907 ug/ml
12) N-OCTACOSANE	16.662	6366270	50.065 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000961.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 15:46
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 23:41:52 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

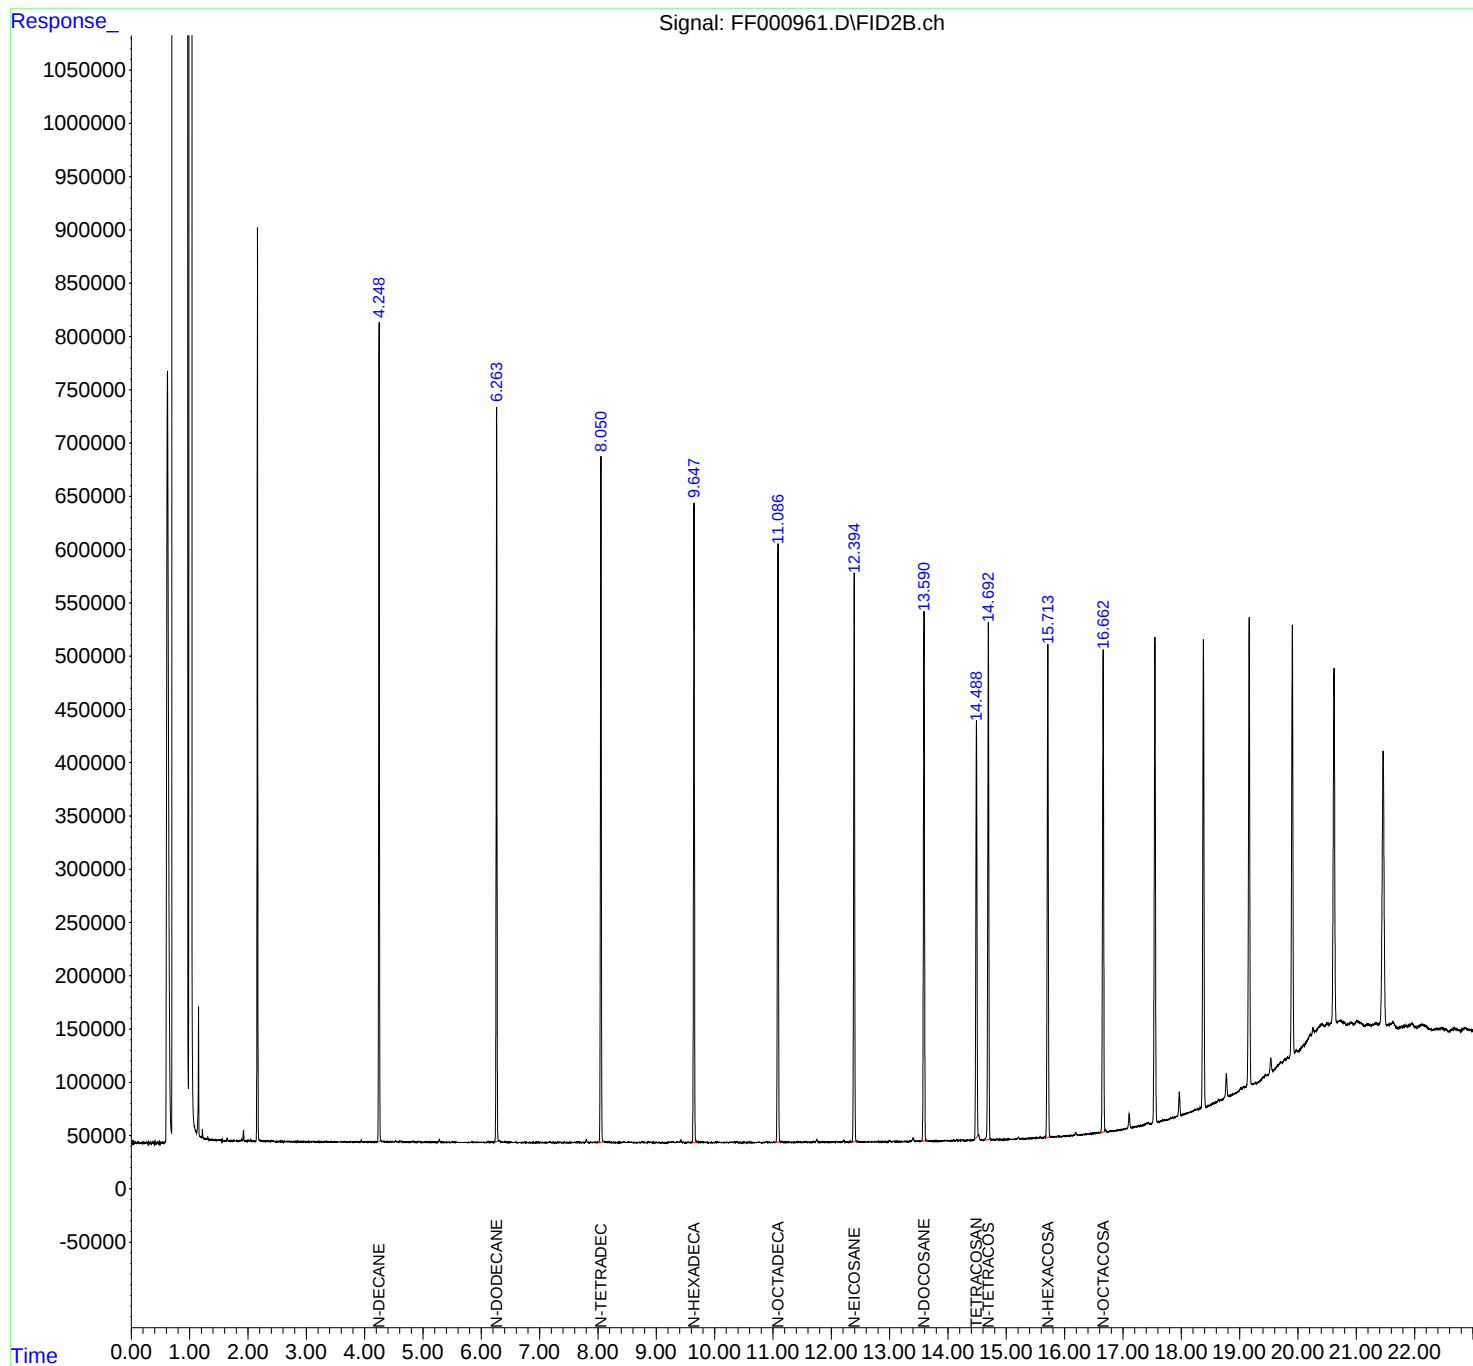


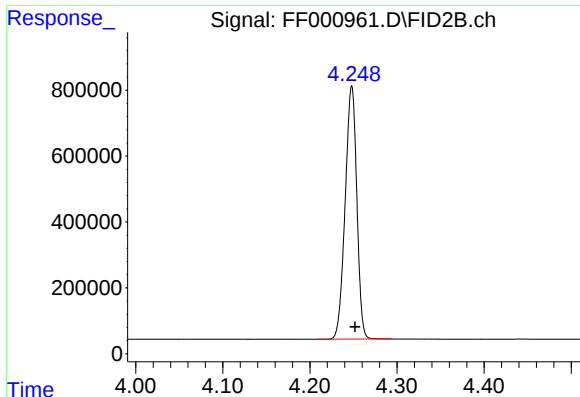

#2 N-DECANE


R.T.: 4.248 min
Delta R.T.: -0.004 min
Response: 7133130
Conc: 50.91 ug/ml

Instrument :
FID_F
ClientSampleId :

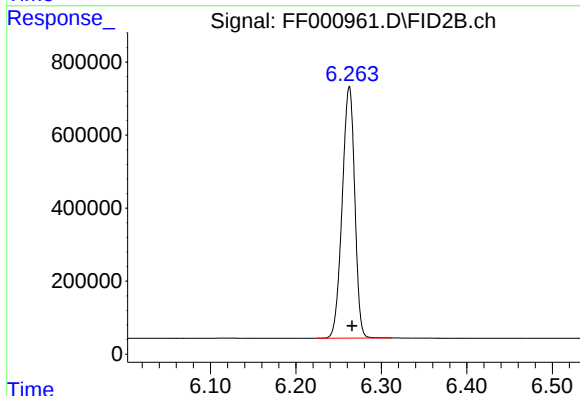


#3 N-DODECANE

R.T.: 6.263 min
Delta R.T.: -0.003 min
Response: 7032201
Conc: 50.18 ug/ml

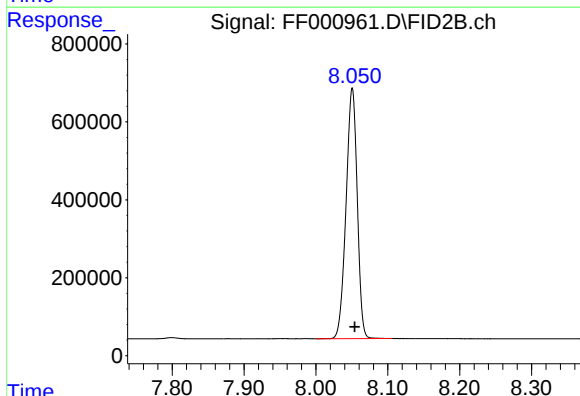


#4 N-TETRADECANE

R.T.: 8.051 min
Delta R.T.: -0.004 min
Response: 6939757
Conc: 49.84 ug/ml

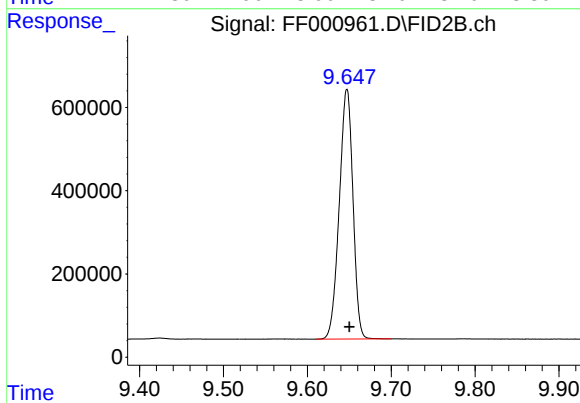

#5 N-HEXADECANE


R.T.: 9.647 min
Delta R.T.: -0.003 min
Response: 6814298
Conc: 49.42 ug/ml

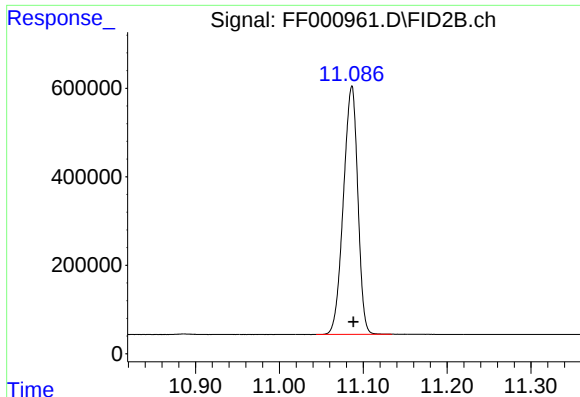

#6 N-OCTADECANE


R.T.: 11.086 min
Delta R.T.: -0.002 min
Response: 6694574
Conc: 49.03 ug/ml

Instrument :
FID_F
ClientSampleId :

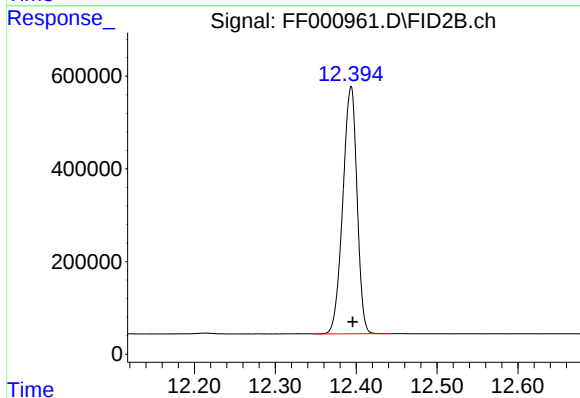


#7 N-EICOSANE

R.T.: 12.394 min
Delta R.T.: -0.002 min
Response: 6524787
Conc: 48.70 ug/ml

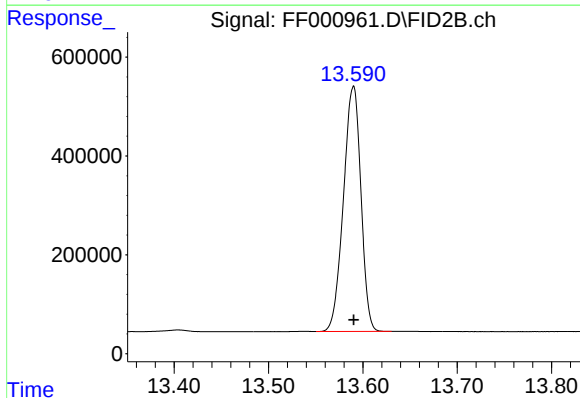


#8 N-DOCOSANE

R.T.: 13.590 min
Delta R.T.: 0.000 min
Response: 6391696
Conc: 48.34 ug/ml

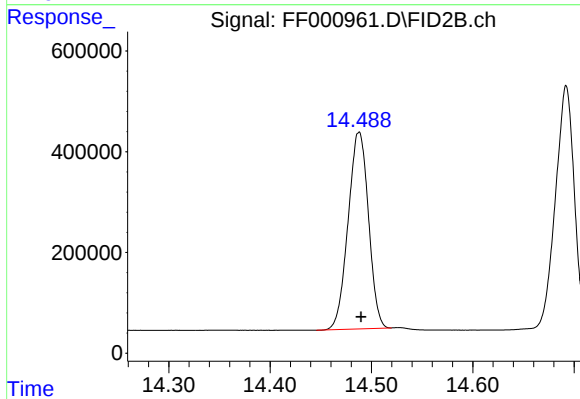

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.488 min
Delta R.T.: -0.002 min
Response: 5456885
Conc: 47.32 ug/ml

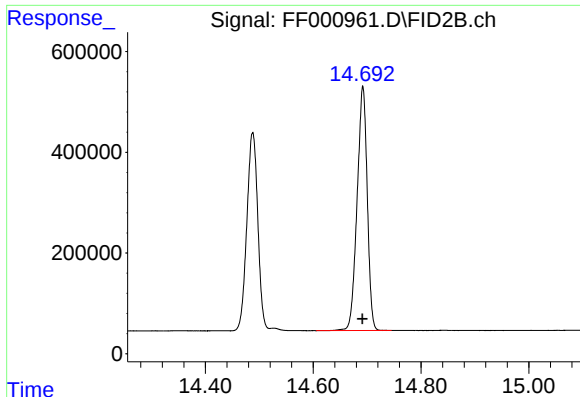

#10 N-TETRACOSANE


R.T.: 14.692 min
Delta R.T.: 0.000 min
Response: 6329508
Conc: 48.80 ug/ml

Instrument :
FID_F
ClientSampleId :

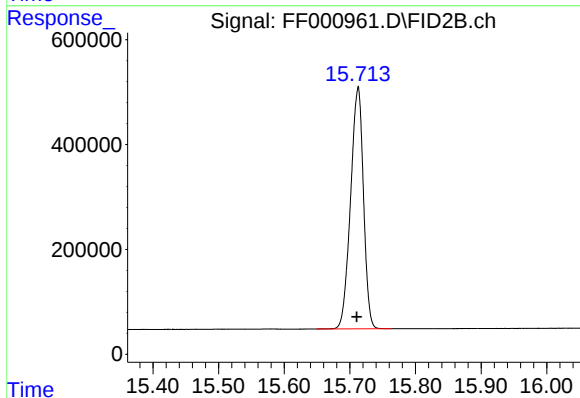

#11 N-HEXACOSANE

R.T.: 15.713 min
Delta R.T.: 0.002 min
Response: 6281842
Conc: 48.91 ug/ml

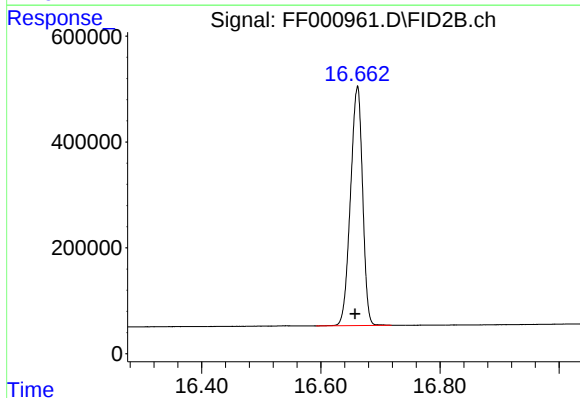

#12 N-OCTACOSANE

R.T.: 16.662 min
Delta R.T.: 0.004 min
Response: 6366270
Conc: 50.07 ug/ml