

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000962.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 16:16
 Operator : UA\AJ
 Sample : PB110281BS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB110281BS

Integration File: autoint1.e
 Quant Time: Jun 15 23:41:56 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.485	1832450	15.890 ug/ml
Target Compounds			
2) N-DECANE	4.246	2454607	17.518 ug/ml
3) N-DODECANE	6.259	2464349	17.583 ug/ml
4) N-TETRADECANE	8.048	2484697	17.846 ug/ml
5) N-HEXADECANE	9.644	2453634	17.796 ug/ml
6) N-OCTADECANE	11.083	2423723	17.749 ug/ml
7) N-EICOSANE	12.390	2366688	17.665 ug/ml
8) N-DOCOSANE	13.587	2323156	17.569 ug/ml
10) N-TETRACOSANE	14.688	2337651	18.022 ug/ml
11) N-HEXACOSANE	15.709	2266701	17.647 ug/ml
12) N-OCTACOSANE	16.658	2299756	18.086 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000962.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 16:16
Operator : UA\AJ
Sample : PB110281BS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB110281BS

Integration File: autoint1.e
Quant Time: Jun 15 23:41:56 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

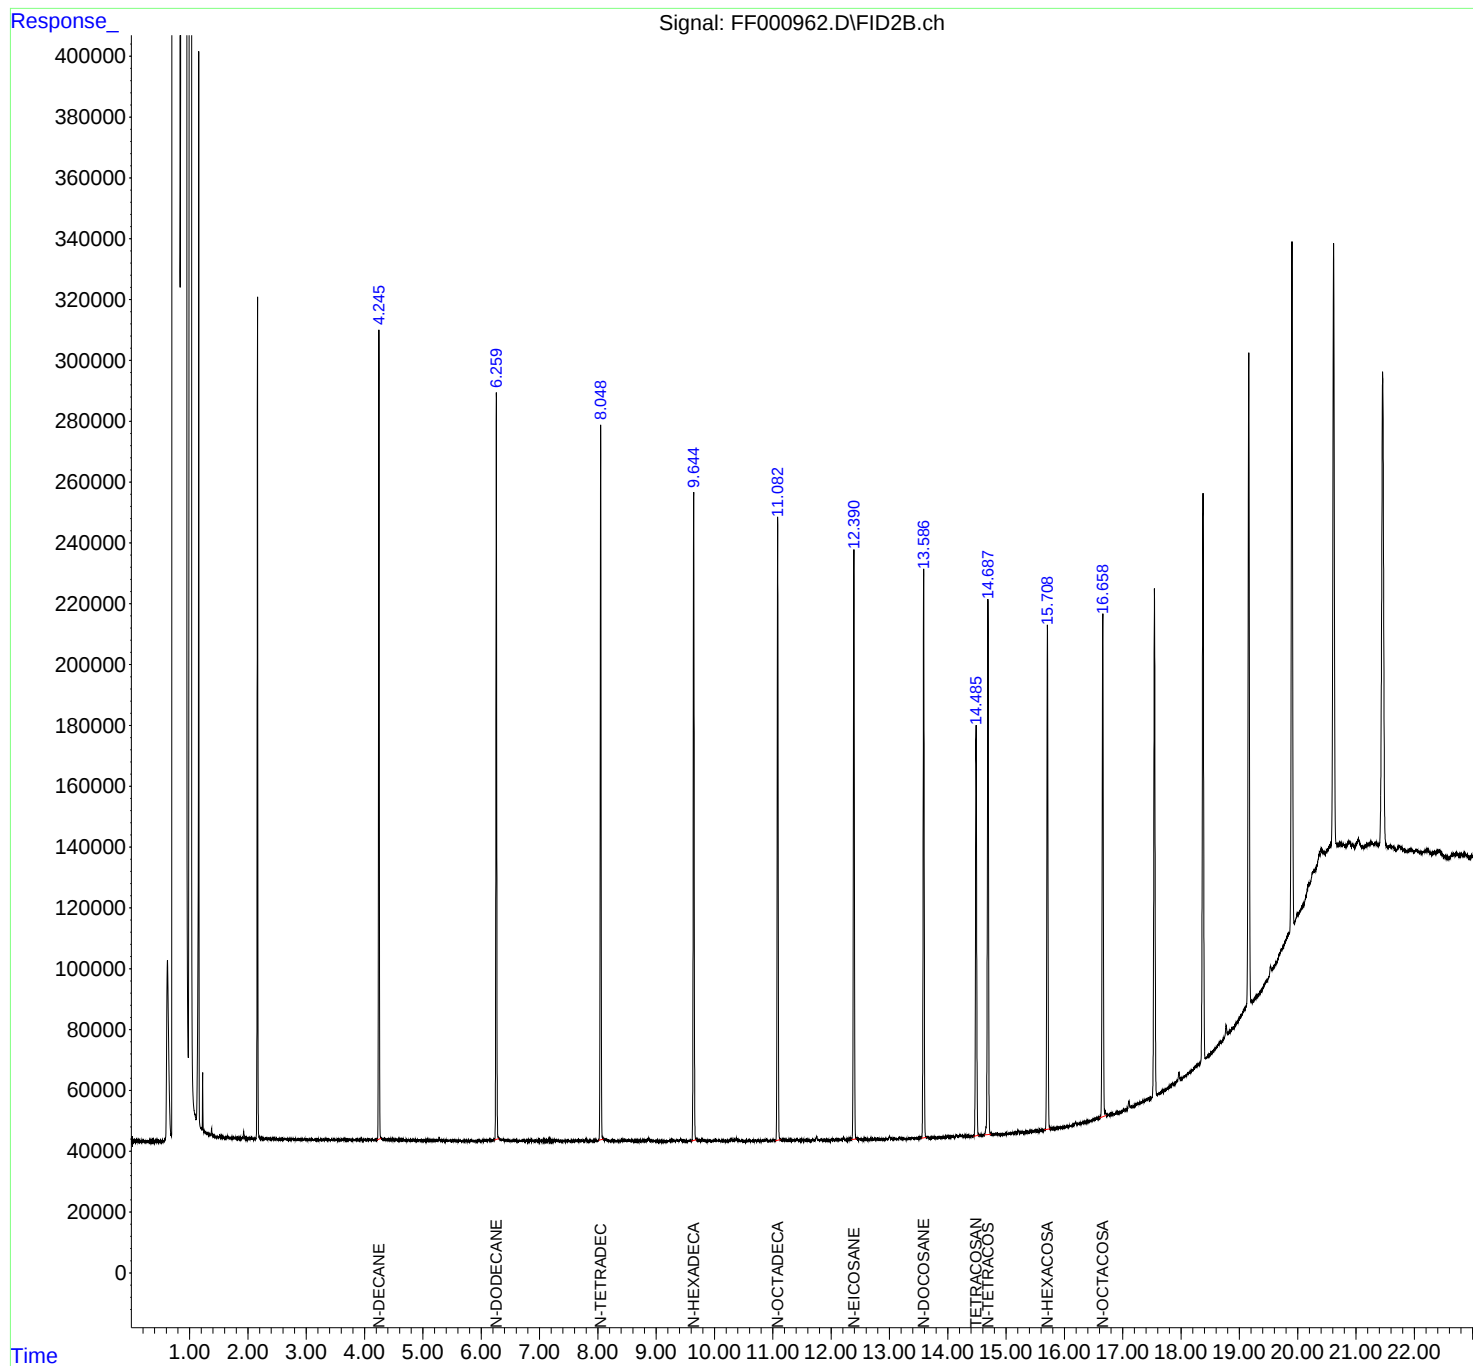


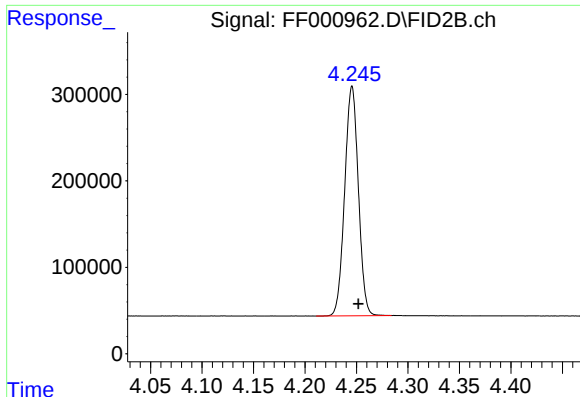

#2 N-DECANE


R.T.: 4.246 min
Delta R.T.: -0.006 min
Response: 2454607
Conc: 17.52 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110281BS

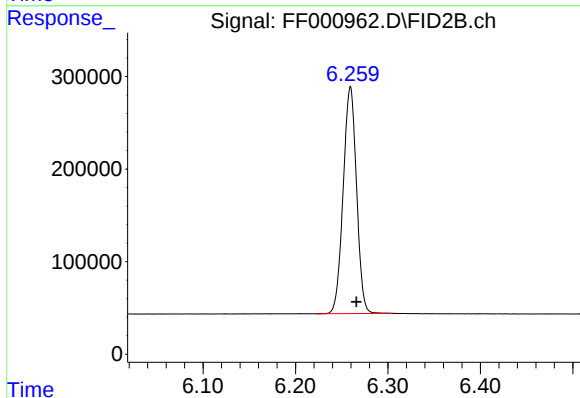


#3 N-DODECANE

R.T.: 6.259 min
Delta R.T.: -0.006 min
Response: 2464349
Conc: 17.58 ug/ml

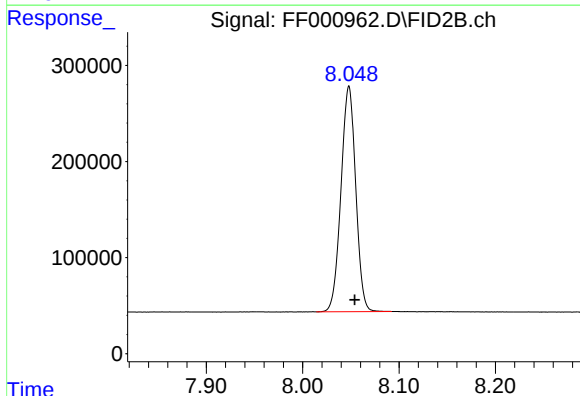


#4 N-TETRADECANE

R.T.: 8.048 min
Delta R.T.: -0.006 min
Response: 2484697
Conc: 17.85 ug/ml

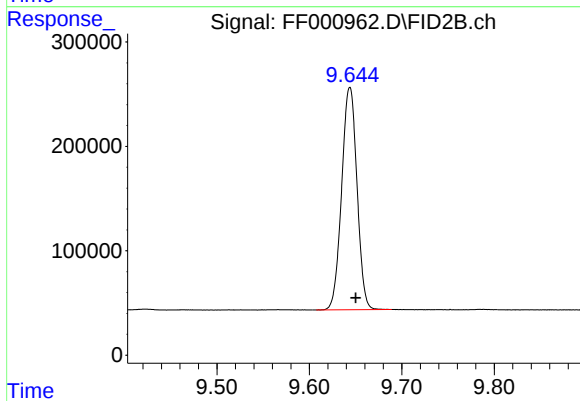

#5 N-HEXADECANE


R.T.: 9.644 min
Delta R.T.: -0.006 min
Response: 2453634
Conc: 17.80 ug/ml

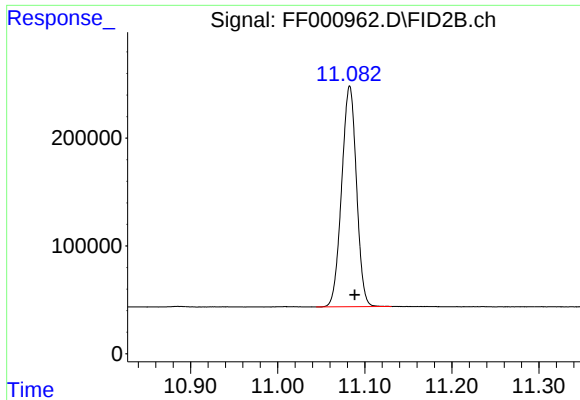

#6 N-OCTADECANE


R.T.: 11.083 min
Delta R.T.: -0.006 min
Response: 2423723
Conc: 17.75 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110281BS

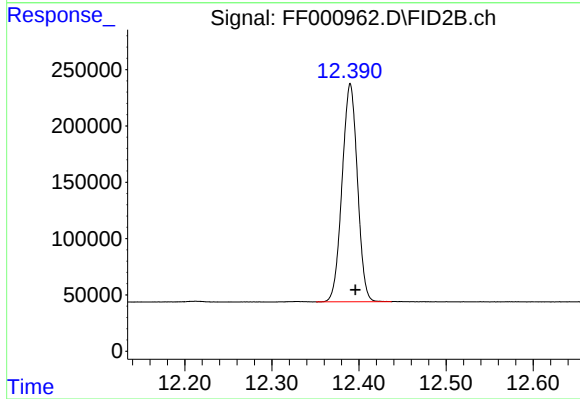


#7 N-EICOSANE

R.T.: 12.390 min
Delta R.T.: -0.006 min
Response: 2366688
Conc: 17.66 ug/ml

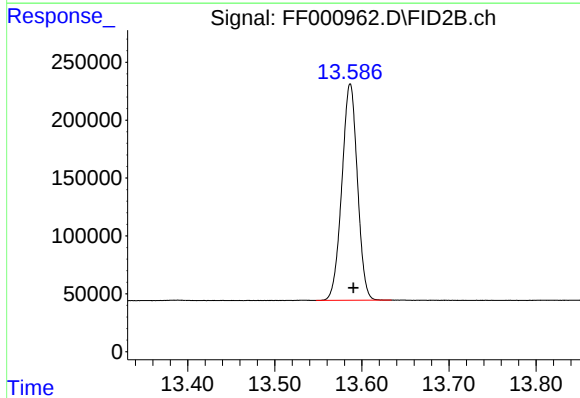


#8 N-DOCOSANE

R.T.: 13.587 min
Delta R.T.: -0.004 min
Response: 2323156
Conc: 17.57 ug/ml

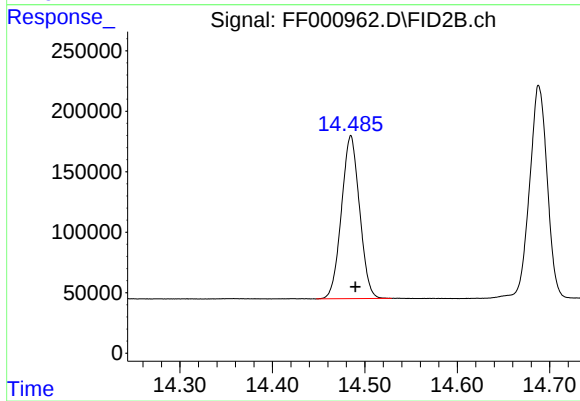

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.485 min
Delta R.T.: -0.005 min
Response: 1832450
Conc: 15.89 ug/ml

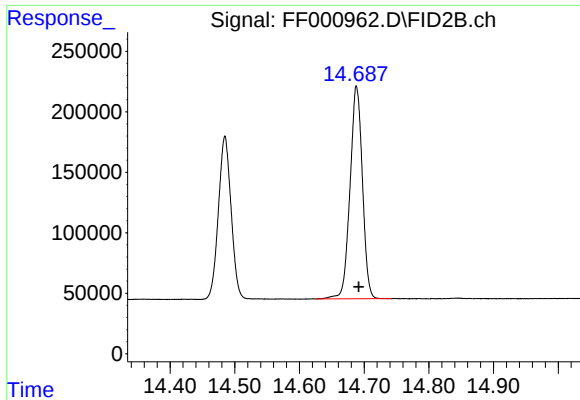

#10 N-TETRACOSANE


R.T.: 14.688 min
Delta R.T.: -0.003 min
Response: 2337651
Conc: 18.02 ug/ml

Instrument :
FID_F
ClientSampleId :
PB110281BS

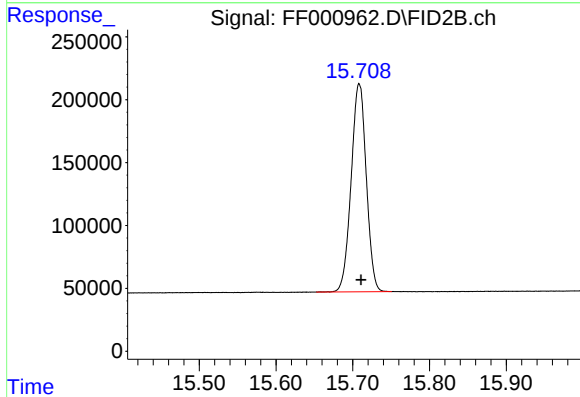

#11 N-HEXACOSANE

R.T.: 15.709 min
Delta R.T.: -0.002 min
Response: 2266701
Conc: 17.65 ug/ml

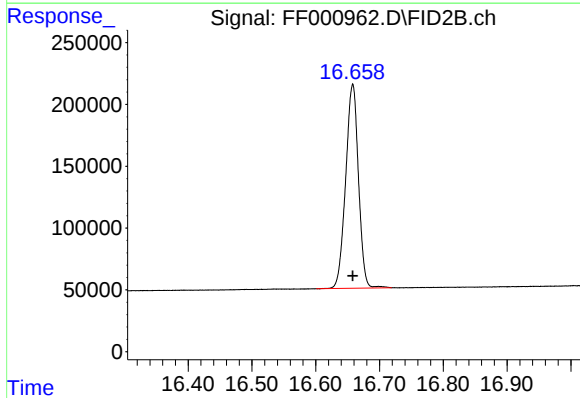

#12 N-OCTACOSANE

R.T.: 16.658 min
Delta R.T.: 0.000 min
Response: 2299756
Conc: 18.09 ug/ml