

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000963.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 16:46
 Operator : UA\AJ
 Sample : PB110281BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 15 23:42:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.484	1806776	15.667 ug/ml
Target Compounds			
2) N-DECANE	4.246	2373533	16.940 ug/ml
3) N-DODECANE	6.259	2369144	16.904 ug/ml
4) N-TETRADECANE	8.047	2388102	17.152 ug/ml
5) N-HEXADECANE	9.644	2367692	17.172 ug/ml
6) N-OCTADECANE	11.082	2353702	17.236 ug/ml
7) N-EICOSANE	12.389	2307176	17.221 ug/ml
8) N-DOCOSANE	13.586	2270131	17.168 ug/ml
10) N-TETRACOSANE	14.688	2284149	17.610 ug/ml
11) N-HEXACOSANE	15.707	2219690	17.281 ug/ml
12) N-OCTACOSANE	16.656	2238176	17.601 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000963.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 16:46
Operator : UA\AJ
Sample : PB110281BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 15 23:42:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

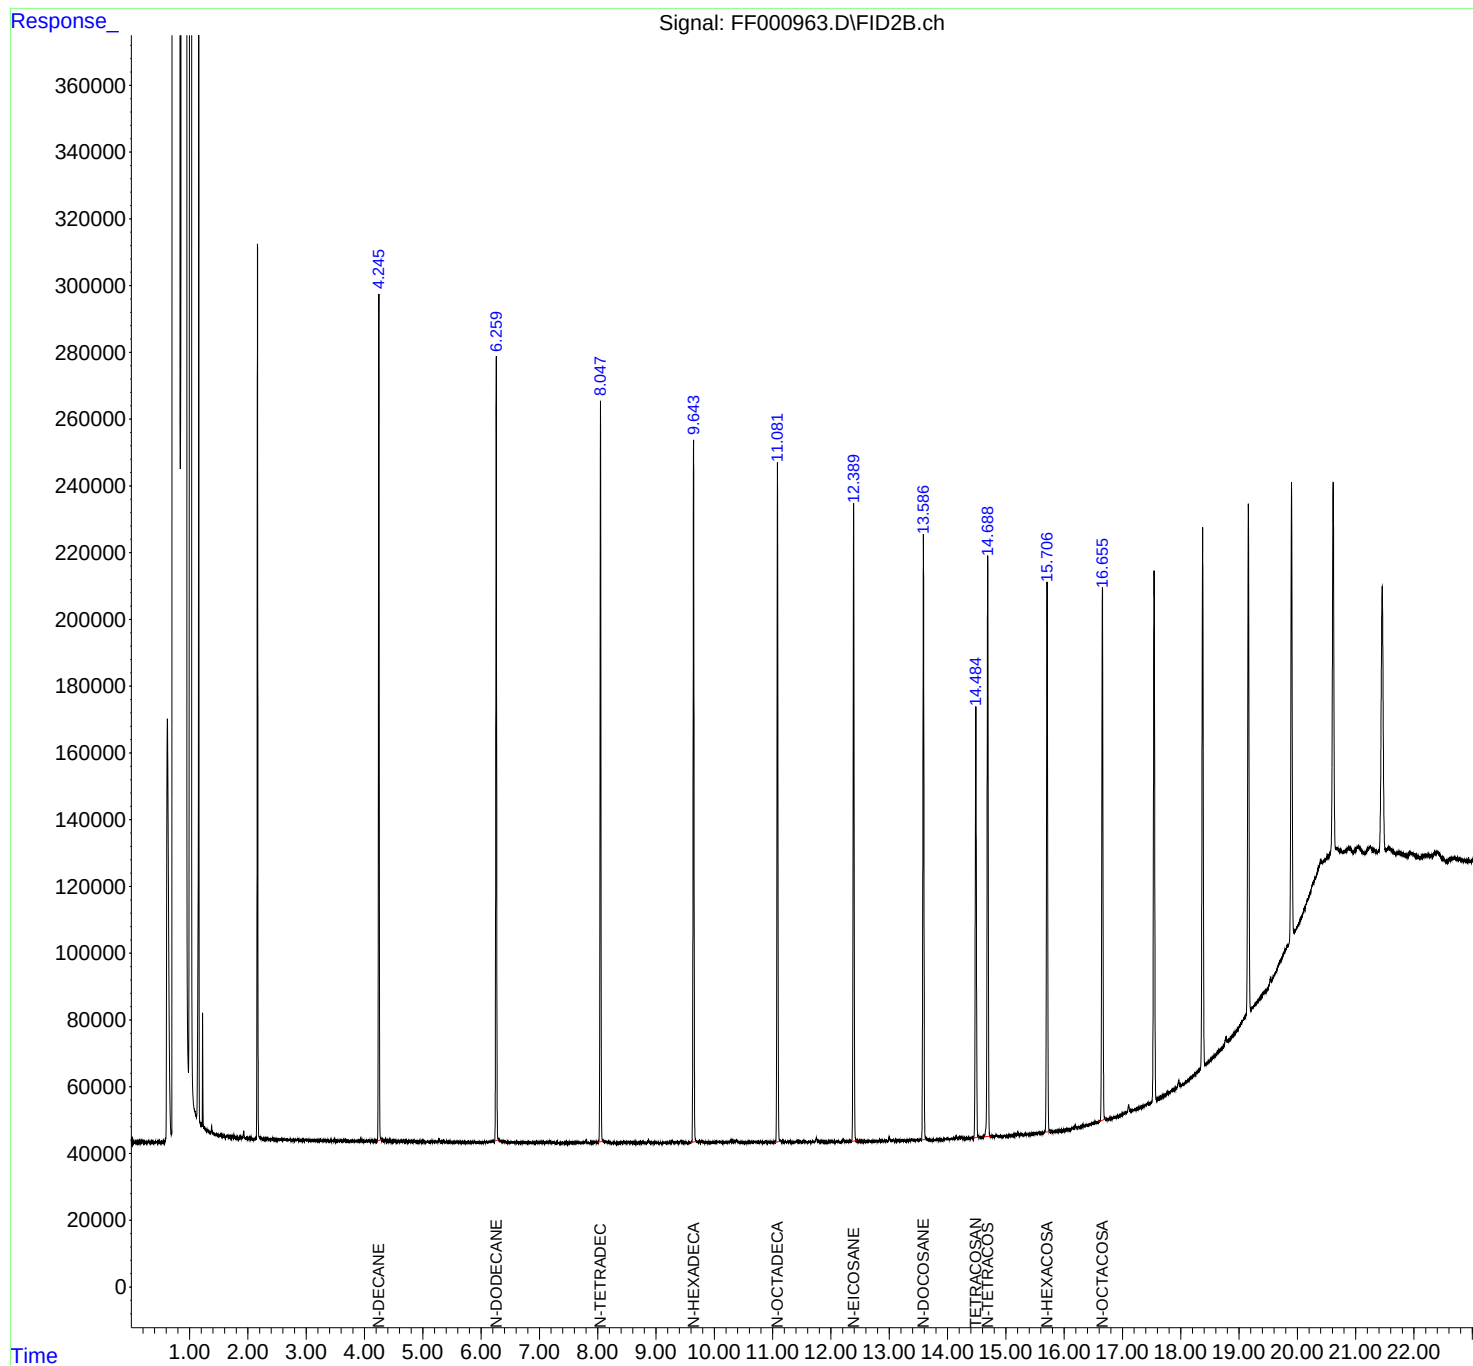


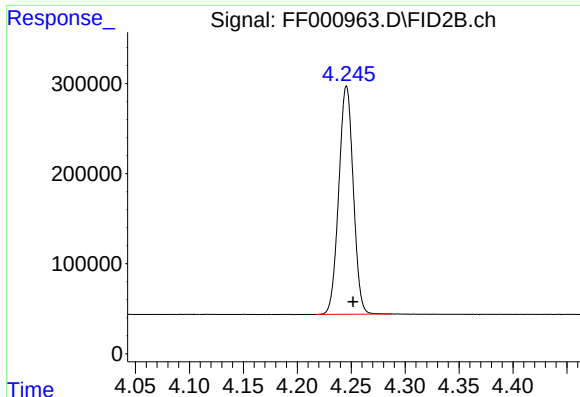

#2 N-DECANE


R.T.: 4.246 min
Delta R.T.: -0.006 min
Response: 2373533
Conc: 16.94 ug/ml

Instrument :
FID_F
ClientSampleId :

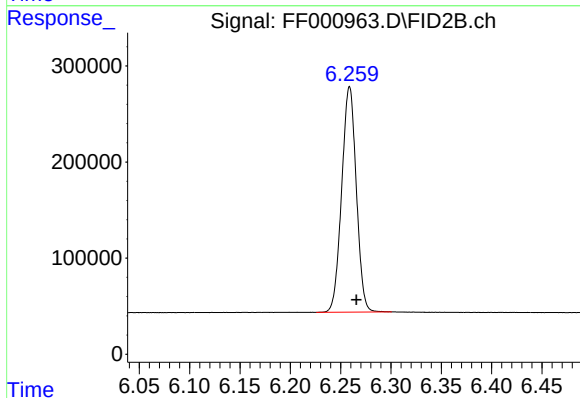


#3 N-DODECANE

R.T.: 6.259 min
Delta R.T.: -0.007 min
Response: 2369144
Conc: 16.90 ug/ml

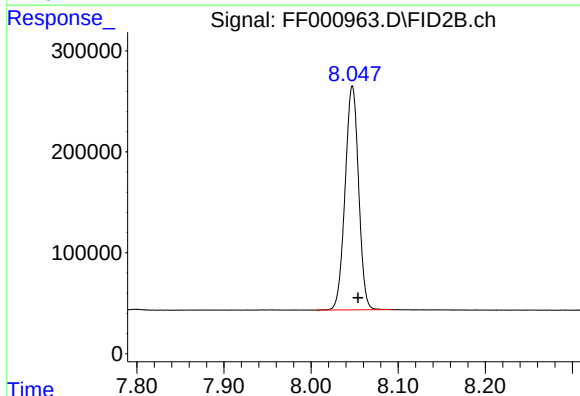


#4 N-TETRADECANE

R.T.: 8.047 min
Delta R.T.: -0.007 min
Response: 2388102
Conc: 17.15 ug/ml

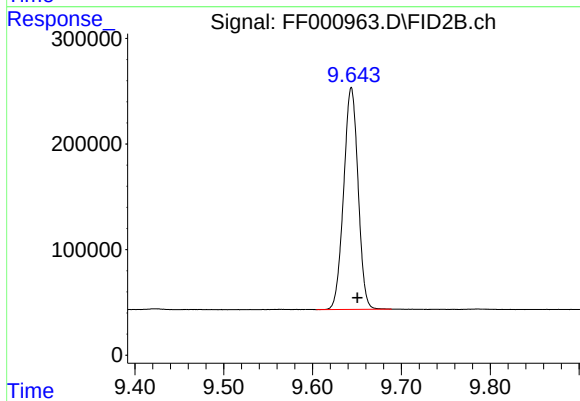

#5 N-HEXADECANE


R.T.: 9.644 min
Delta R.T.: -0.007 min
Response: 2367692
Conc: 17.17 ug/ml

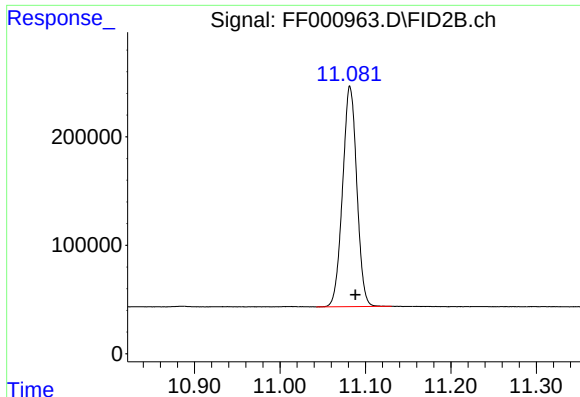

#6 N-OCTADECANE


R.T.: 11.082 min
Delta R.T.: -0.006 min
Response: 2353702
Conc: 17.24 ug/ml

Instrument :
FID_F
ClientSampleId :

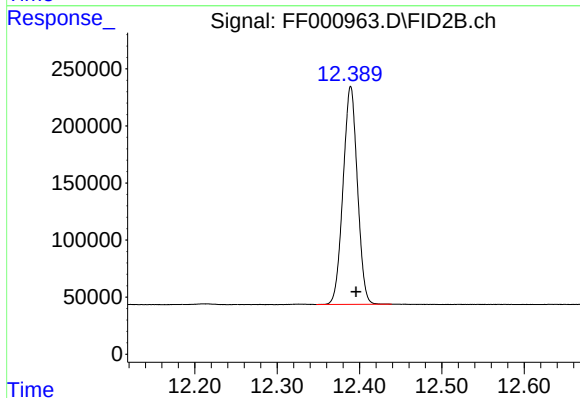


#7 N-EICOSANE

R.T.: 12.389 min
Delta R.T.: -0.007 min
Response: 2307176
Conc: 17.22 ug/ml

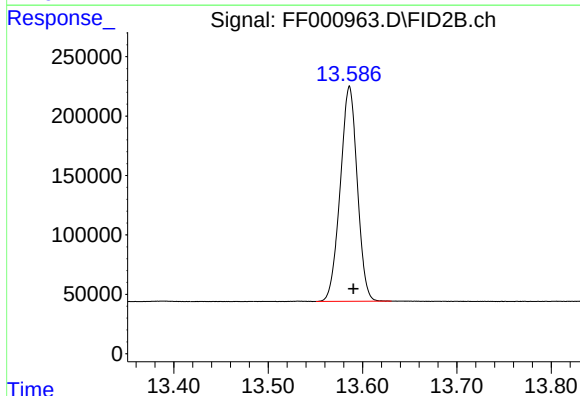


#8 N-DOCOSANE

R.T.: 13.586 min
Delta R.T.: -0.004 min
Response: 2270131
Conc: 17.17 ug/ml

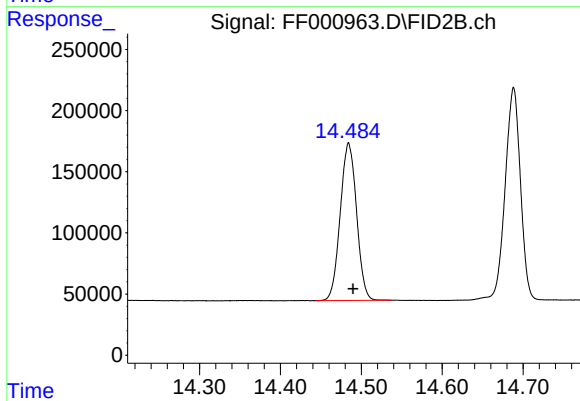

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.484 min
Delta R.T.: -0.005 min
Response: 1806776
Conc: 15.67 ug/ml

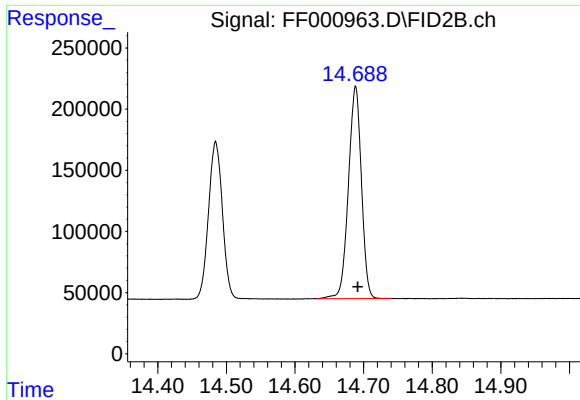

#10 N-TETRACOSANE


R.T.: 14.688 min
Delta R.T.: -0.003 min
Response: 2284149
Conc: 17.61 ug/ml

Instrument :
FID_F
ClientSampleId :

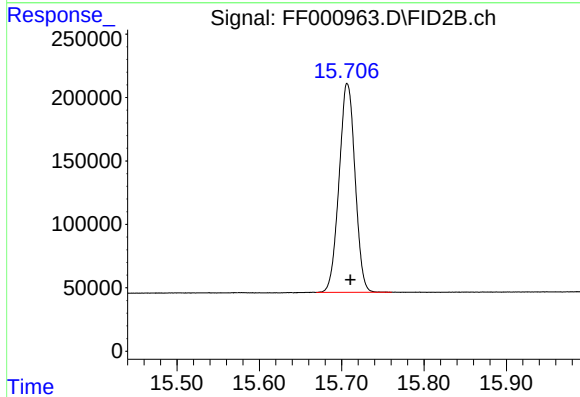

#11 N-HEXACOSANE

R.T.: 15.707 min
Delta R.T.: -0.004 min
Response: 2219690
Conc: 17.28 ug/ml

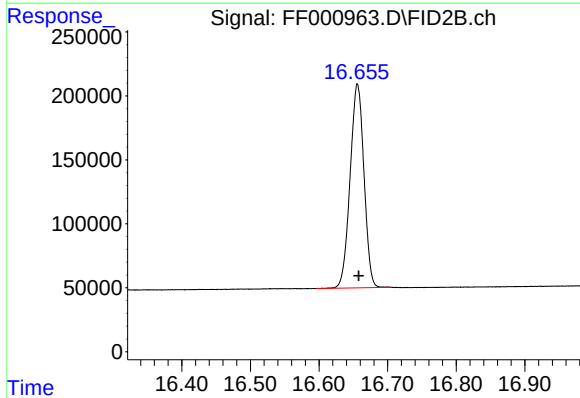

#12 N-OCTACOSANE

R.T.: 16.656 min
Delta R.T.: -0.002 min
Response: 2238176
Conc: 17.60 ug/ml