

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
 Data File : FF000965.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2018 17:46
 Operator : UA\AJ
 Sample : J3518-04MS
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EPE-106-7(70-72)MS

Integration File: autoint1.e
 Quant Time: Jun 15 23:42:08 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.485	2075573	17.998 ug/ml
Target Compounds			
2) N-DECANE	4.245	2169451	15.483 ug/ml
3) N-DODECANE	6.258	2282878	16.289 ug/ml
4) N-TETRADECANE	8.047	2427132	17.432 ug/ml
5) N-HEXADECANE	9.643	2615407	18.969 ug/ml
6) N-OCTADECANE	11.082	2538747	18.592 ug/ml
7) N-EICOSANE	12.390	2402868	17.935 ug/ml
8) N-DOCOSANE	13.586	2402531	18.170 ug/ml
10) N-TETRACOSANE	14.687	2379634	18.346 ug/ml
11) N-HEXACOSANE	15.707	2343944	18.249 ug/ml
12) N-OCTACOSANE	16.655	2497070	19.637 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061518\
Data File : FF000965.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2018 17:46
Operator : UA\AJ
Sample : J3518-04MS
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EPE-106-7(70-72)MS

Integration File: autoint1.e
Quant Time: Jun 15 23:42:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

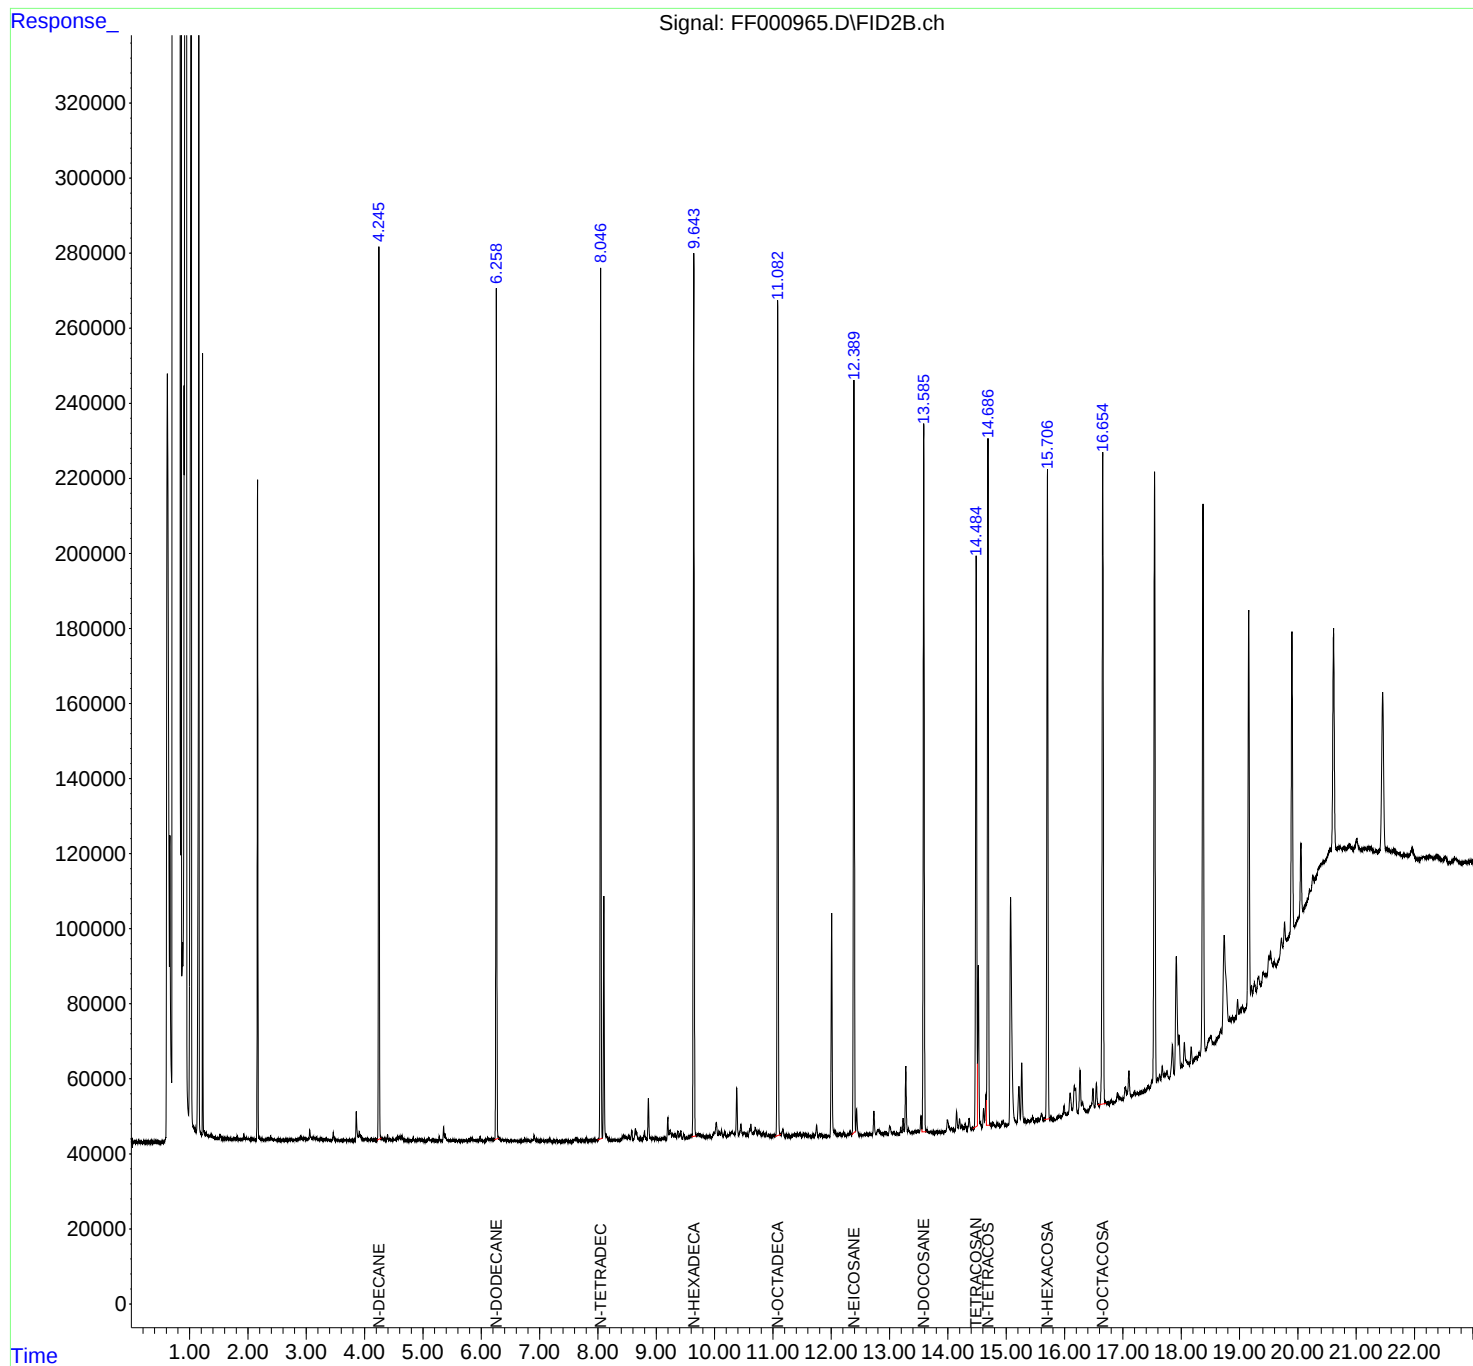


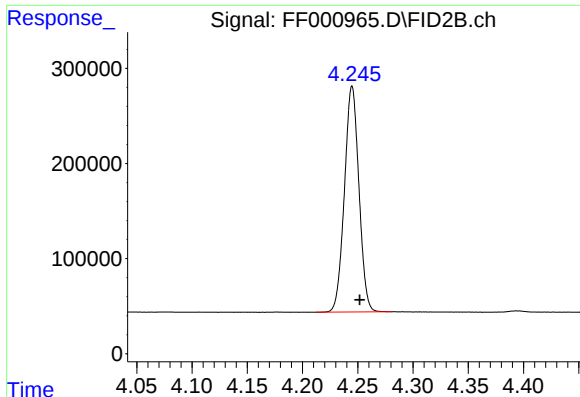

#2 N-DECANE


R.T.: 4.245 min
Delta R.T.: -0.007 min
Response: 2169451
Conc: 15.48 ug/ml

Instrument :
FID_F
ClientSampleId :
EPE-106-7(70-72)MS

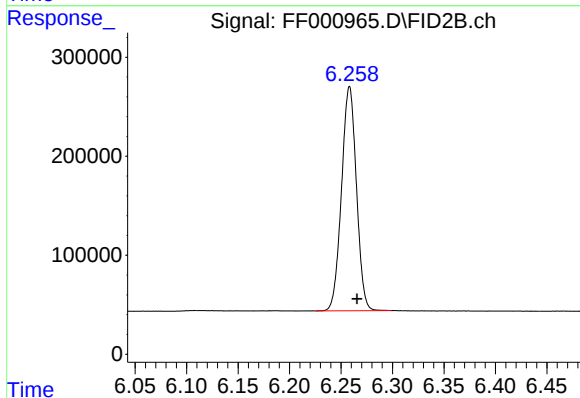


#3 N-DODECANE

R.T.: 6.258 min
Delta R.T.: -0.007 min
Response: 2282878
Conc: 16.29 ug/ml

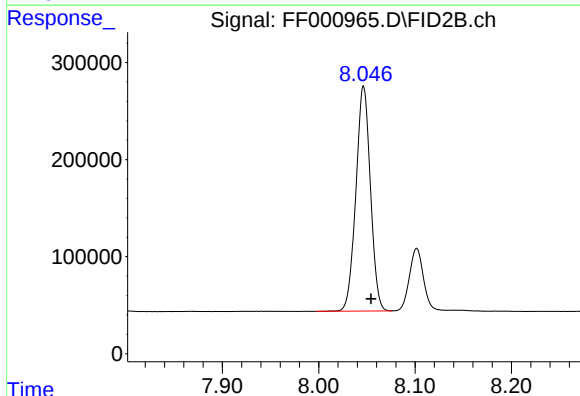


#4 N-TETRADECANE

R.T.: 8.047 min
Delta R.T.: -0.008 min
Response: 2427132
Conc: 17.43 ug/ml

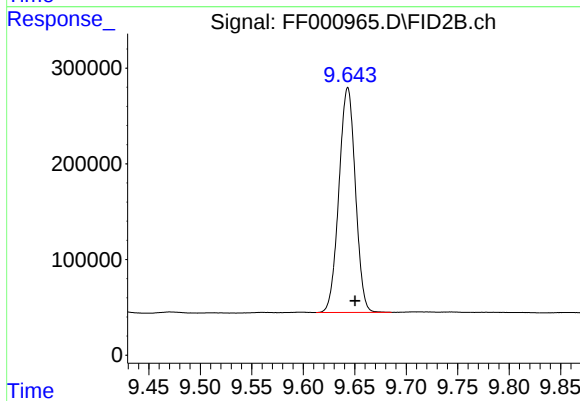

#5 N-HEXADECANE


R.T.: 9.643 min
Delta R.T.: -0.007 min
Response: 2615407
Conc: 18.97 ug/ml

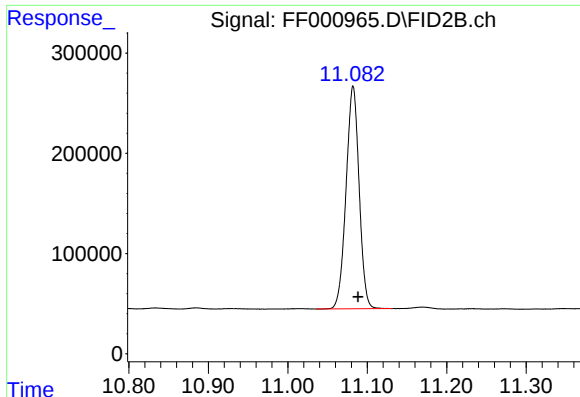

#6 N-OCTADECANE


R.T.: 11.082 min
Delta R.T.: -0.006 min
Response: 2538747
Conc: 18.59 ug/ml

Instrument :
FID_F
ClientSampleId :
EPE-106-7(70-72)MS

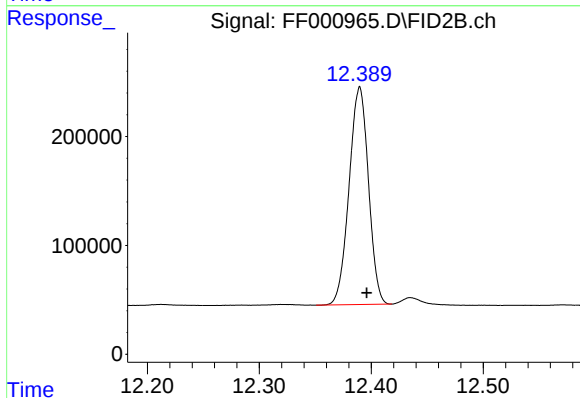


#7 N-EICOSANE

R.T.: 12.390 min
Delta R.T.: -0.006 min
Response: 2402868
Conc: 17.93 ug/ml

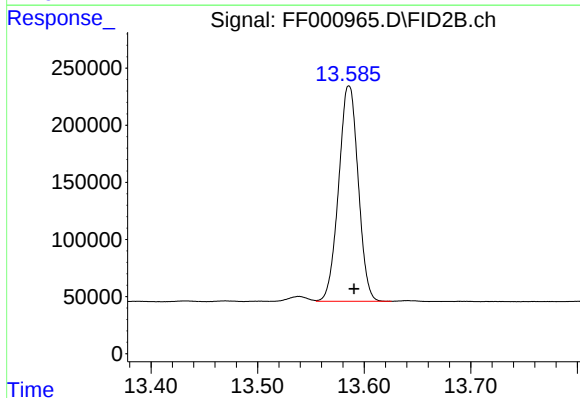


#8 N-DOCOSANE

R.T.: 13.586 min
Delta R.T.: -0.005 min
Response: 2402531
Conc: 18.17 ug/ml

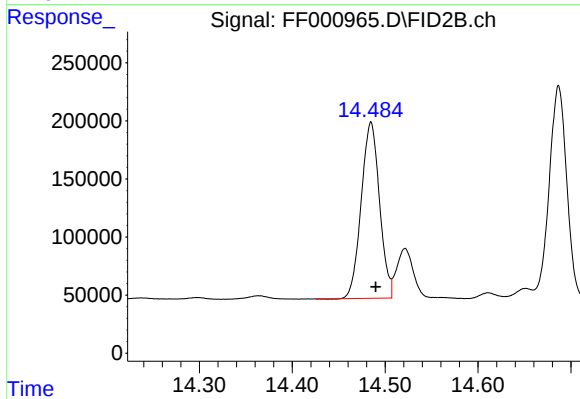

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.485 min
Delta R.T.: -0.005 min
Response: 2075573
Conc: 18.00 ug/ml

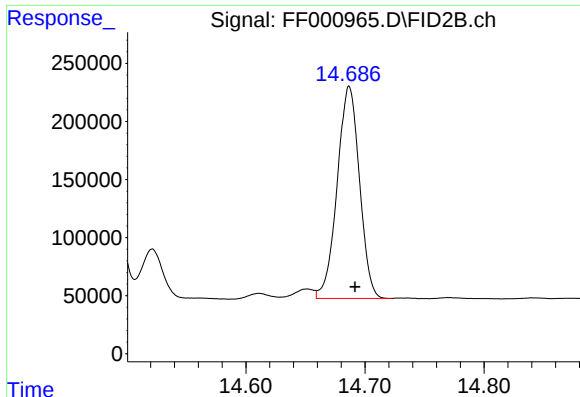

#10 N-TETRACOSANE


R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 2379634
Conc: 18.35 ug/ml

Instrument :
FID_F
ClientSampleId :
EPE-106-7(70-72)MS

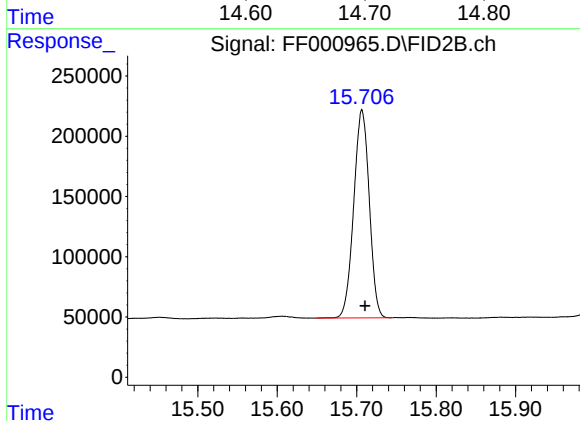

#11 N-HEXACOSANE

R.T.: 15.707 min
Delta R.T.: -0.004 min
Response: 2343944
Conc: 18.25 ug/ml

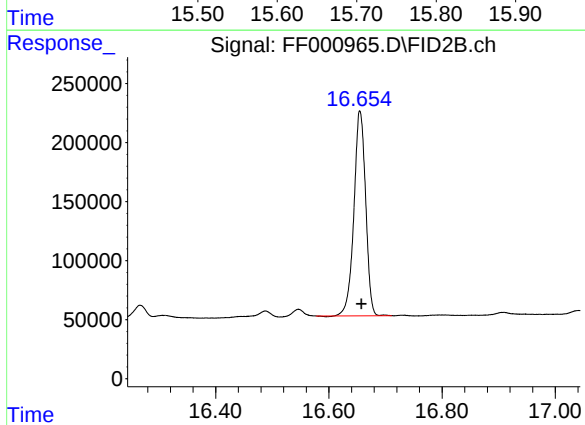

#12 N-OCTACOSANE

R.T.: 16.655 min
Delta R.T.: -0.003 min
Response: 2497070
Conc: 19.64 ug/ml