

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008629.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 15:53
 Operator : DD\AJ
 Sample : PB137117BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 02:02:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	1898815	18.021 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.941	121345	0.990 ug/ml
16) N-HEXATRIACONTANE	20.190	181412	1.636 ug/ml
18) N-TETRACONTANE	21.862	284594	2.694 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008629.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 15:53
Operator : DD\AJ
Sample : PB137117BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:02:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

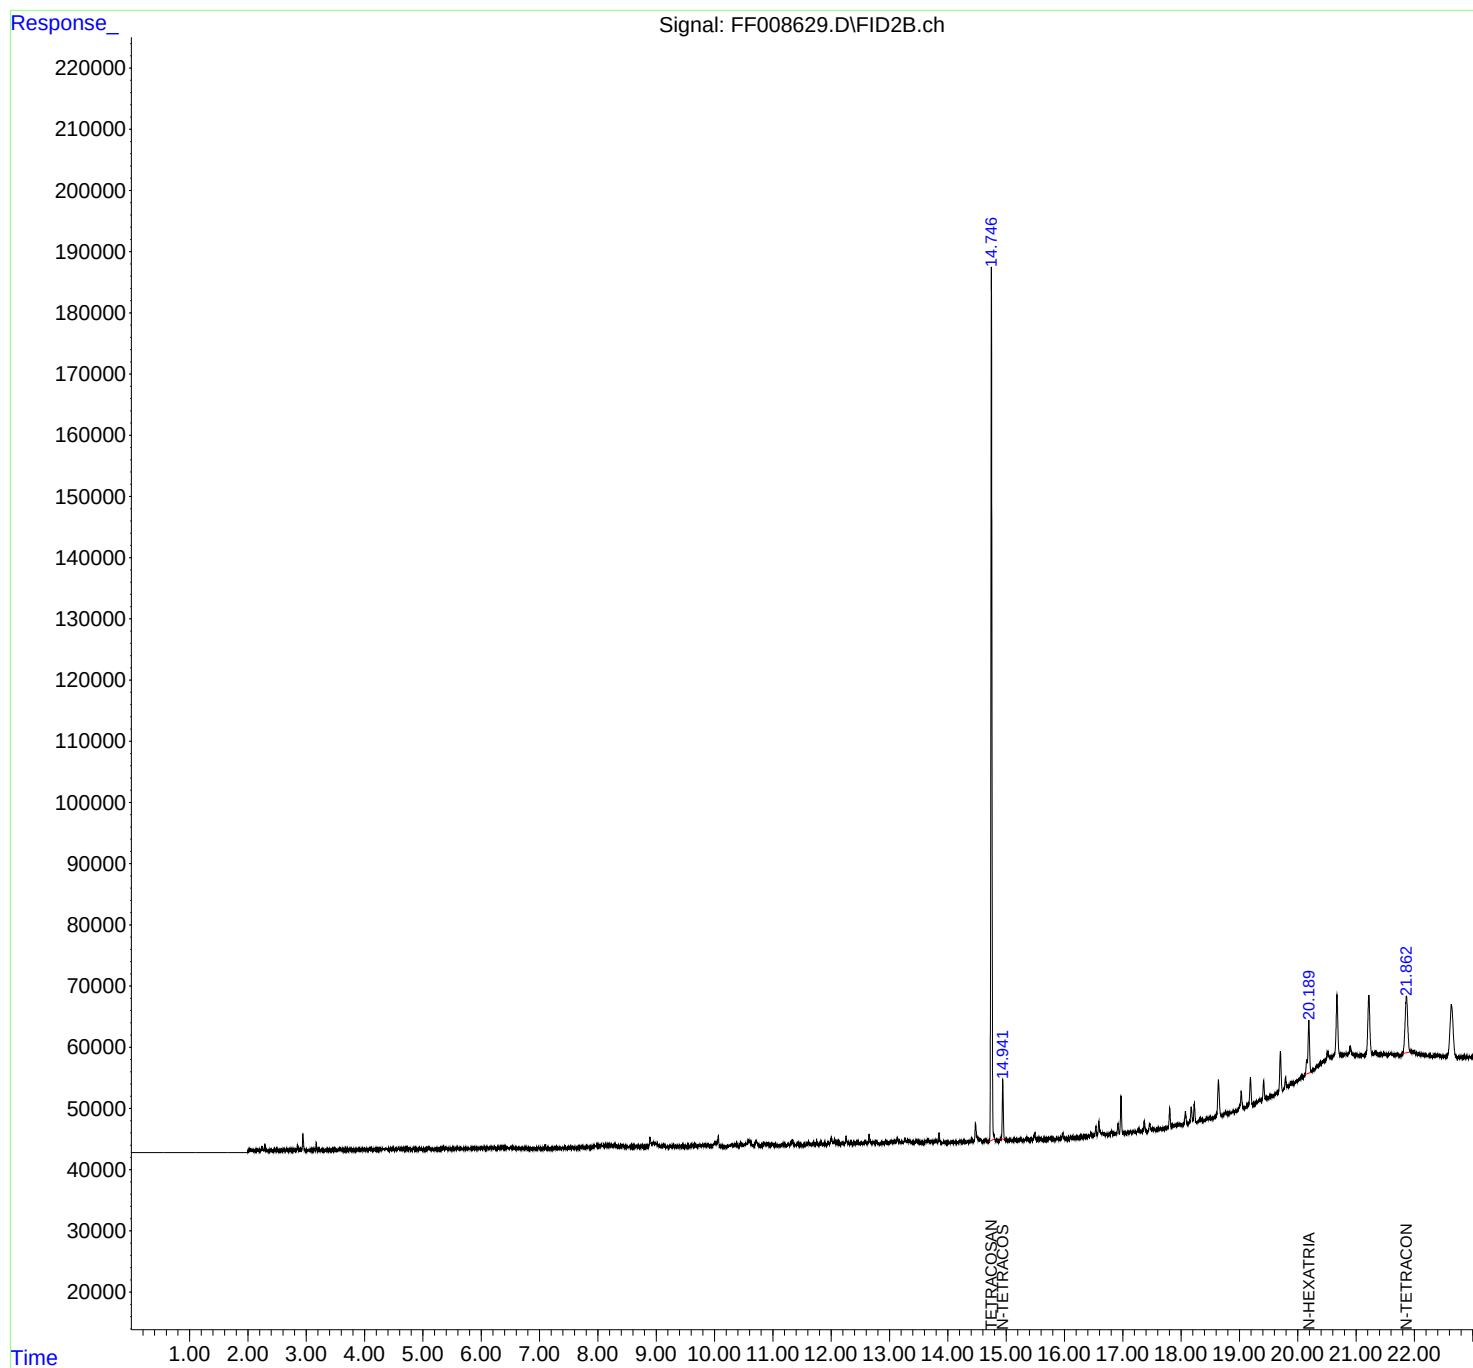


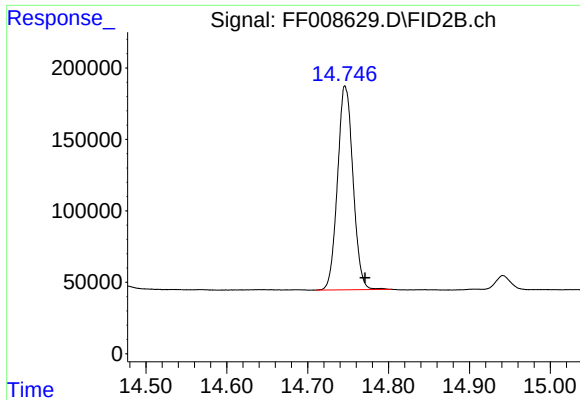

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.746 min
Delta R.T.: -0.025 min
Response: 1898815
Conc: 18.02 ug/ml

Instrument :
FID_F
ClientSampleId :

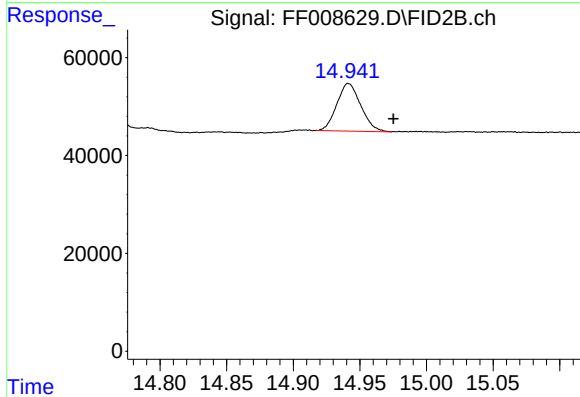


#10 N-TETRACOSANE

R.T.: 14.941 min
Delta R.T.: -0.034 min
Response: 121345
Conc: 0.99 ug/ml

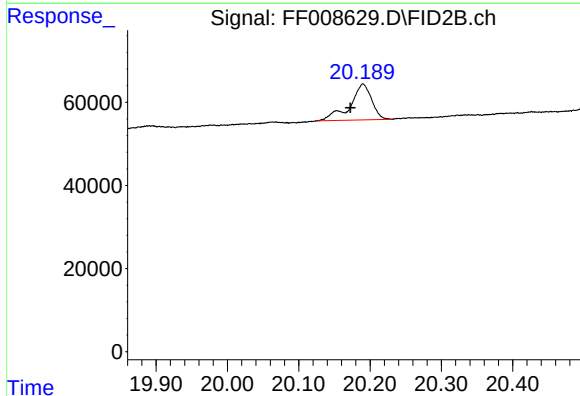

#16 N-HEXATRIACONTANE

R.T.: 20.190 min
Delta R.T.: 0.018 min
Response: 181412
Conc: 1.64 ug/ml

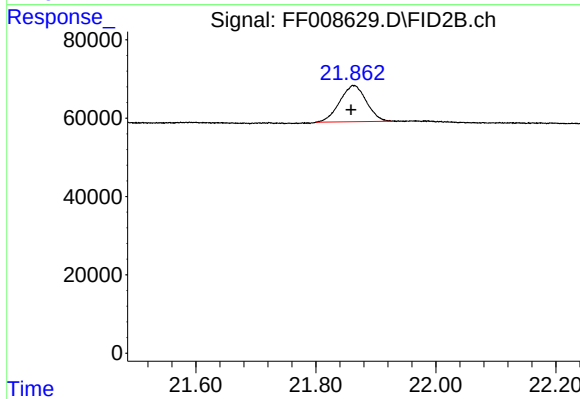

#18 N-TETRACONTANE

R.T.: 21.862 min
Delta R.T.: 0.003 min
Response: 284594
Conc: 2.69 ug/ml