

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008631.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 16:56
 Operator : DD\AJ
 Sample : M2672-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 02:02:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	2120968	20.129 ug/ml
Target Compounds			
3) N-DODECANE	6.532	202759	1.625 ug/ml
7) N-EICOSANE	12.654	78745	0.617 ug/ml
8) N-DOCOSANE	13.850	116119	0.924 ug/ml
10) N-TETRACOSANE	14.945	364742	2.977 ug/ml
11) N-HEXACOSANE	15.972	73843	0.616 ug/ml
14) N-DOTRIACONTANE	18.634	122083	1.014 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008631.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 16:56
Operator : DD\AJ
Sample : M2672-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:02:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

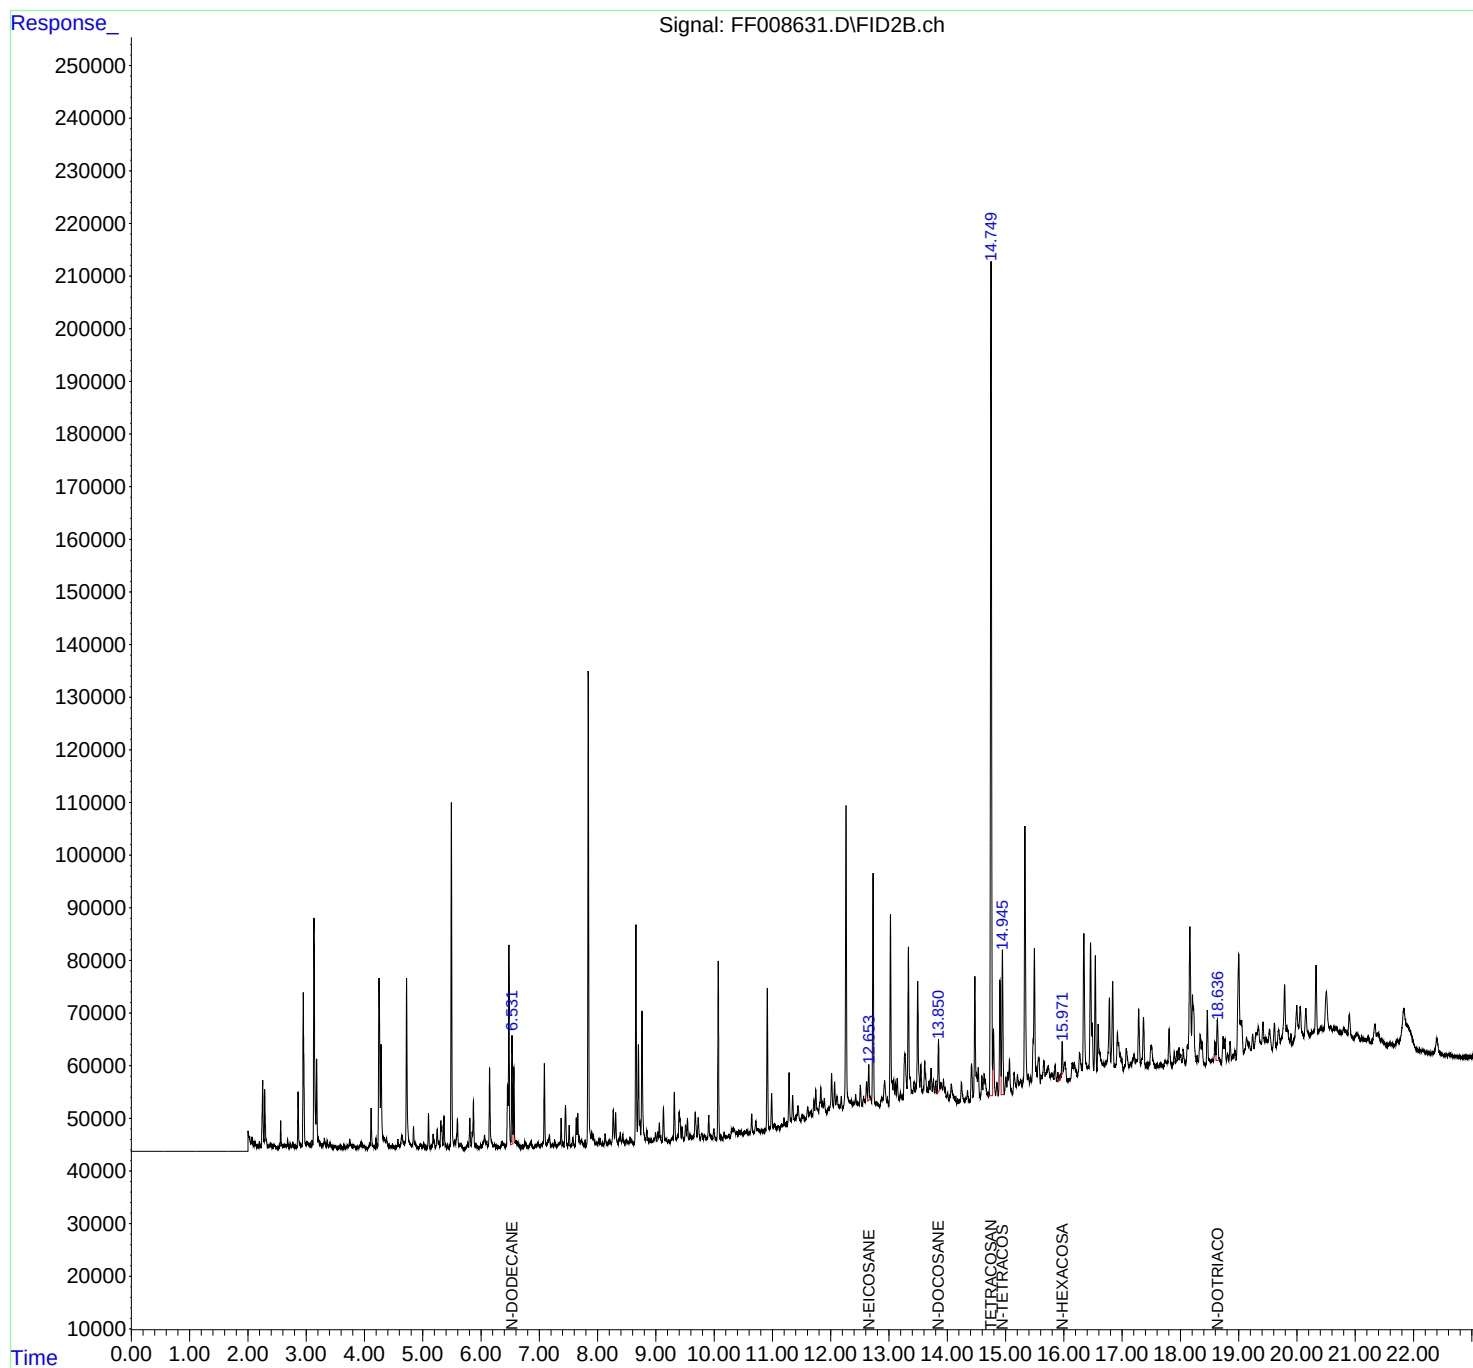


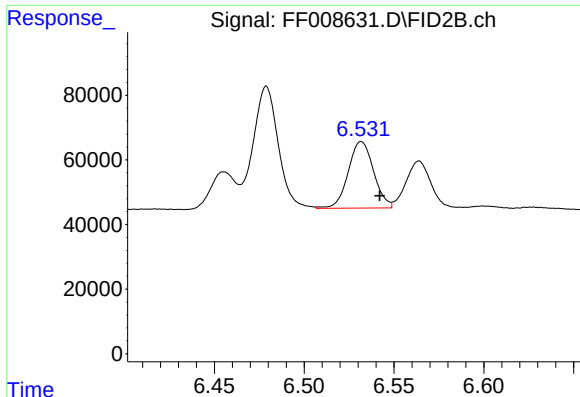

#3 N-DODECANE


R.T.: 6.532 min
Delta R.T.: -0.010 min
Response: 202759
Conc: 1.63 ug/ml

Instrument :
FID_F
ClientSampleId :

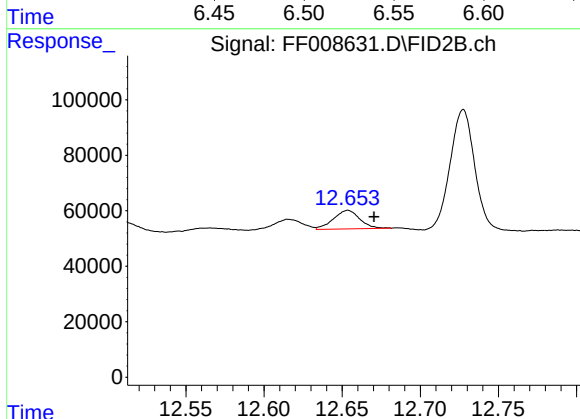


#7 N-EICOSANE

R.T.: 12.654 min
Delta R.T.: -0.017 min
Response: 78745
Conc: 0.62 ug/ml

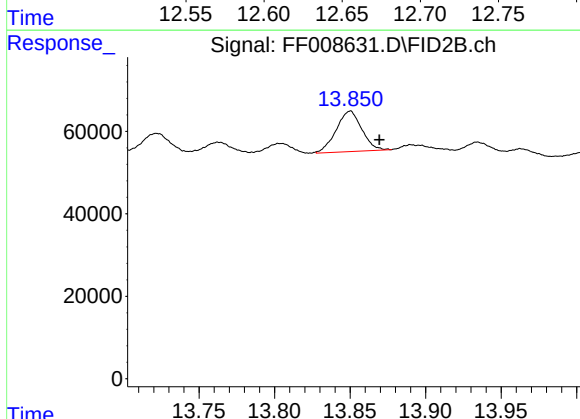


#8 N-DOCOSANE

R.T.: 13.850 min
Delta R.T.: -0.019 min
Response: 116119
Conc: 0.92 ug/ml

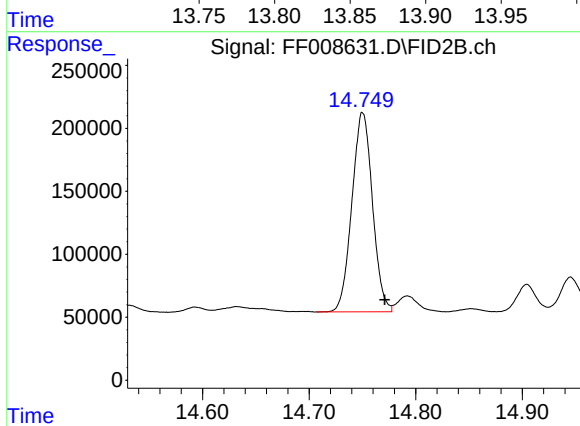

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.750 min
Delta R.T.: -0.021 min
Response: 2120968
Conc: 20.13 ug/ml

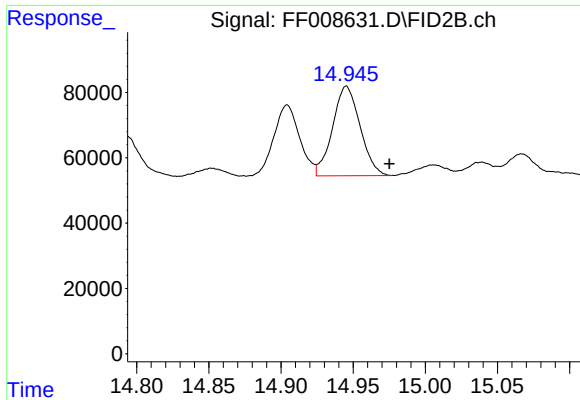

#10 N-TETRACOSANE


R.T.: 14.945 min
Delta R.T.: -0.030 min
Response: 364742
Conc: 2.98 ug/ml

Instrument :
FID_F
ClientSampleId :

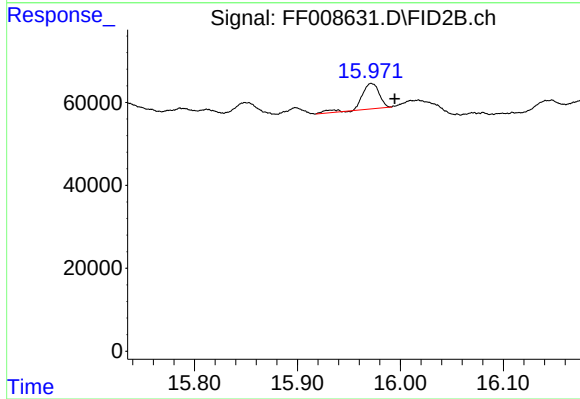

#11 N-HEXACOSANE

R.T.: 15.972 min
Delta R.T.: -0.023 min
Response: 73843
Conc: 0.62 ug/ml

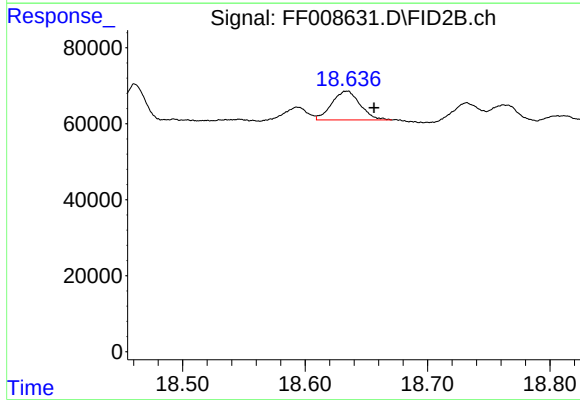

#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: -0.022 min
Response: 122083
Conc: 1.01 ug/ml