

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008636.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 19:35
 Operator : DD\AJ
 Sample : M2672-06
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 02:02:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.751	1192234	11.315 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.952	97626	0.797 ug/ml
11) N-HEXACOSANE	15.972	92709	0.773 ug/ml
12) N-OCTACOSANE	16.921	88787	0.748 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008636.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 19:35
Operator : DD\AJ
Sample : M2672-06
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:02:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

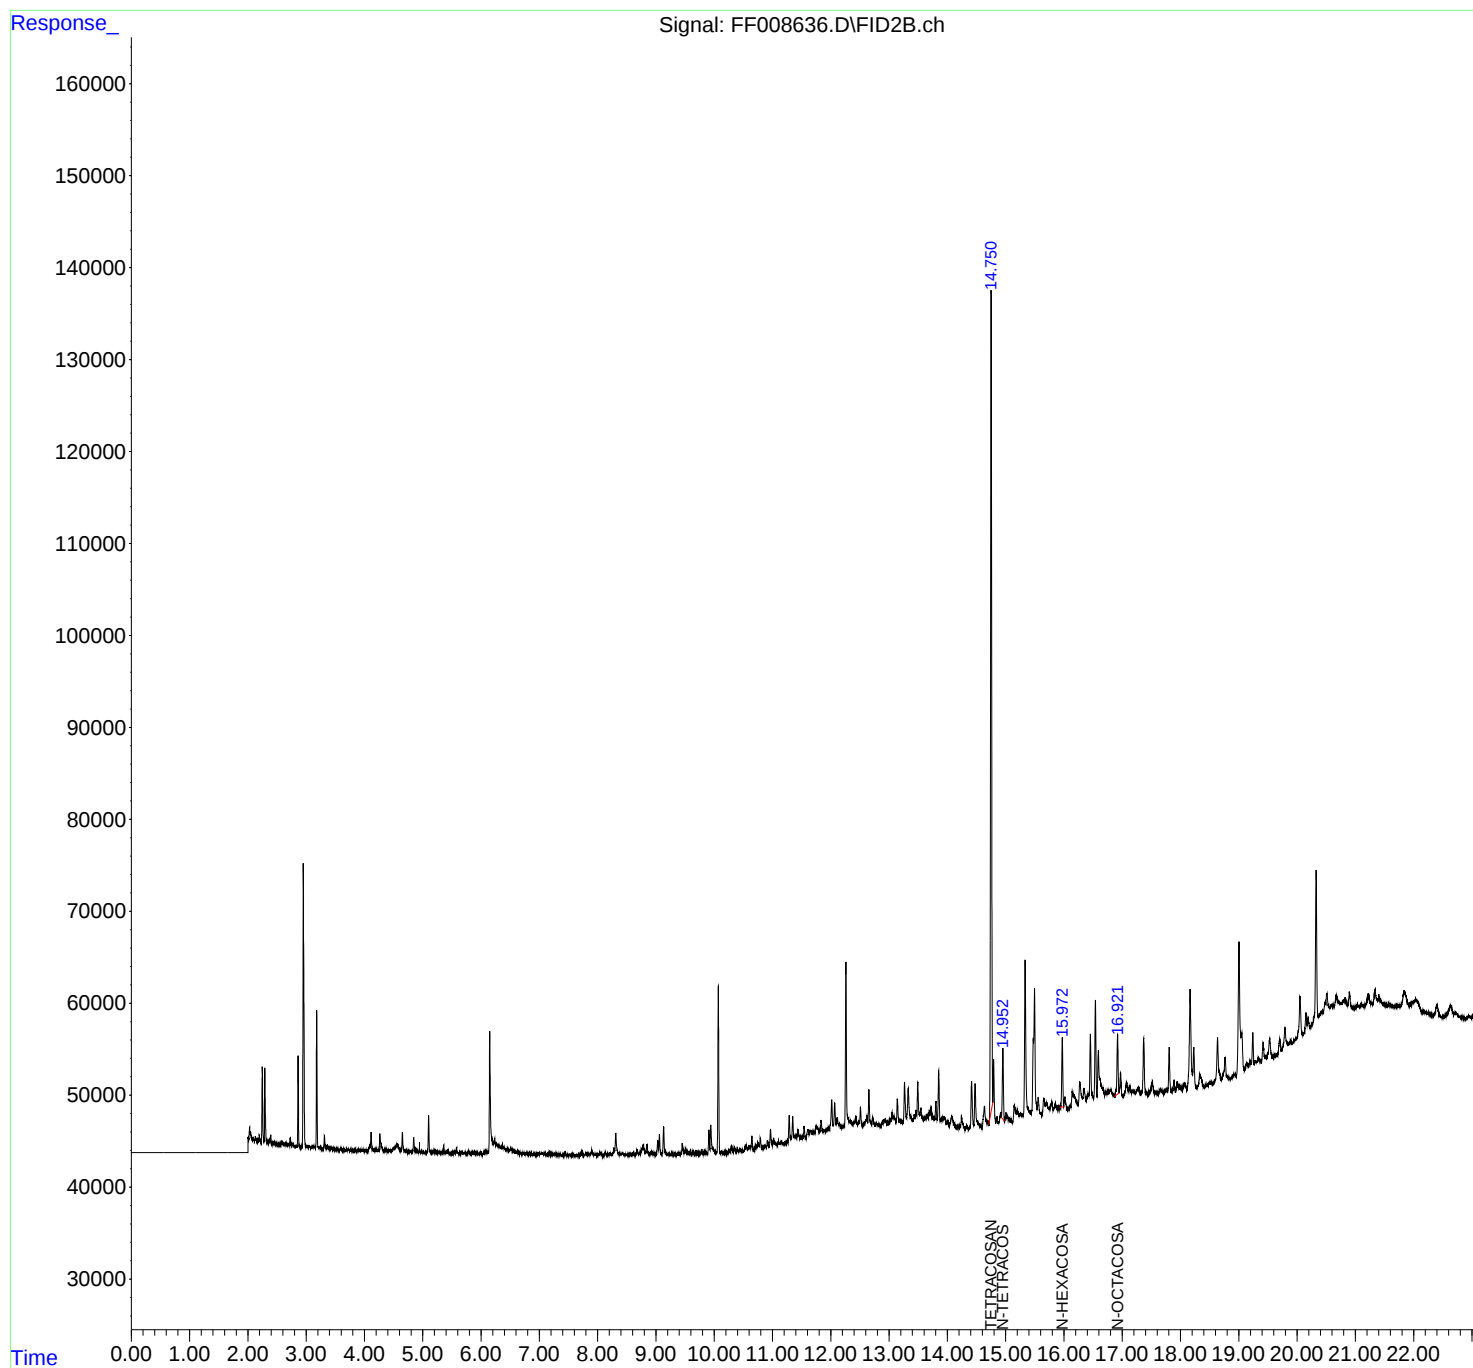


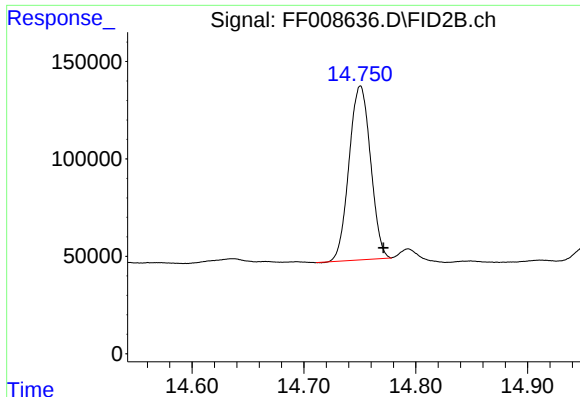

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.751 min
Delta R.T.: -0.020 min
Response: 1192234
Conc: 11.32 ug/ml

Instrument :
FID_F
ClientSampleId :

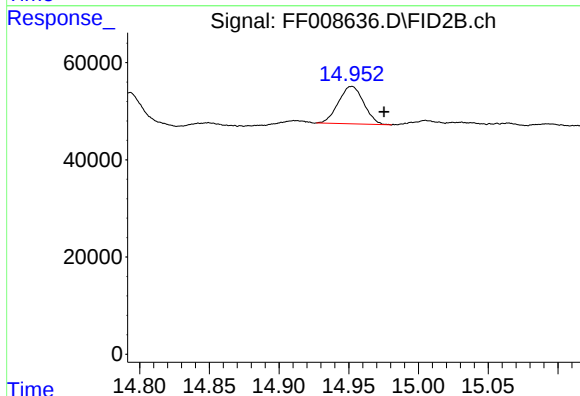


#10 N-TETRACOSANE

R.T.: 14.952 min
Delta R.T.: -0.023 min
Response: 97626
Conc: 0.80 ug/ml

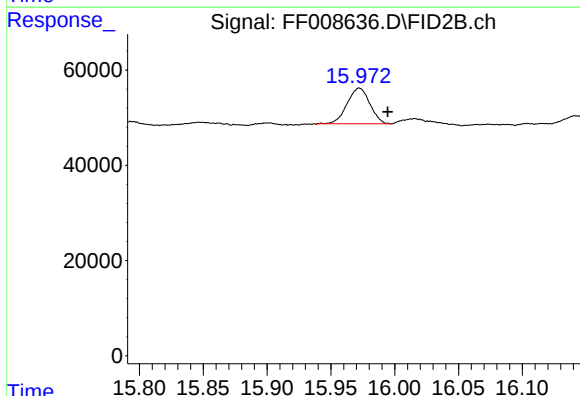

#11 N-HEXACOSANE

R.T.: 15.972 min
Delta R.T.: -0.022 min
Response: 92709
Conc: 0.77 ug/ml

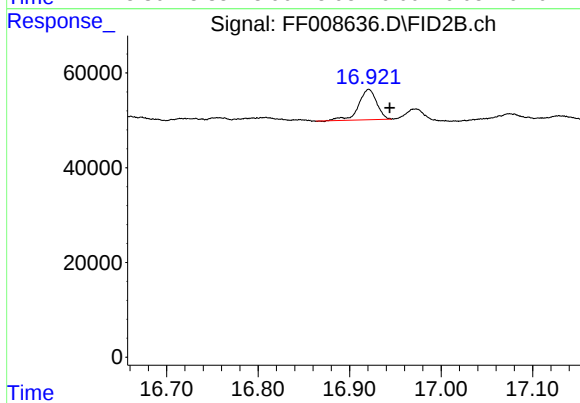

#12 N-OCTACOSANE

R.T.: 16.921 min
Delta R.T.: -0.023 min
Response: 88787
Conc: 0.75 ug/ml