

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008637.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 20:06
Operator : DD\AJ
Sample : M2672-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:03:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	2006845	19.046 ug/ml
Target Compounds			
8) N-DOCOSANE	13.850	83584	0.665 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008637.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 20:06
Operator : DD\AJ
Sample : M2672-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:03:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

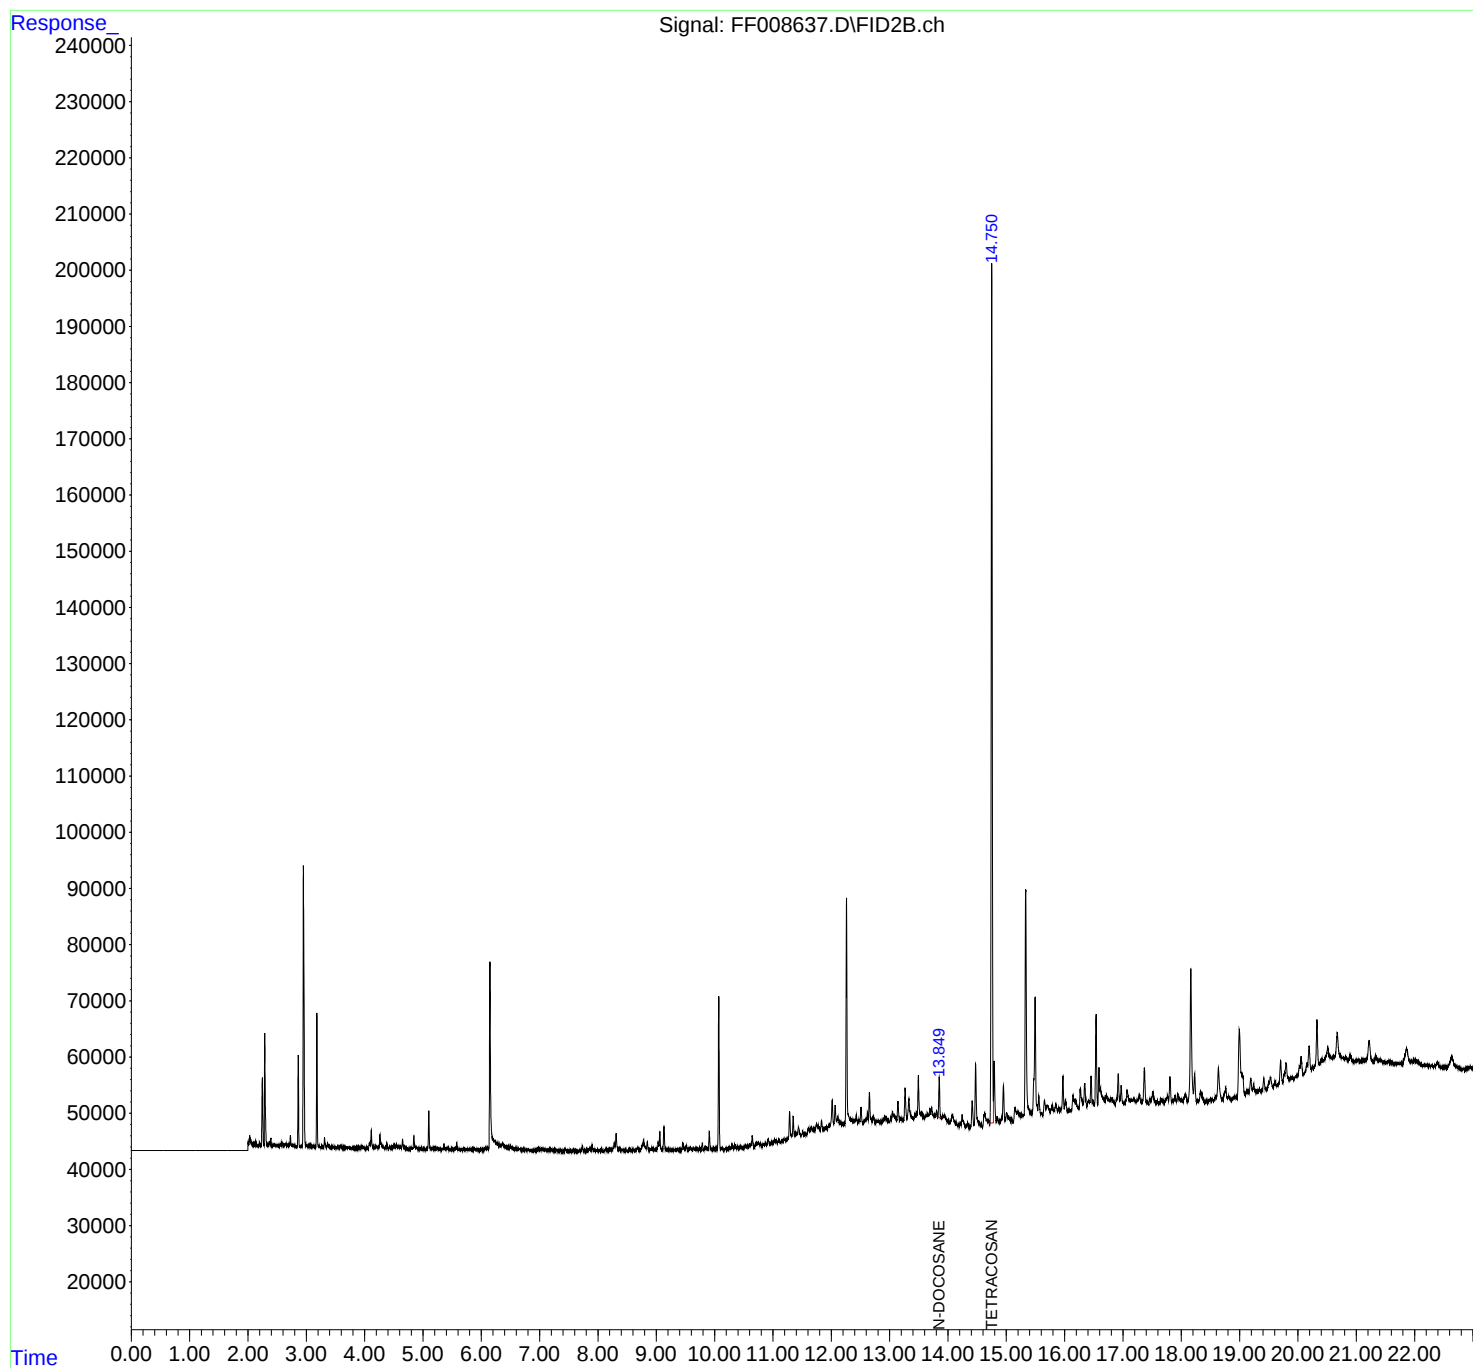


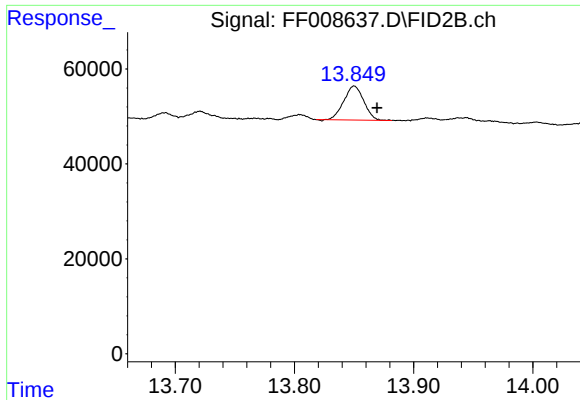

#8 N-DOCOSANE

R.T.: 13.850 min
Delta R.T.: -0.019 min
Response: 83584
Conc: 0.66 ug/ml

Instrument :
FID_F
ClientSampleId :

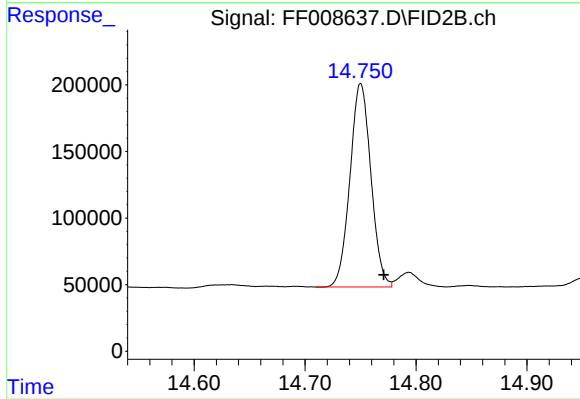

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.021 min
Response: 2006845
Conc: 19.05 ug/ml