

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008638.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 20:38
 Operator : DD\AJ
 Sample : M2672-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 02:03:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.792	127148	1.207 ug/ml
Target Compounds			
8) N-DOCOSANE	13.850	93536	0.744 ug/ml
10) N-TETRACOSANE	14.953	137272	1.120 ug/ml
11) N-HEXACOSANE	15.972	140718	1.173 ug/ml
12) N-OCTACOSANE	16.920	120260	1.014 ug/ml
13) N-TRIACONTANE	17.803	98813	0.834 ug/ml
14) N-DOTRIACONTANE	18.635	73943	0.614 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008638.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 20:38
Operator : DD\AJ
Sample : M2672-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:03:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

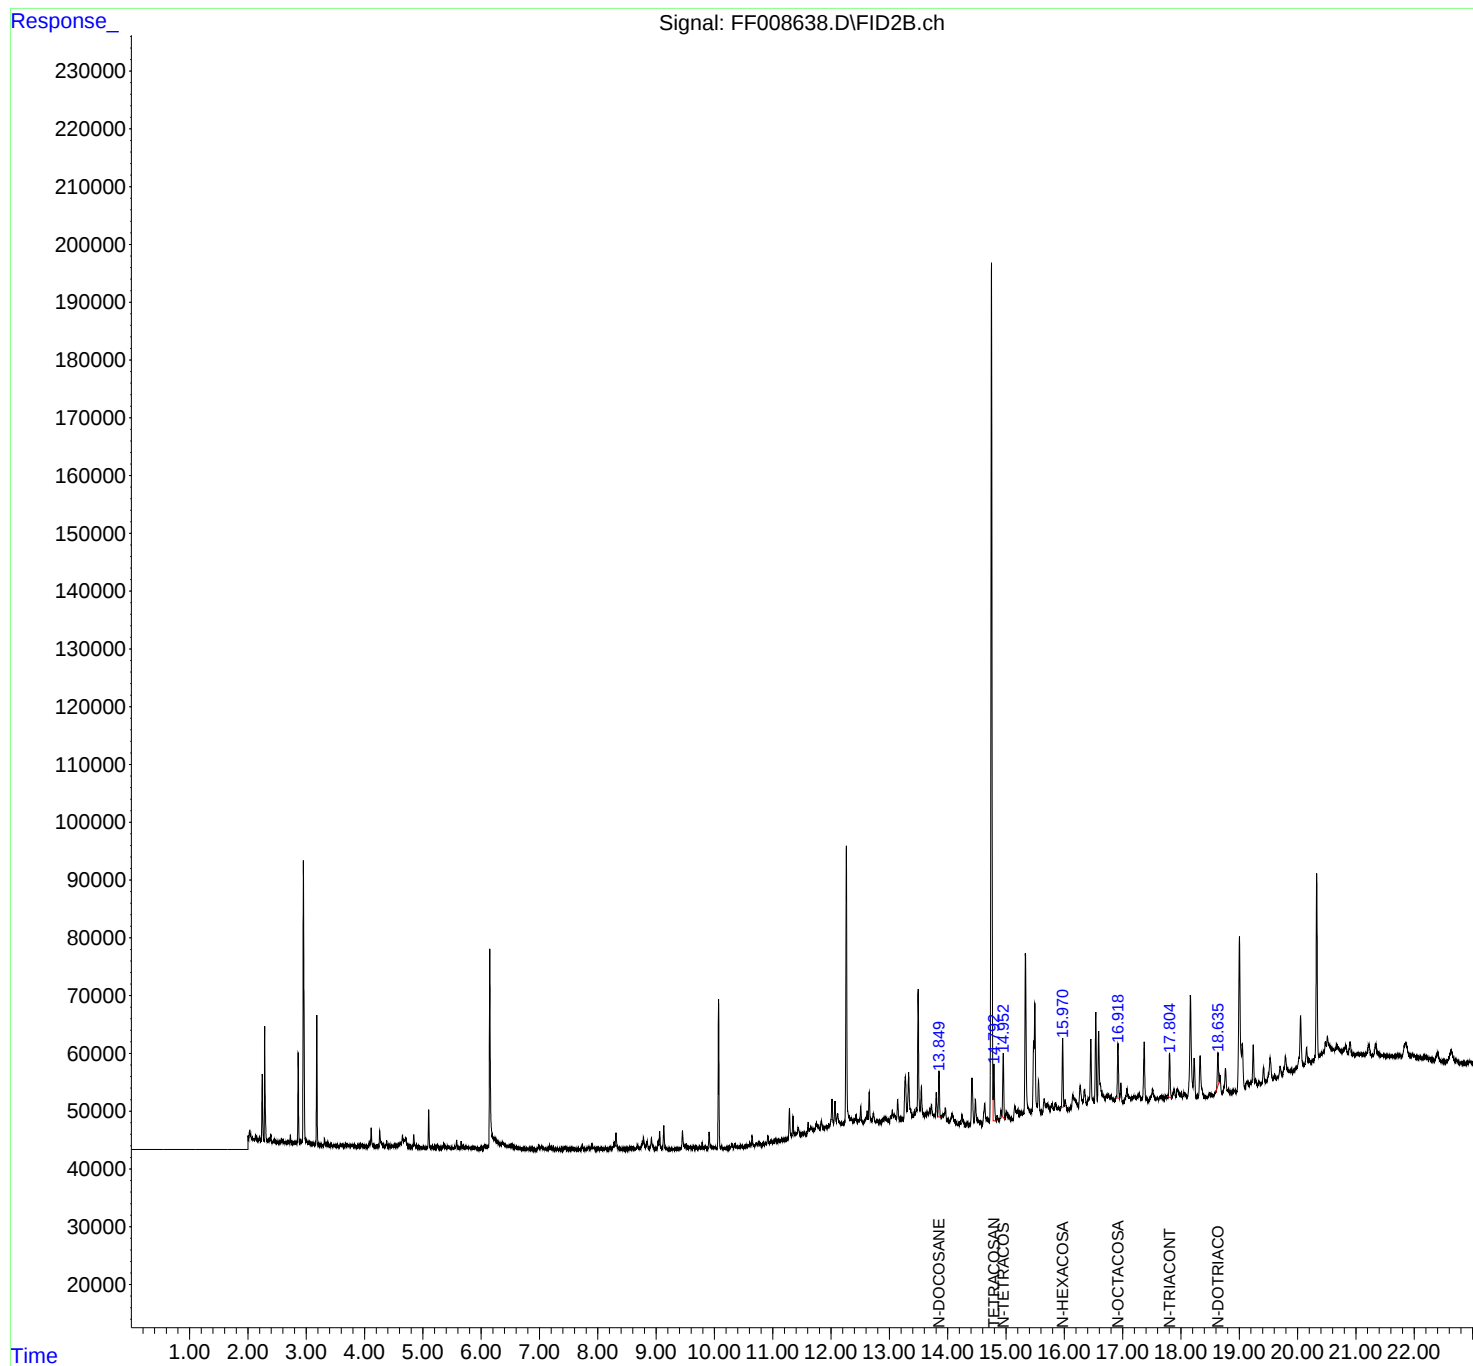


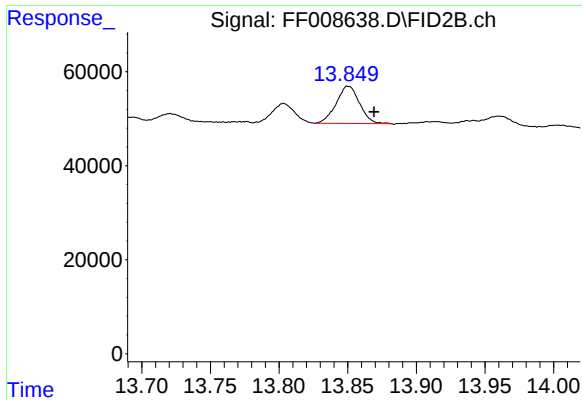

#8 N-DOCOSANE


R.T.: 13.850 min
Delta R.T.: -0.019 min
Response: 93536
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

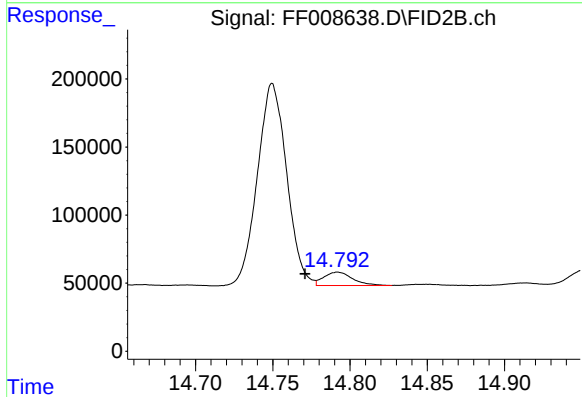


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.792 min
Delta R.T.: 0.021 min
Response: 127148
Conc: 1.21 ug/ml

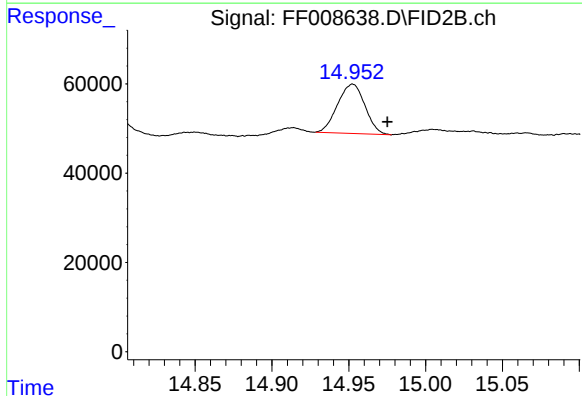


#10 N-TETRACOSANE

R.T.: 14.953 min
Delta R.T.: -0.023 min
Response: 137272
Conc: 1.12 ug/ml

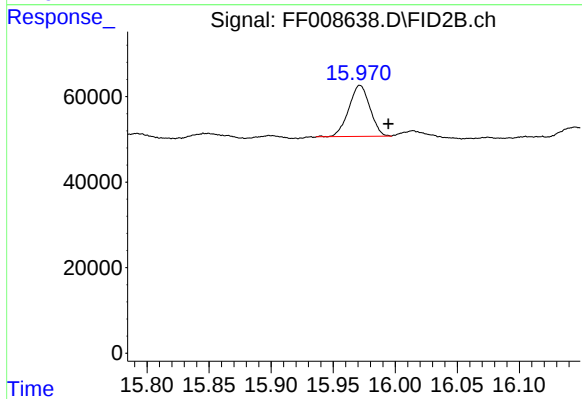

#11 N-HEXACOSANE


R.T.: 15.972 min
Delta R.T.: -0.023 min
Response: 140718
Conc: 1.17 ug/ml

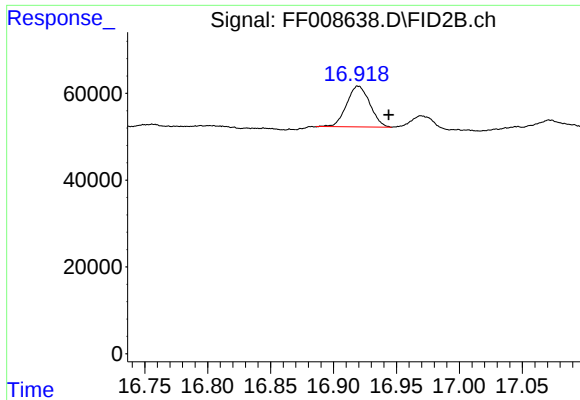

#12 N-OCTACOSANE


R.T.: 16.920 min
Delta R.T.: -0.024 min
Response: 120260
Conc: 1.01 ug/ml

Instrument :
FID_F
ClientSampleId :

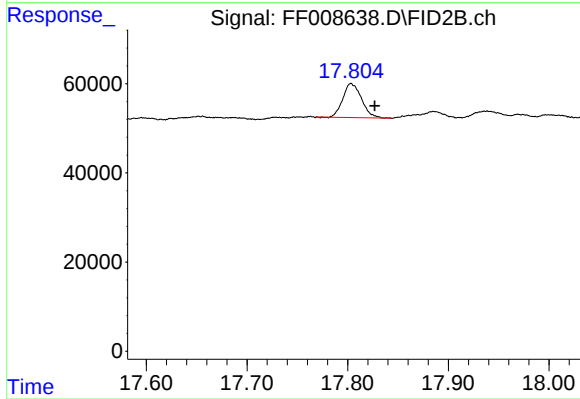

#13 N-TRIACONTANE

R.T.: 17.803 min
Delta R.T.: -0.024 min
Response: 98813
Conc: 0.83 ug/ml

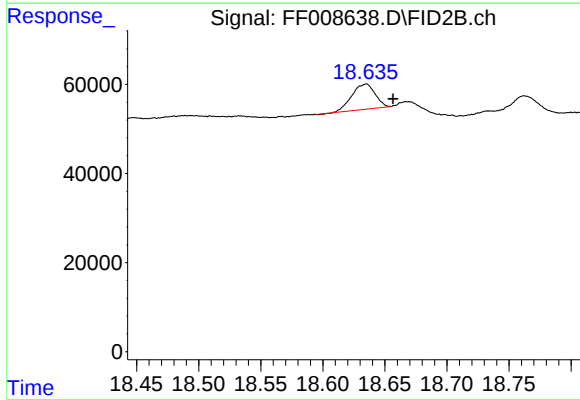

#14 N-DOTRIACONTANE

R.T.: 18.635 min
Delta R.T.: -0.021 min
Response: 73943
Conc: 0.61 ug/ml