

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008639.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 21:09
 Operator : DD\AJ
 Sample : M2672-09
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 02:03:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.791	125156	1.188 ug/ml
Target Compounds			
8) N-DOCOSANE	13.850	89324	0.711 ug/ml
10) N-TETRACOSANE	14.950	127892	1.044 ug/ml
11) N-HEXACOSANE	15.972	94801	0.791 ug/ml
12) N-OCTACOSANE	16.919	90312	0.761 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008639.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 21:09
Operator : DD\AJ
Sample : M2672-09
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:03:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

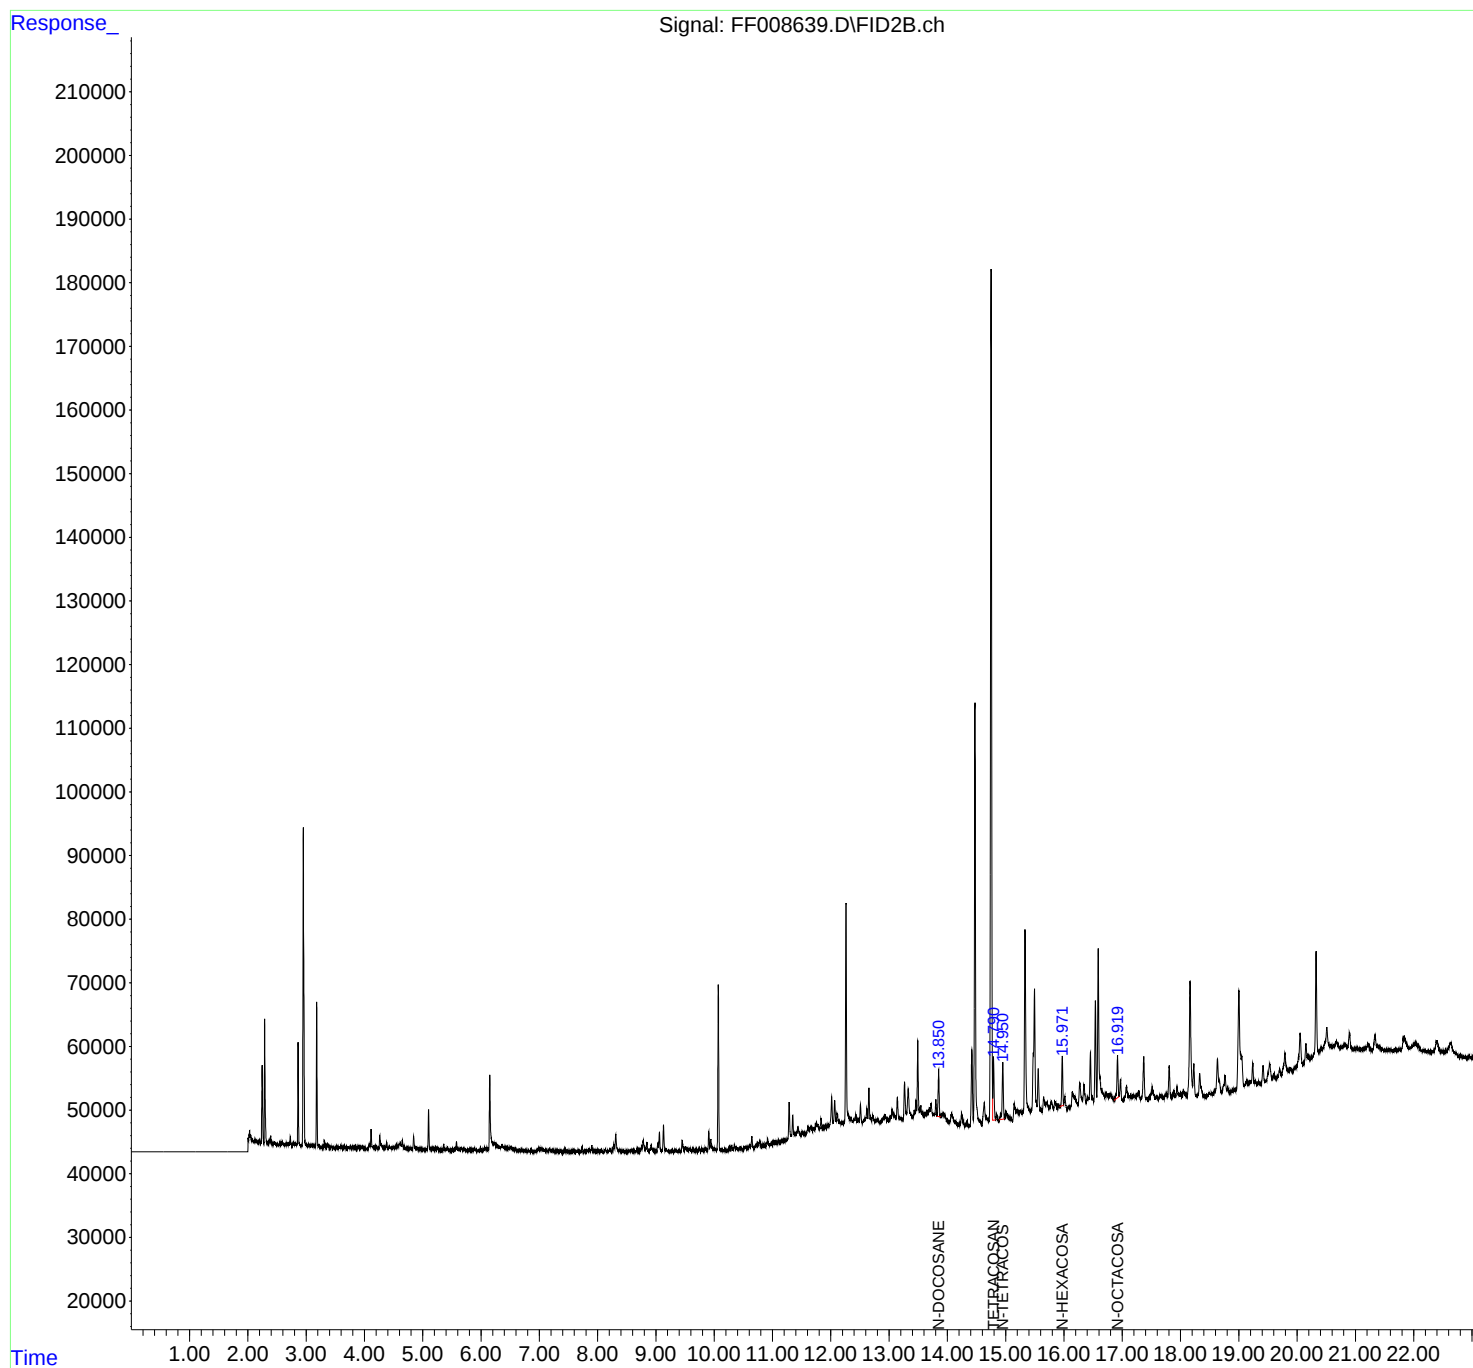


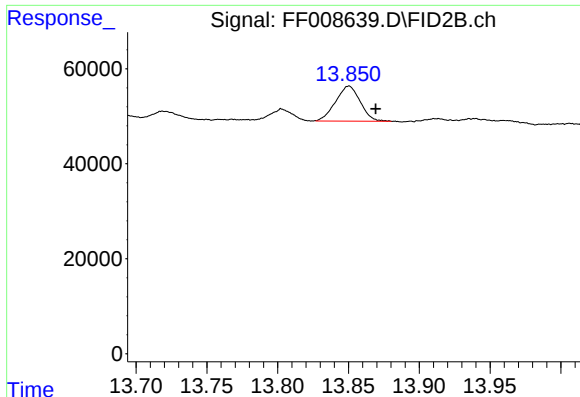

#8 N-DOCOSANE


R.T.: 13.850 min
Delta R.T.: -0.019 min
Response: 89324
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

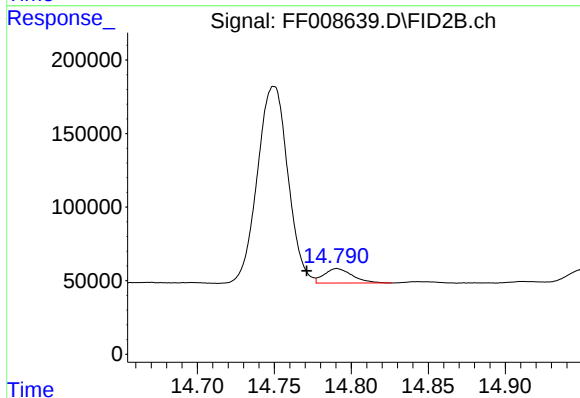


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.791 min
Delta R.T.: 0.020 min
Response: 125156
Conc: 1.19 ug/ml

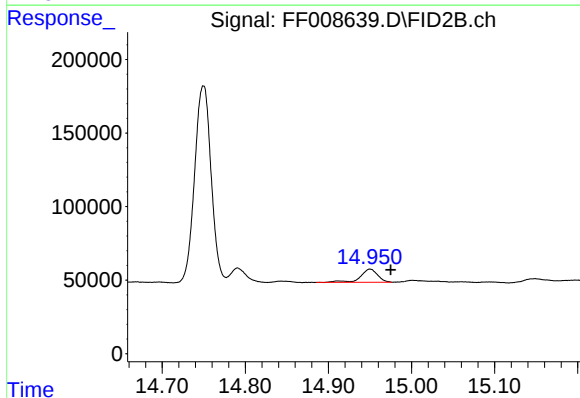


#10 N-TETRACOSANE

R.T.: 14.950 min
Delta R.T.: -0.025 min
Response: 127892
Conc: 1.04 ug/ml

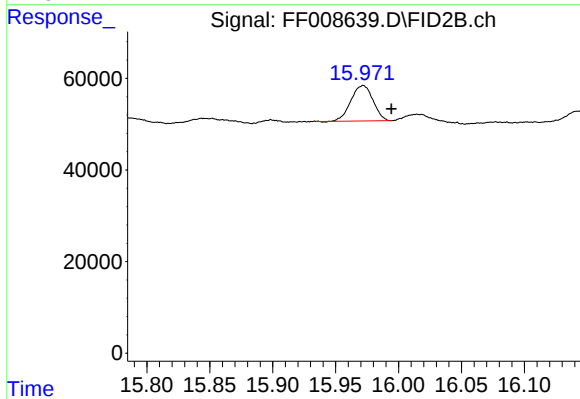

#11 N-HEXACOSANE

R.T.: 15.972 min
Delta R.T.: -0.023 min
Response: 94801
Conc: 0.79 ug/ml

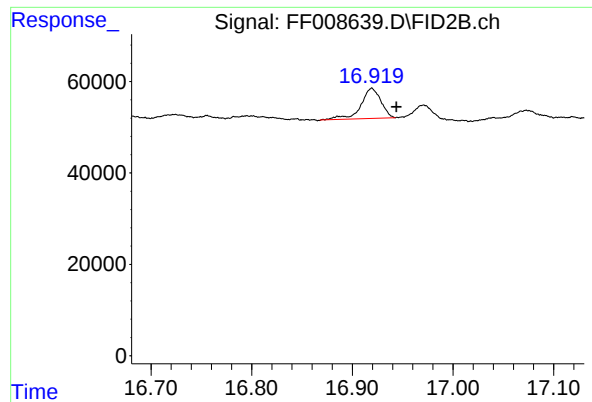

#12 N-OCTACOSANE

R.T.: 16.919 min
Delta R.T.: -0.025 min
Response: 90312
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :