

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008640.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 21:41
Operator : DD\AJ
Sample : M2672-10
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:03:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.751	1985124	18.840 ug/ml
Target Compounds			
8) N-DOCOSANE	13.850	78855	0.627 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008640.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 21:41
Operator : DD\AJ
Sample : M2672-10
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 02:03:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

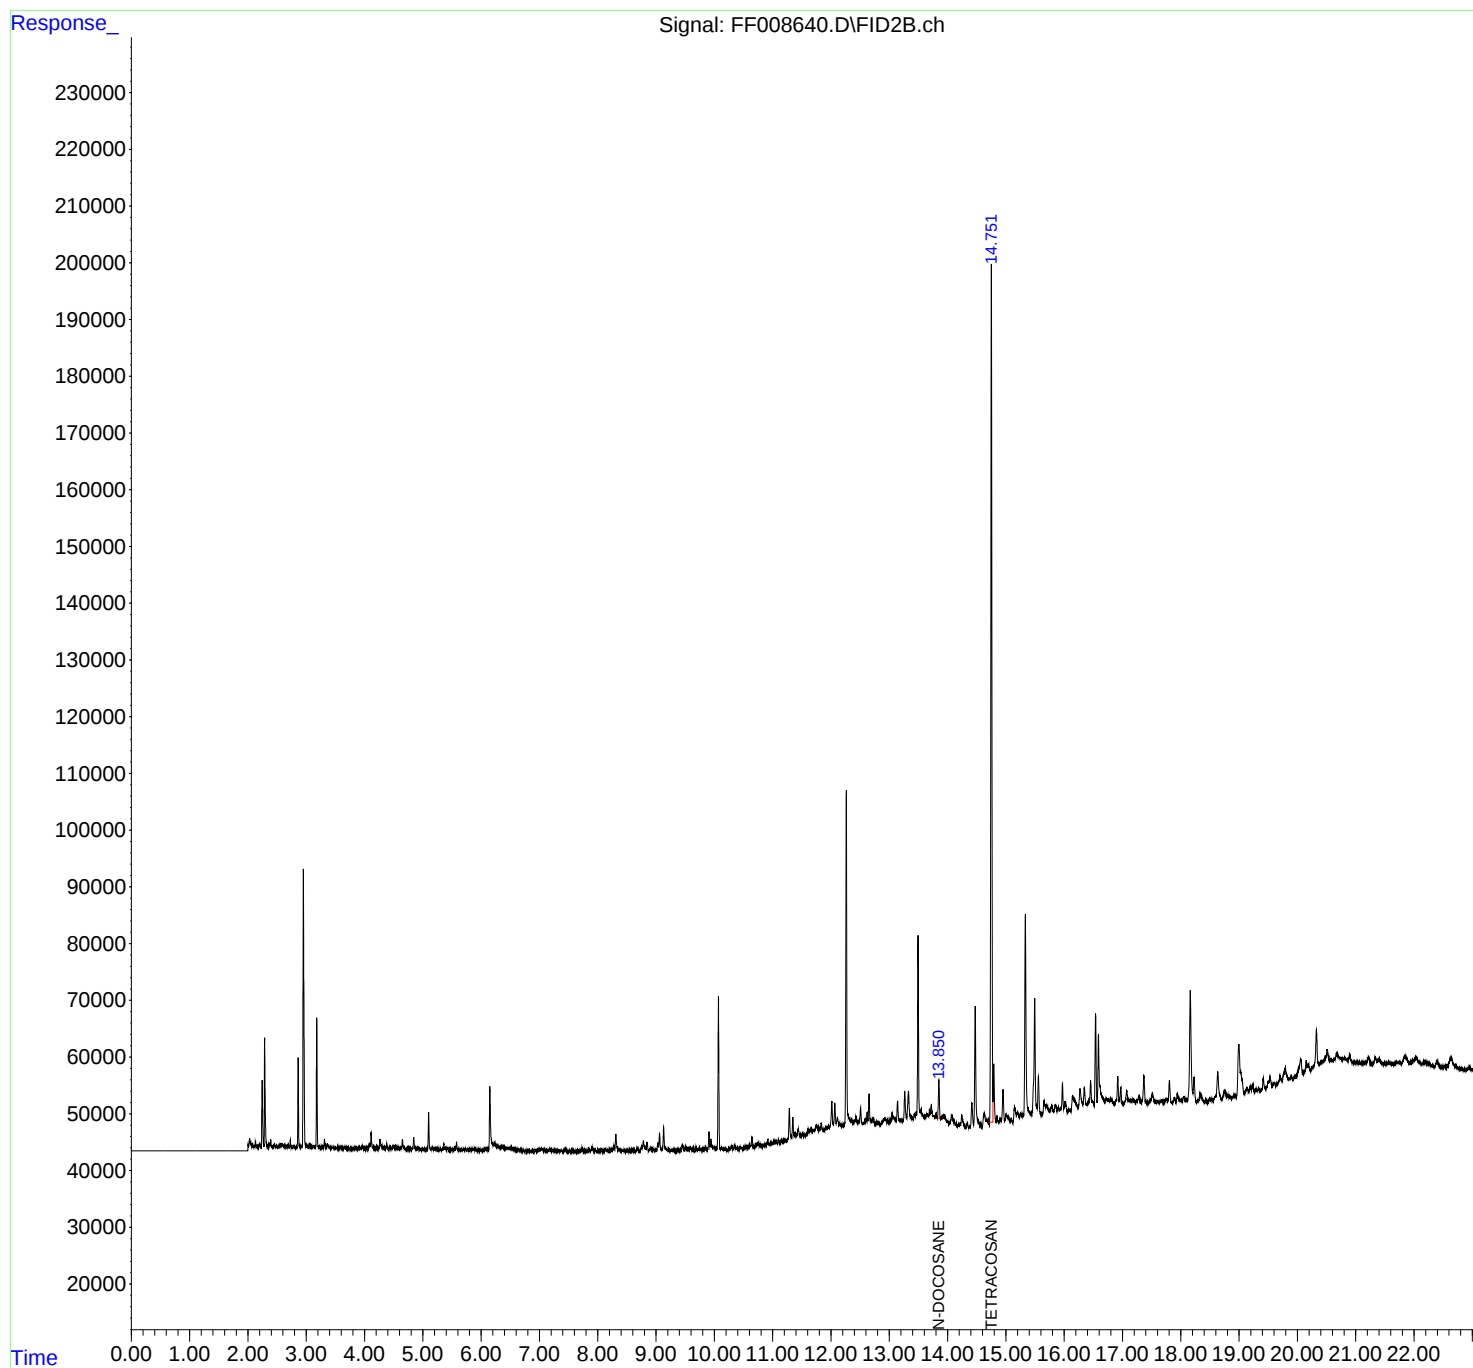


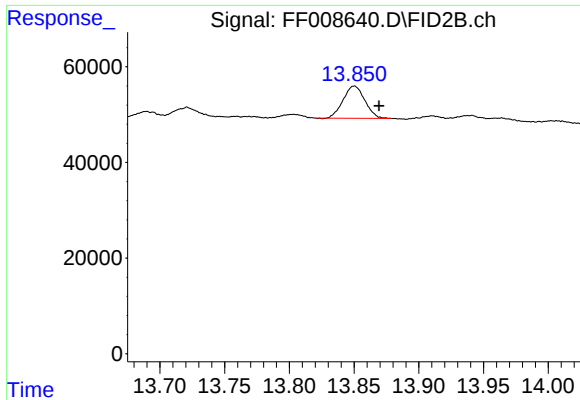

#8 N-DOCOSANE

R.T.: 13.850 min
Delta R.T.: -0.019 min
Response: 78855
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

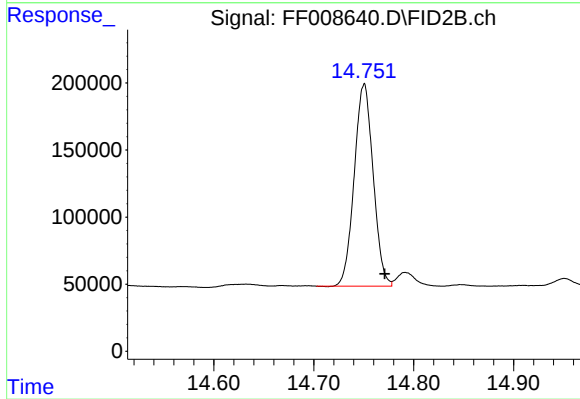

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.751 min
Delta R.T.: -0.020 min
Response: 1985124
Conc: 18.84 ug/ml