

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008634.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 18:31
Operator : DD\AJ
Sample : M2672-04
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
17-B6(20-24)

Integration File: autoint1.e
Quant Time: Jun 16 02:02:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	1772306	16.820 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008634.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 18:31
Operator : DD\AJ
Sample : M2672-04
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
17-B6(20-24)

Integration File: autoint1.e
Quant Time: Jun 16 02:02:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

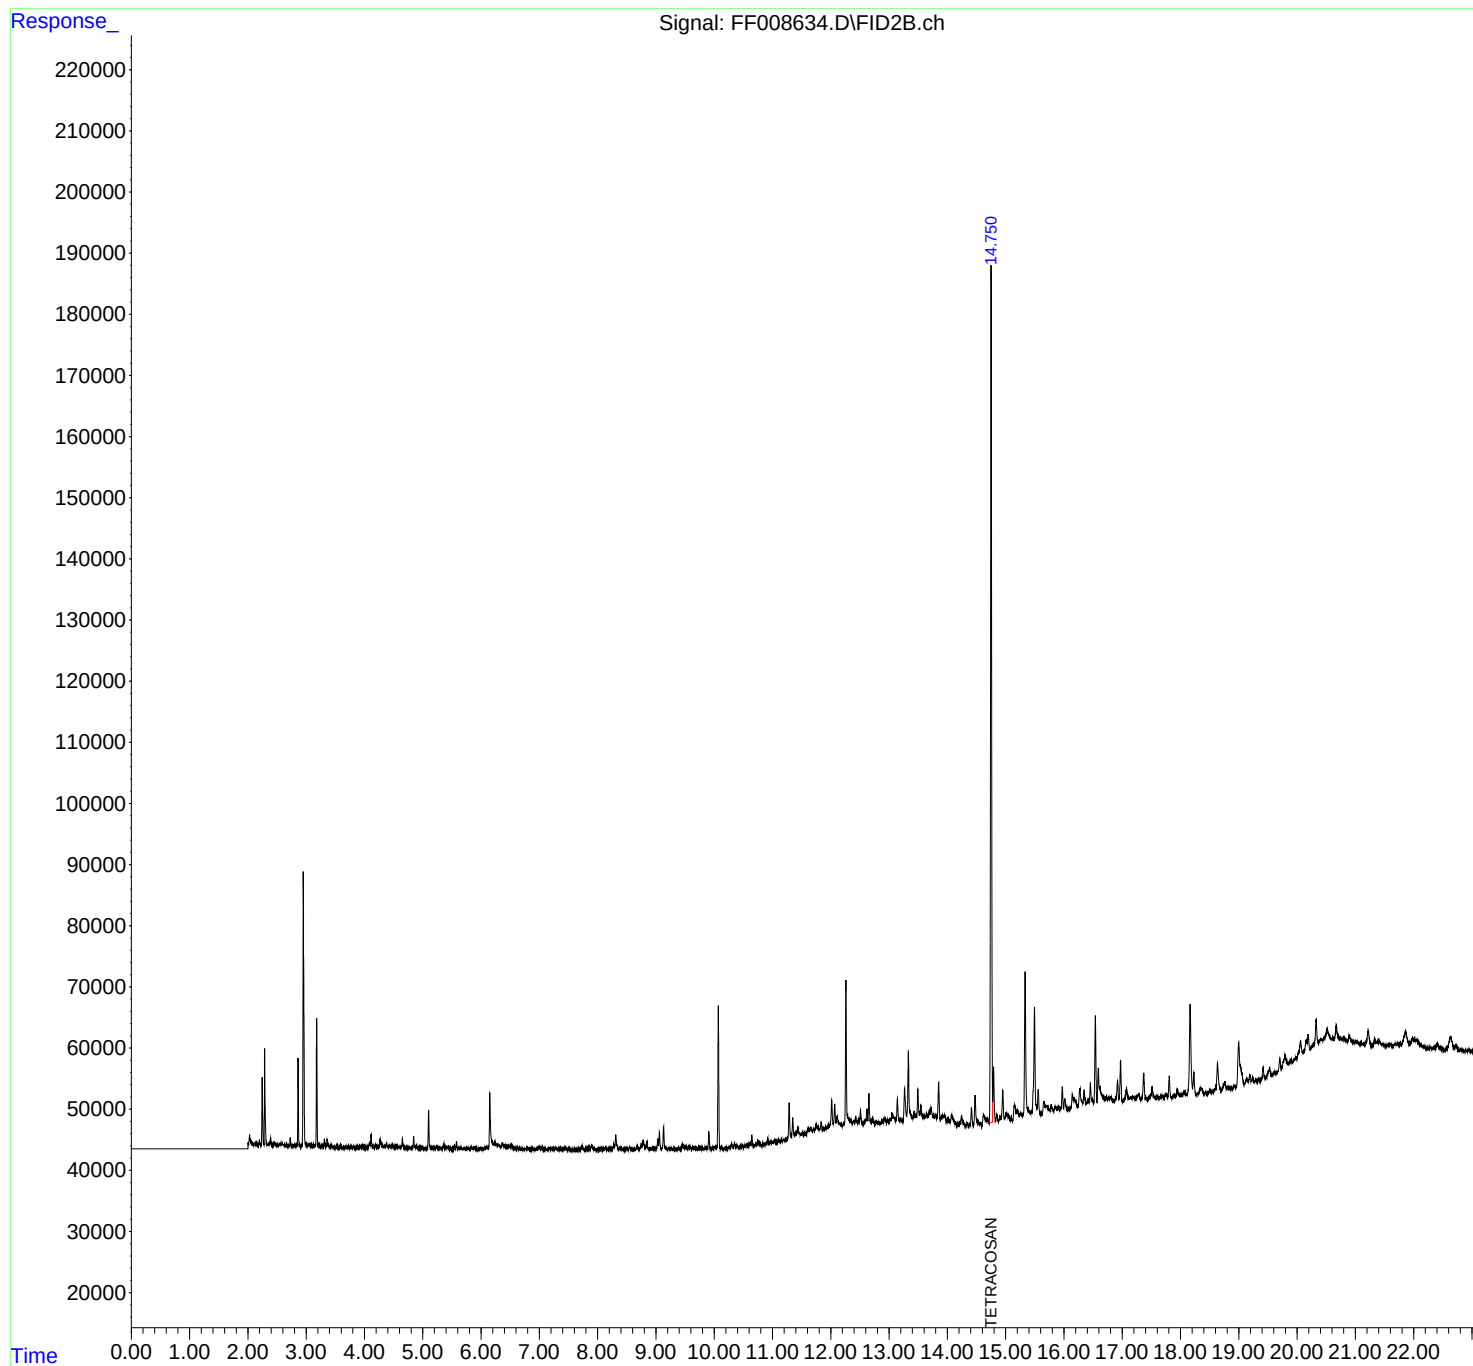

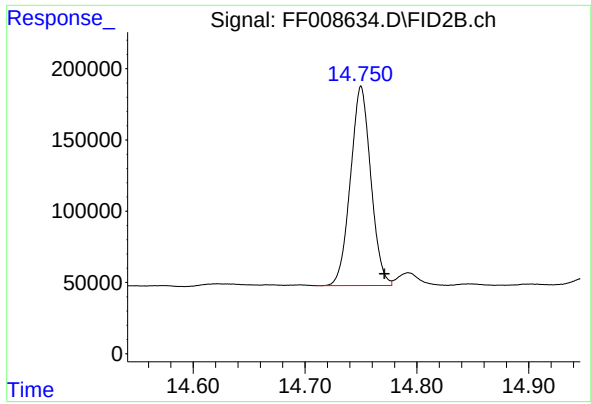

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.021 min
Response: 1772306
Conc: 16.82 ug/ml

Instrument :
FID_F
ClientSampleId :
17-B6(20-24)