

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
 Data File : FF008636.D
 Signal(s) : FID2B.ch
 Acq On : 15 Jun 2021 19:35
 Operator : DD\AJ
 Sample : M2672-06
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 17-B6(28-32)

Manual Integrations
 APPROVED

Ankita
 6/16/2021 2:26:02 PM

Integration File: autoint1.e
 Quant Time: Jun 16 02:02:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	1242424	11.791 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061521\
Data File : FF008636.D
Signal(s) : FID2B.ch
Acq On : 15 Jun 2021 19:35
Operator : DD\AJ
Sample : M2672-06
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
17-B6(28-32)


Manual Integrations
APPROVED

Ankita
6/16/2021 2:26:02 PM

Integration File: autoint1.e
Quant Time: Jun 16 02:02:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

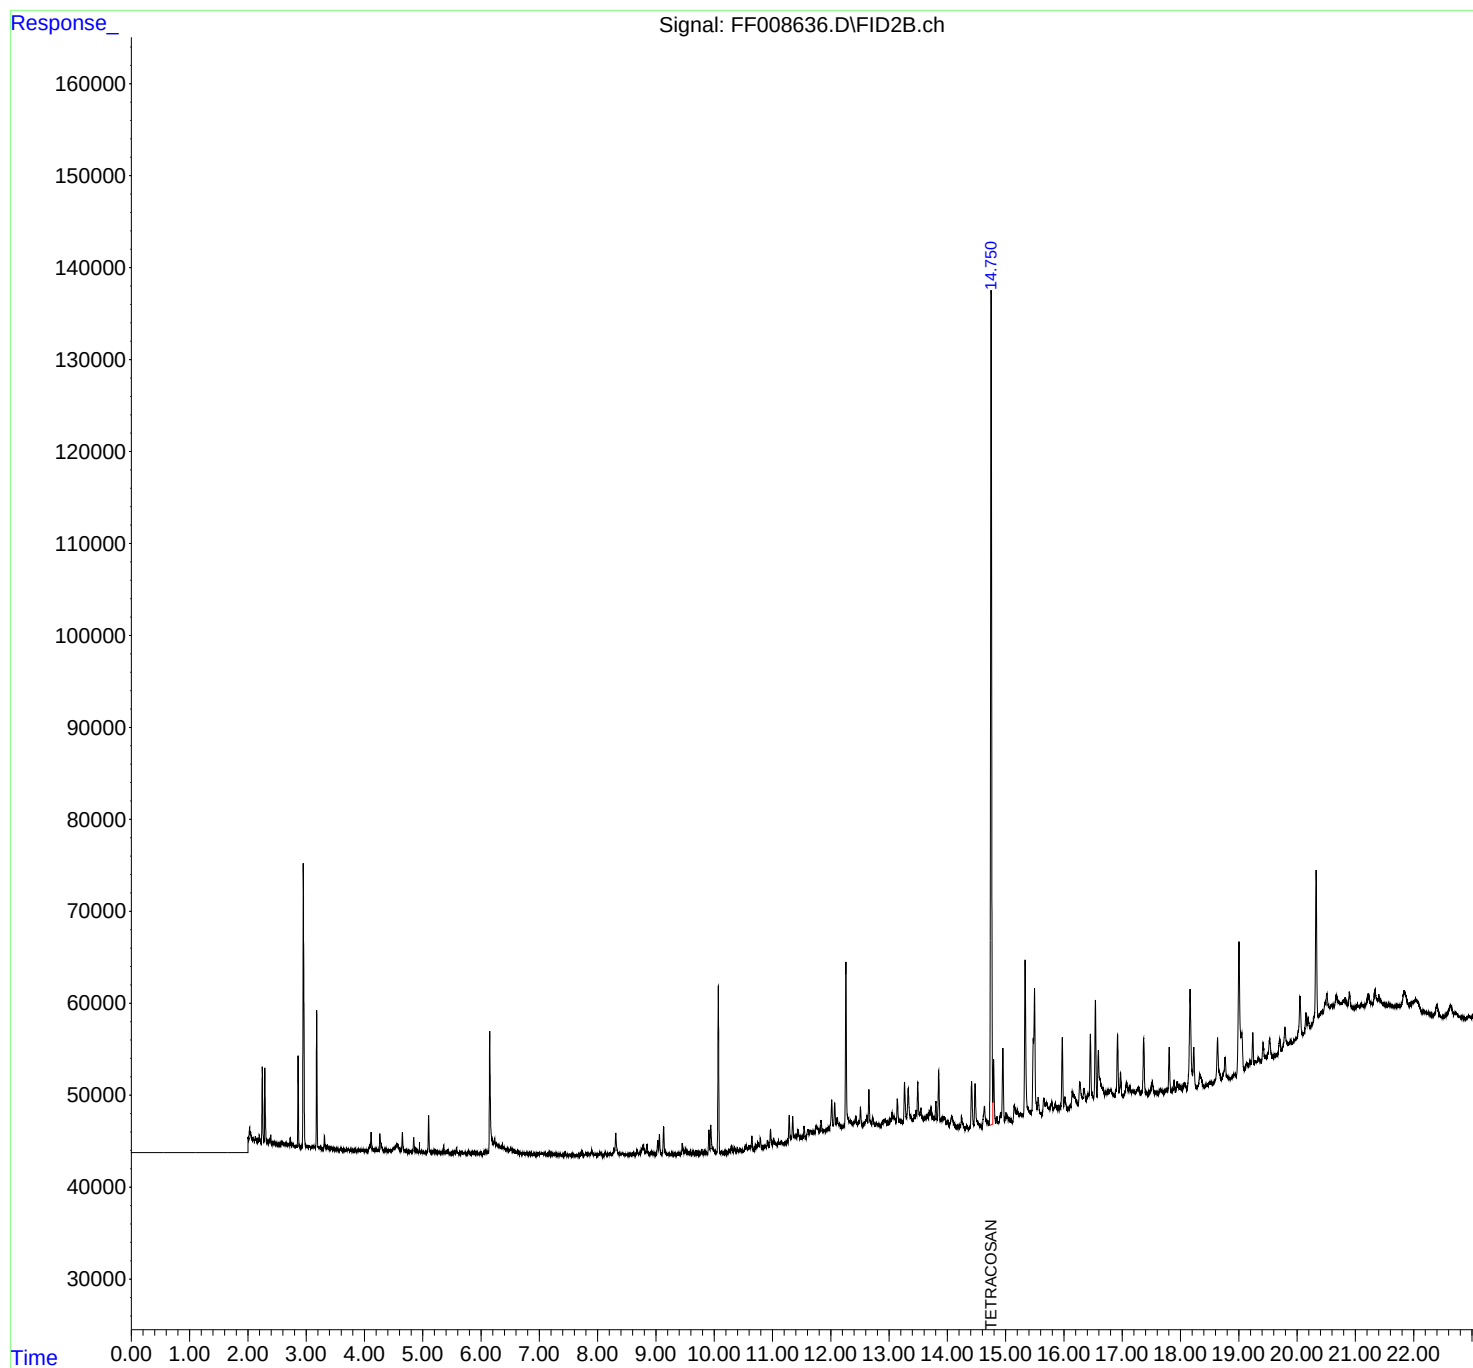

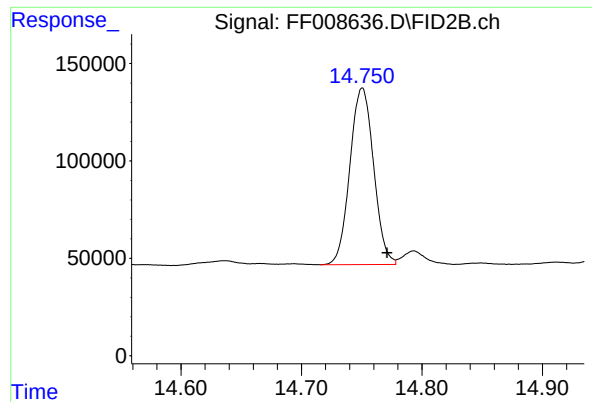

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: -0.021 min
Response: 1242424
Conc: 11.79 ug/ml m

Instrument :
FID_F
ClientSampleId :
17-B6(28-32)

Manual Integrations
APPROVED

Ankita
6/16/2021 2:26:02 PM