

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061719\
 Data File : FF004814.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jun 2019 16:03
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 17 17:39:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.708	5849624	47.904 ug/ml
Target Compounds			
2) N-DECANE	4.415	7505118	51.254 ug/ml
3) N-DODECANE	6.440	7478027	50.533 ug/ml
4) N-TETRADECANE	8.236	7326467	49.878 ug/ml
5) N-HEXADECANE	9.840	7226632	48.946 ug/ml
6) N-OCTADECANE	11.286	6972019	48.022 ug/ml
7) N-EICOSANE	12.601	6862270	47.382 ug/ml
8) N-DOCOSANE	13.805	6701278	47.424 ug/ml
10) N-TETRACOSANE	14.913	6646907	47.962 ug/ml
11) N-HEXACOSANE	15.939	6625011	48.623 ug/ml
12) N-OCTACOSANE	16.894	6629536	48.761 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061719\
Data File : FF004814.D
Signal(s) : FID2B.ch
Acq On : 17 Jun 2019 16:03
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 17 17:39:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

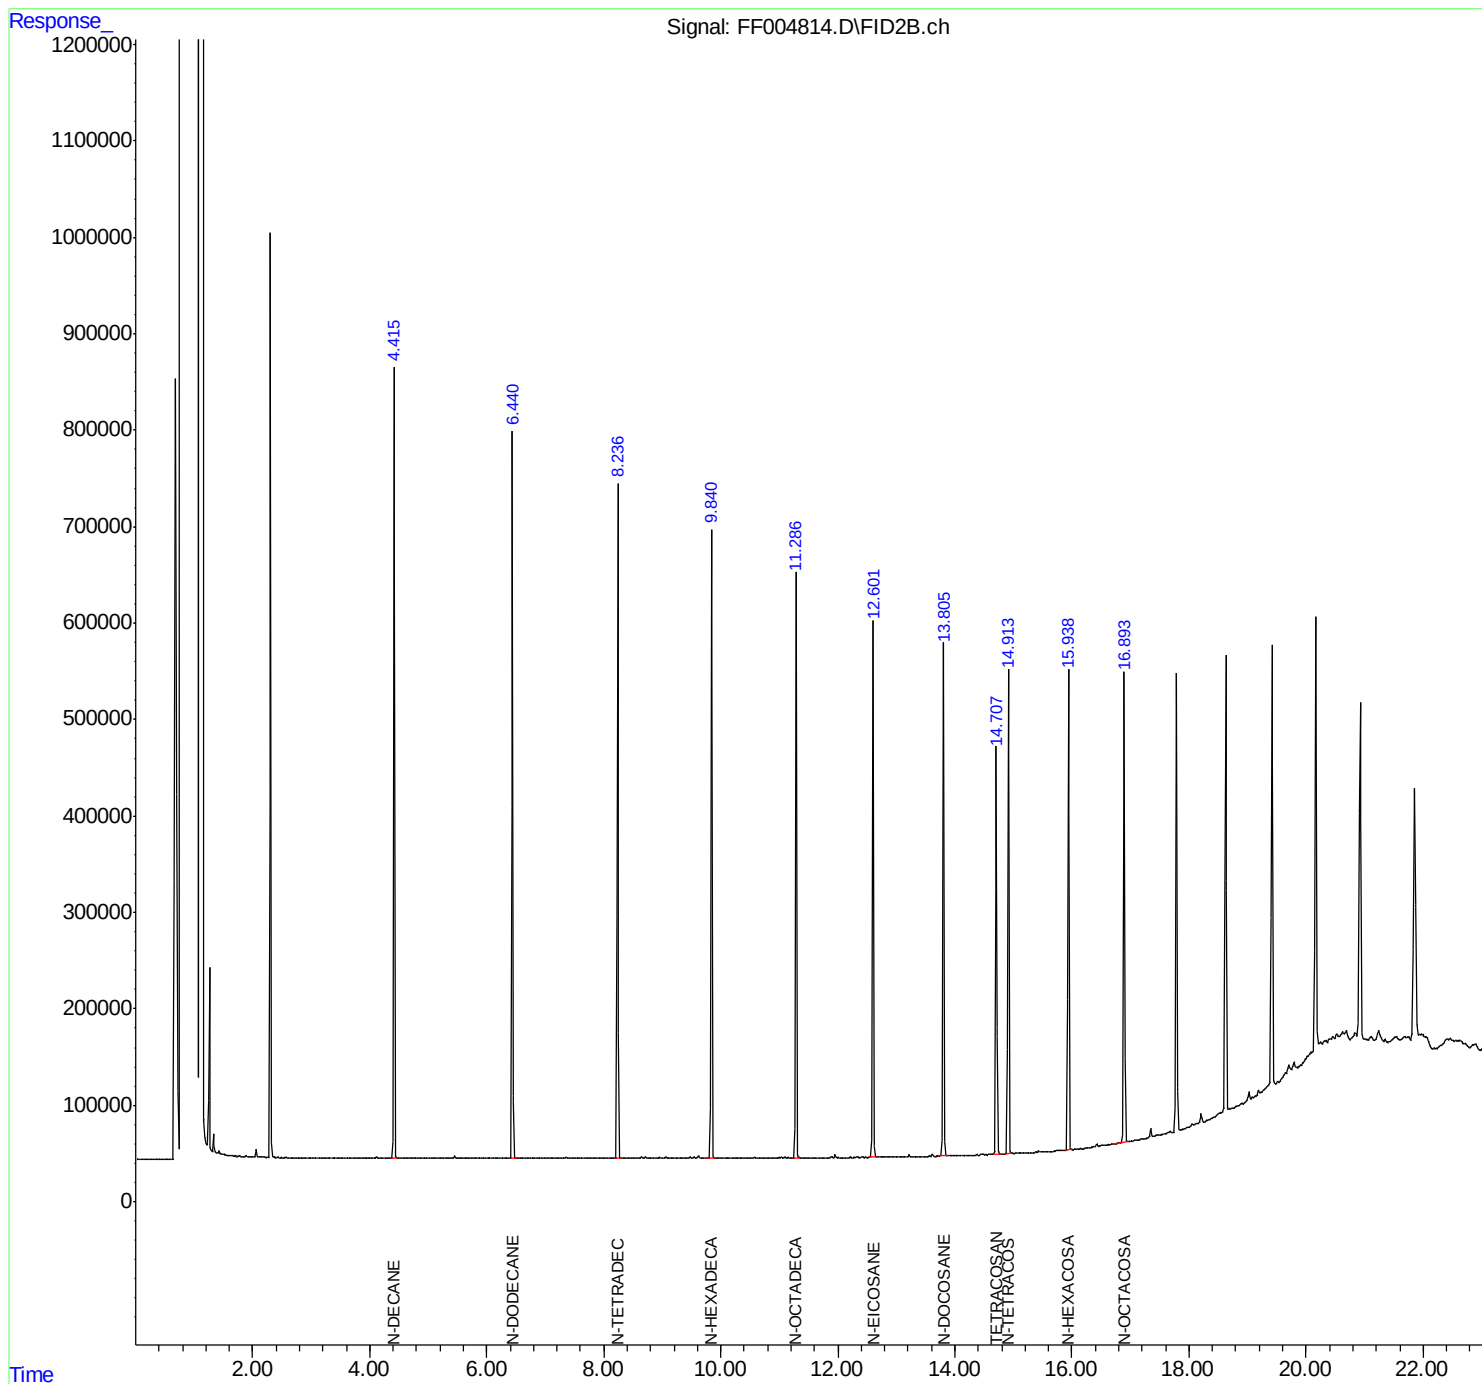

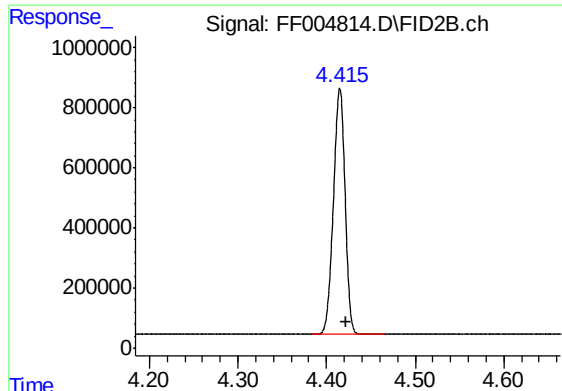


#2 N-DECANE

R.T.: 4.415 min
Delta R.T.: -0.007 min
Response: 7505118
Conc: 51.25 ug/ml

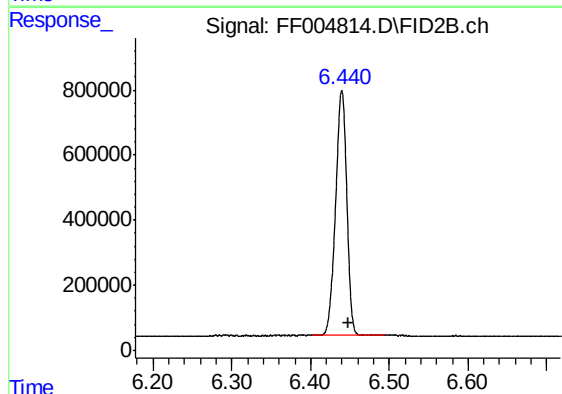


#3 N-DODECANE

R.T.: 6.440 min
Delta R.T.: -0.008 min
Response: 7478027
Conc: 50.53 ug/ml

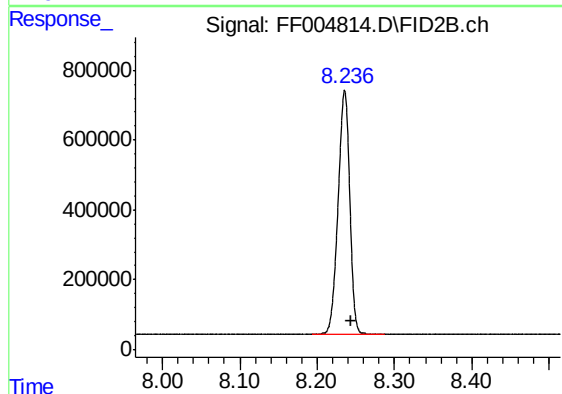


#4 N-TETRADECANE

R.T.: 8.236 min
Delta R.T.: -0.008 min
Response: 7326467
Conc: 49.88 ug/ml

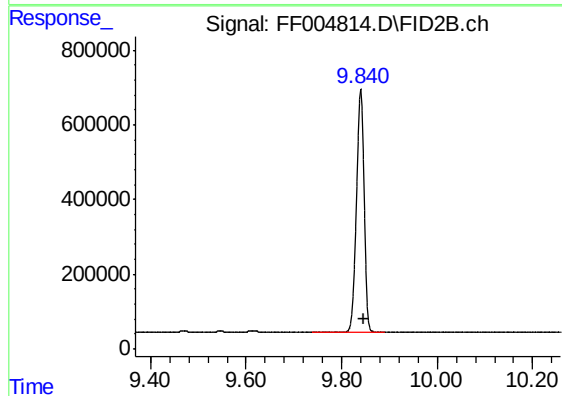


#5 N-HEXADECANE

R.T.: 9.840 min
Delta R.T.: -0.008 min
Response: 7226632
Conc: 48.95 ug/ml

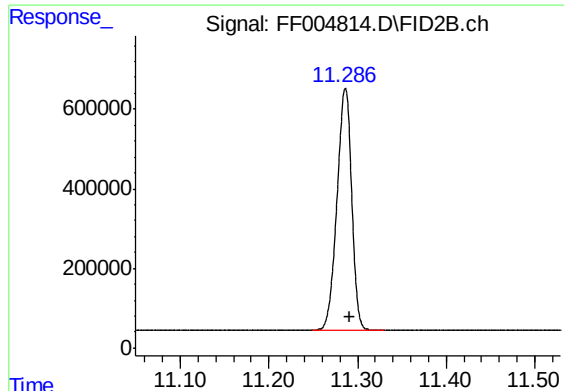


#6 N-OCTADECANE

R.T.: 11.286 min
Delta R.T.: -0.005 min
Response: 6972019
Conc: 48.02 ug/ml

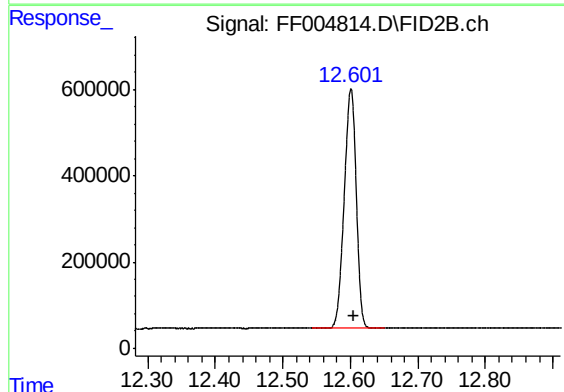


#7 N-EICOSANE

R.T.: 12.601 min
Delta R.T.: -0.005 min
Response: 6862270
Conc: 47.38 ug/ml

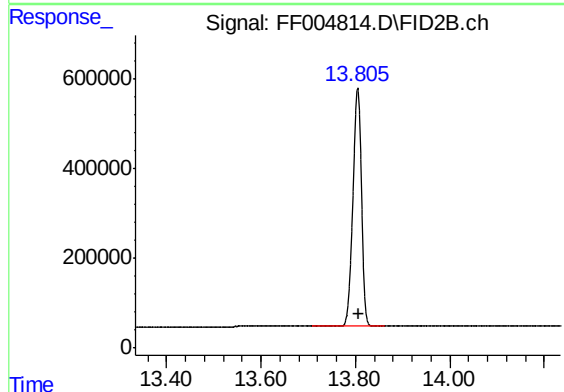


#8 N-DOCOSANE

R.T.: 13.805 min
Delta R.T.: -0.002 min
Response: 6701278
Conc: 47.42 ug/ml

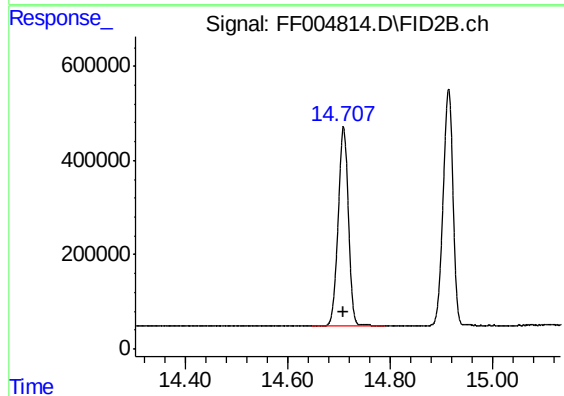


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.708 min
Delta R.T.: 0.000 min
Response: 5849624
Conc: 47.90 ug/ml

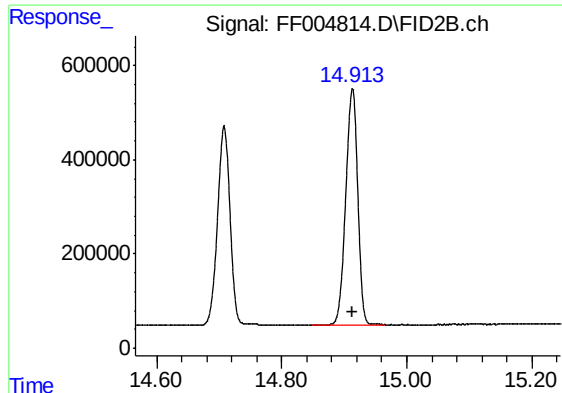


#10 N-TETRACOSANE

R.T.: 14.913 min
Delta R.T.: 0.000 min
Response: 6646907
Conc: 47.96 ug/ml

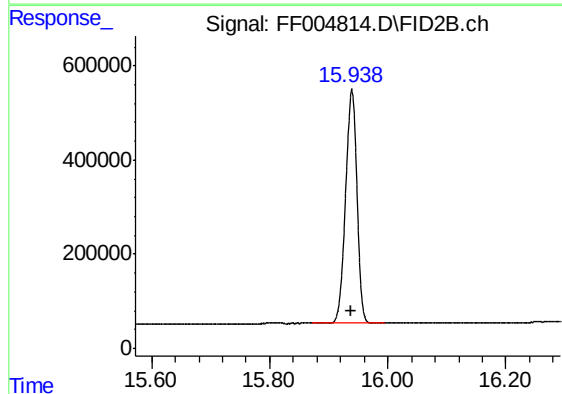

#11 N-HEXACOSANE

R.T.: 15.939 min
Delta R.T.: 0.002 min
Response: 6625011
Conc: 48.62 ug/ml

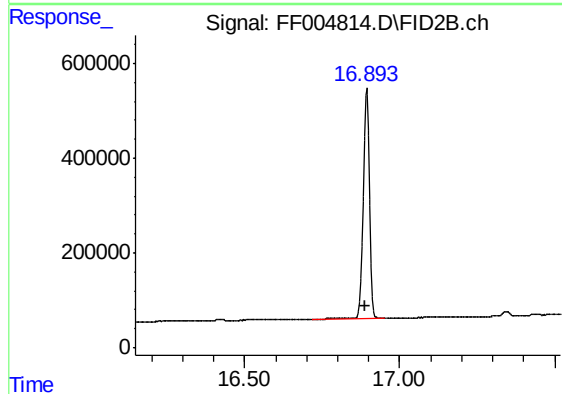

#12 N-OCTACOSANE

R.T.: 16.894 min
Delta R.T.: 0.004 min
Response: 6629536
Conc: 48.76 ug/ml