

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
 Data File : FF010796.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jun 2022 15:57
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 23:19:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.553	3072082	25.279 ug/ml
12) N-OCTACOSANE	16.993	3134472	25.684 ug/ml
13) N-TRIACONTANE	17.877	561259	4.579 ug/ml
14) N-DOTRIACONTANE	18.707	741510	6.111 ug/ml
15) N-TETRATRIACONTANE	19.489	575022	5.533 ug/ml
16) N-HEXATRIACONTANE	20.226	355846	4.138 ug/ml
17) N-OCTATRIACONTANE	20.934	226396	2.956 ug/ml
18) N-TETRACONTANE	21.758	214561	2.746 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
Data File : FF010796.D
Signal(s) : FID2B.ch
Acq On : 17 Jun 2022 15:57
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:19:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

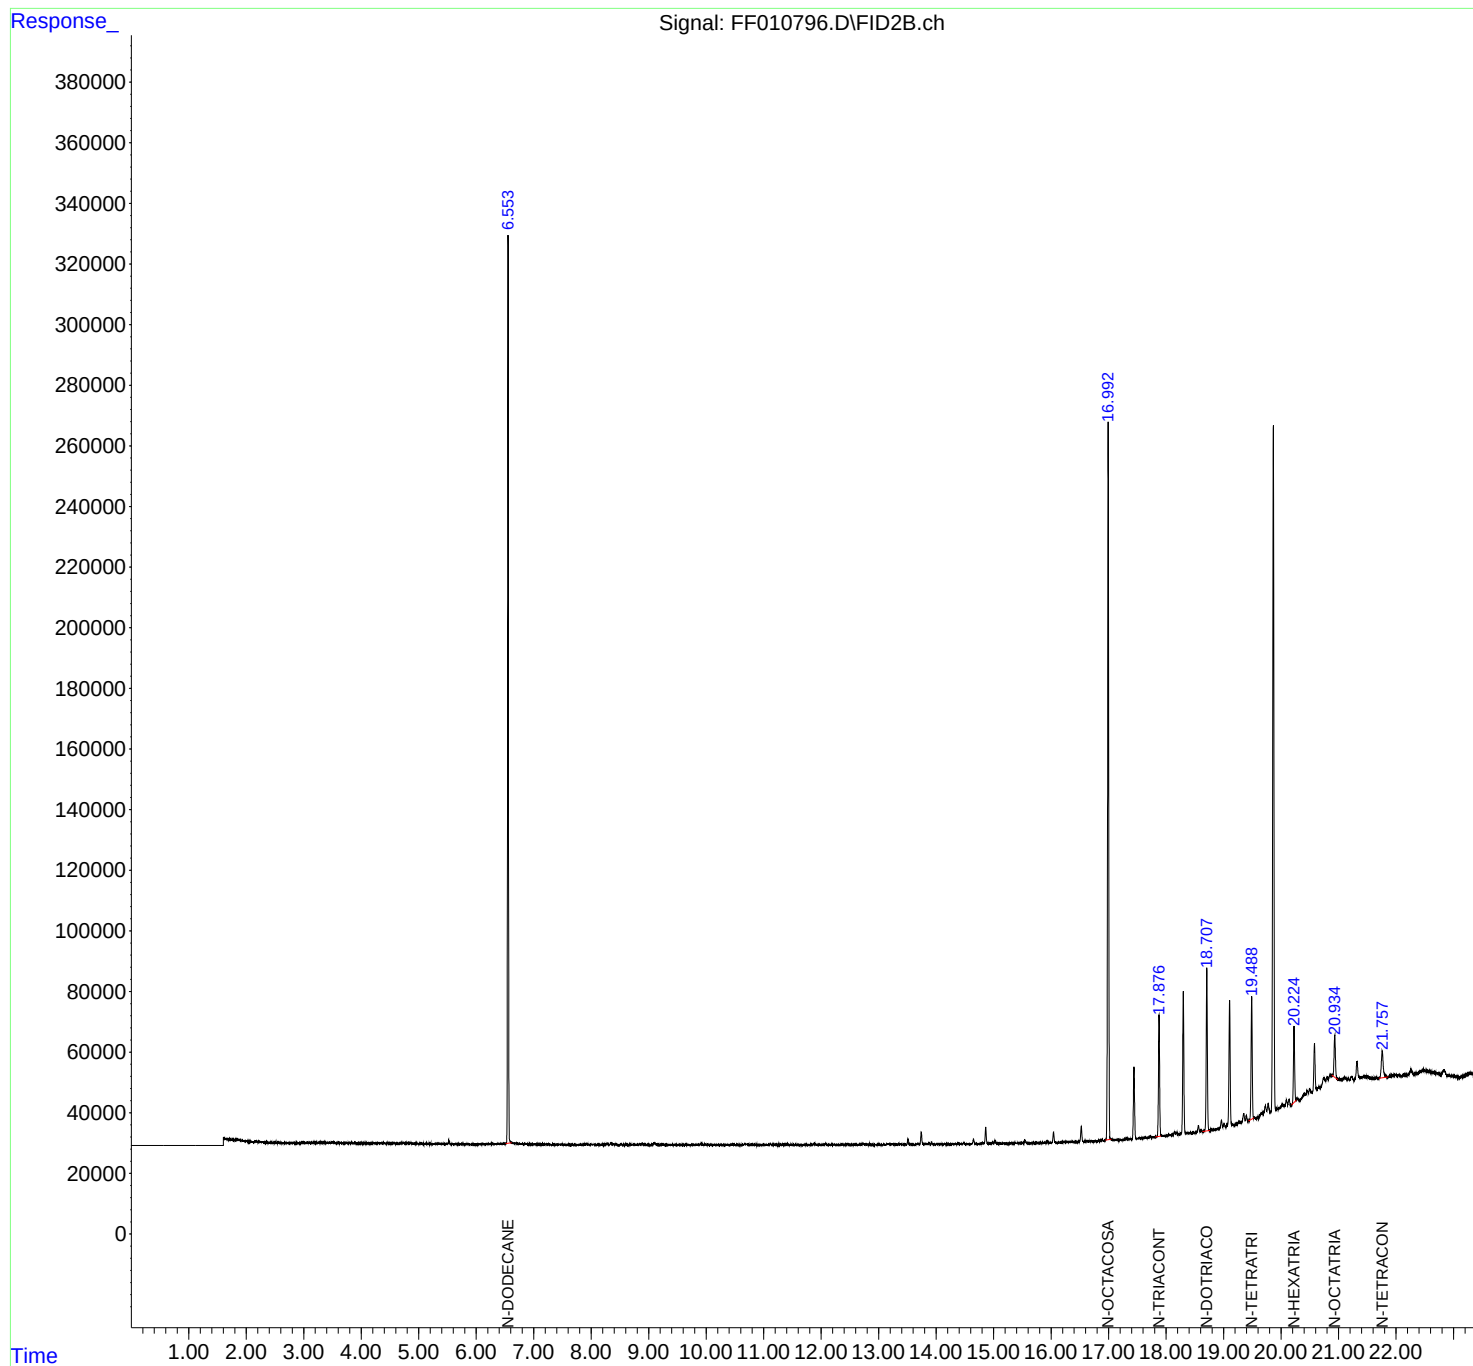


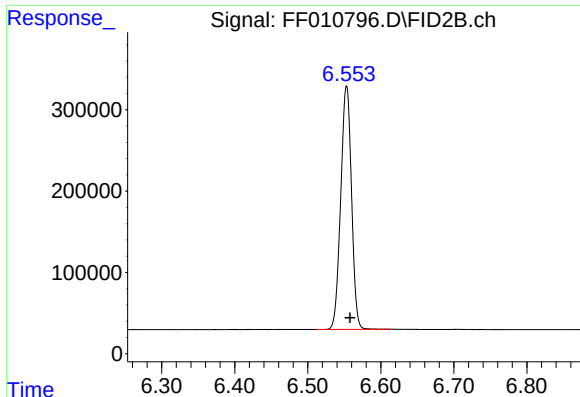

#3 N-DODECANE


R.T.: 6.553 min
Delta R.T.: -0.005 min
Response: 3072082
Conc: 25.28 ug/ml

Instrument :
FID_F
ClientSampleId :

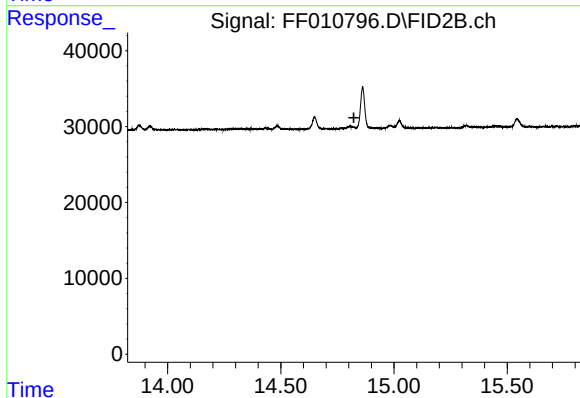


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

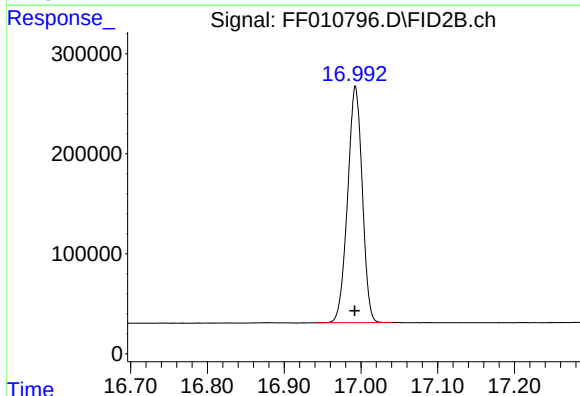


#12 N-OCTACOSANE

R.T.: 16.993 min
Delta R.T.: 0.000 min
Response: 3134472
Conc: 25.68 ug/ml

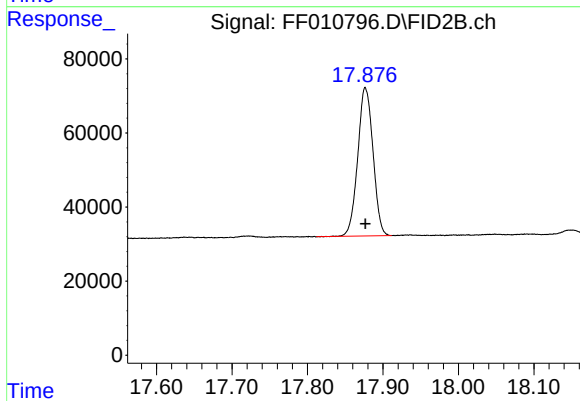

#13 N-TRIACONTANE


R.T.: 17.877 min
Delta R.T.: 0.000 min
Response: 561259
Conc: 4.58 ug/ml

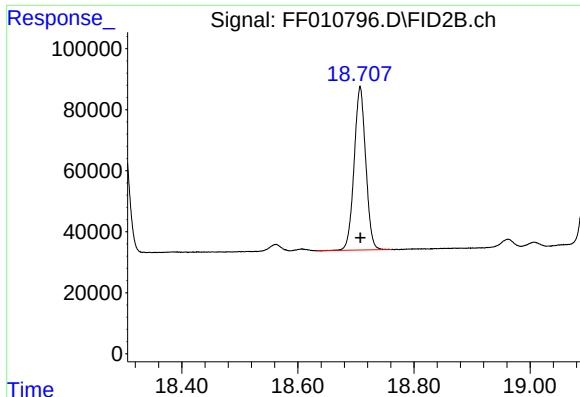

#14 N-DOTRIACONTANE


R.T.: 18.707 min
Delta R.T.: 0.000 min
Response: 741510
Conc: 6.11 ug/ml

Instrument :
FID_F
ClientSampleId :

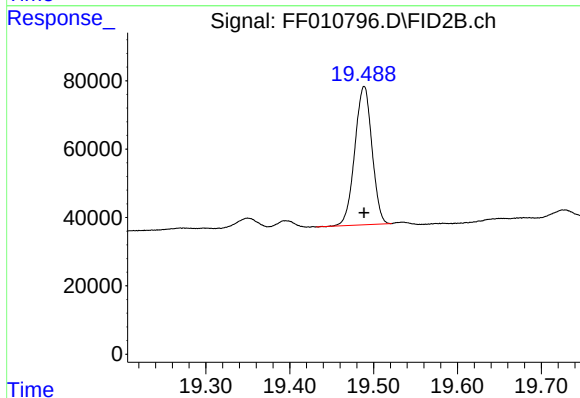


#15 N-TETRATRIACONTANE

R.T.: 19.489 min
Delta R.T.: 0.000 min
Response: 575022
Conc: 5.53 ug/ml

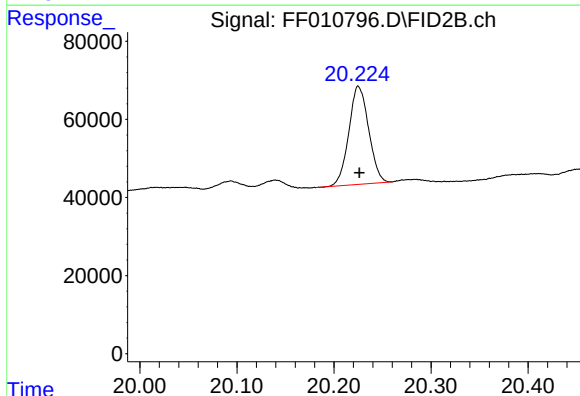


#16 N-HEXATRIACONTANE

R.T.: 20.226 min
Delta R.T.: 0.000 min
Response: 355846
Conc: 4.14 ug/ml

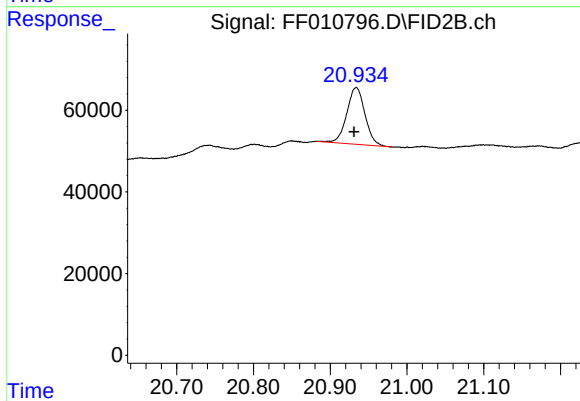

#17 N-OCTATRIACONTANE

R.T.: 20.934 min
Delta R.T.: 0.003 min
Response: 226396
Conc: 2.96 ug/ml

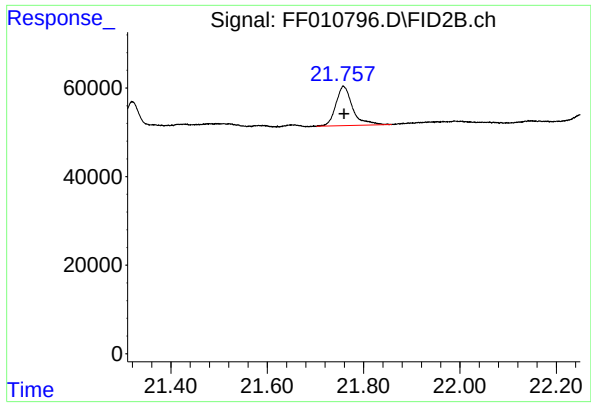

#18 N-TETRACONTANE

R.T.: 21.758 min
Delta R.T.: 0.000 min
Response: 214561
Conc: 2.75 ug/ml

Instrument :
FID_F
ClientSampleId :