

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
 Data File : FF010799.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jun 2022 17:47
 Operator : AJ\MA
 Sample : N3373-12
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 23:21:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.820	1495985	13.235 ug/ml
Target Compounds			
3) N-DODECANE	6.555	1727950	14.219 ug/ml
8) N-DOCOSANE	13.920	1186233	9.393 ug/ml
10) N-TETRACOSANE	15.023	1241906	9.908 ug/ml
11) N-HEXACOSANE	16.043	1761353	13.905 ug/ml
12) N-OCTACOSANE	16.993	2828633	23.178 ug/ml
13) N-TRIACONTANE	17.880	3223139	26.299 ug/ml
14) N-DOTRIACONTANE	18.709	2281480	18.802 ug/ml
15) N-TETRATRIACONTANE	19.491	1388588	13.361 ug/ml
16) N-HEXATRIACONTANE	20.227	745800	8.672 ug/ml
17) N-OCTATRIACONTANE	20.931	507046	6.621 ug/ml
18) N-TETRACONTANE	21.756	466773	5.974 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
Data File : FF010799.D
Signal(s) : FID2B.ch
Acq On : 17 Jun 2022 17:47
Operator : AJ\MA
Sample : N3373-12
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:21:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

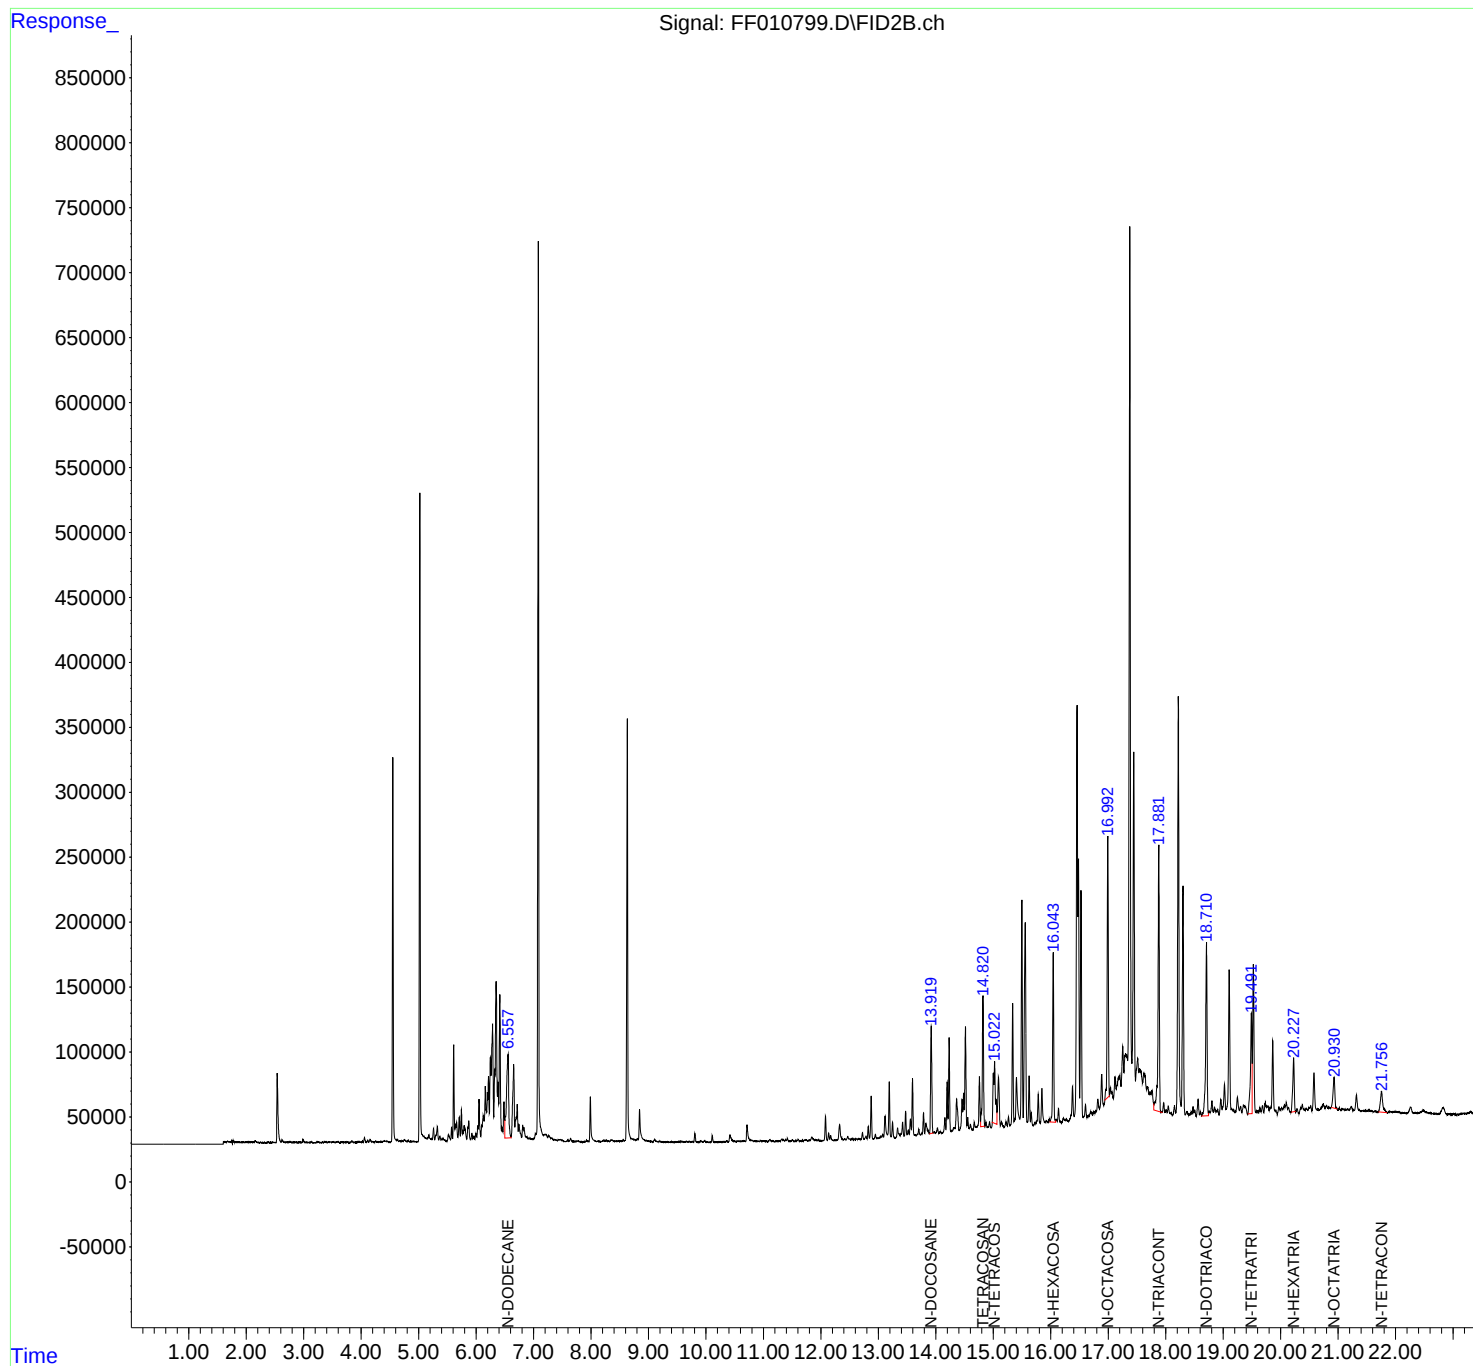


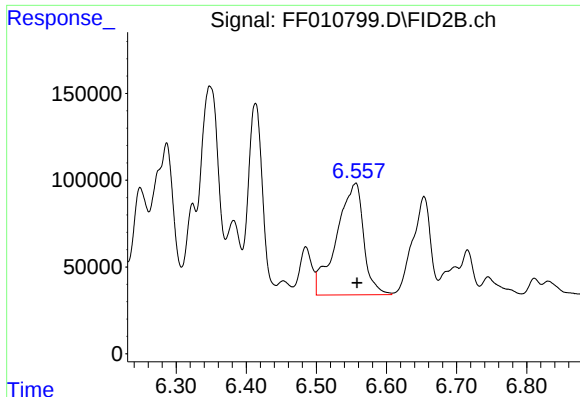

#3 N-DODECANE


R.T.: 6.555 min
Delta R.T.: -0.003 min
Response: 1727950
Conc: 14.22 ug/ml

Instrument :
FID_F
ClientSampleId :

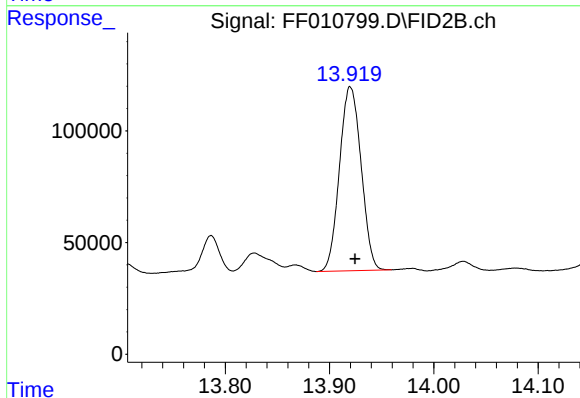


#8 N-DOCOSANE

R.T.: 13.920 min
Delta R.T.: -0.004 min
Response: 1186233
Conc: 9.39 ug/ml

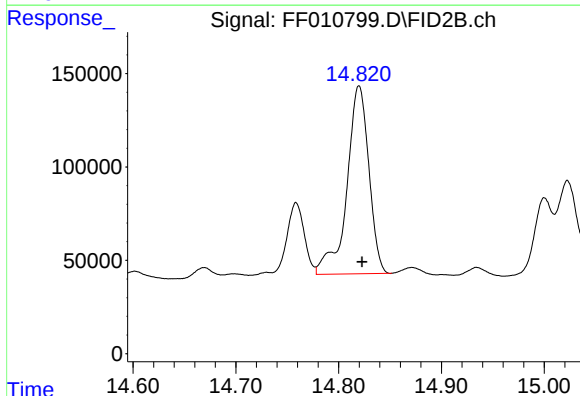


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.820 min
Delta R.T.: -0.003 min
Response: 1495985
Conc: 13.23 ug/ml

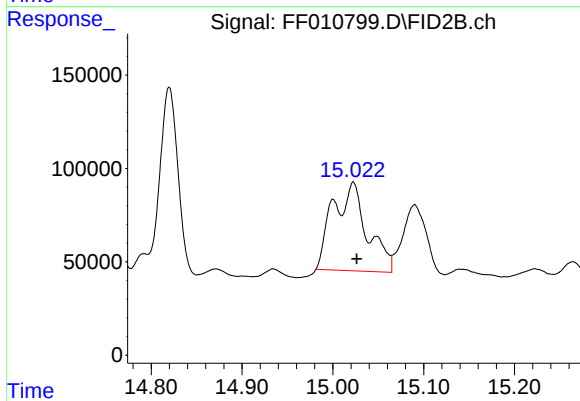

#10 N-TETRACOSANE


R.T.: 15.023 min
Delta R.T.: -0.004 min
Response: 1241906
Conc: 9.91 ug/ml

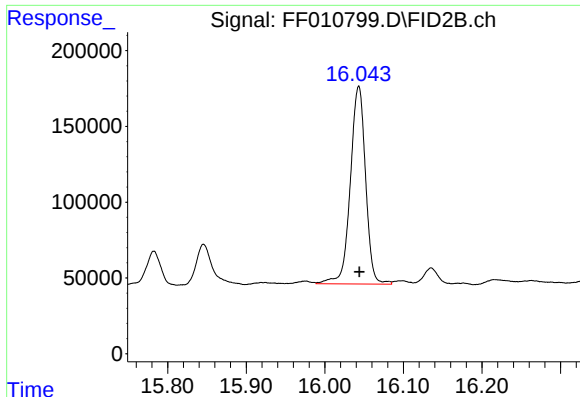

#11 N-HEXACOSANE


R.T.: 16.043 min
Delta R.T.: -0.001 min
Response: 1761353
Conc: 13.91 ug/ml

Instrument :
FID_F
ClientSampleId :

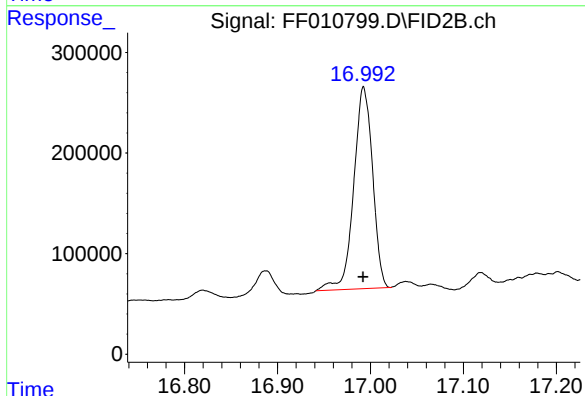


#12 N-OCTACOSANE

R.T.: 16.993 min
Delta R.T.: 0.000 min
Response: 2828633
Conc: 23.18 ug/ml

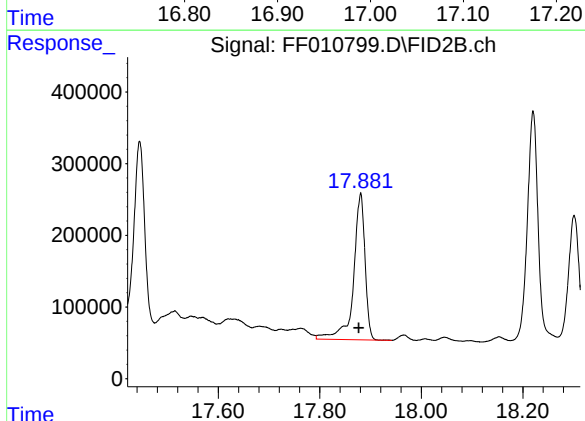


#13 N-TRIACONTANE

R.T.: 17.880 min
Delta R.T.: 0.003 min
Response: 3223139
Conc: 26.30 ug/ml

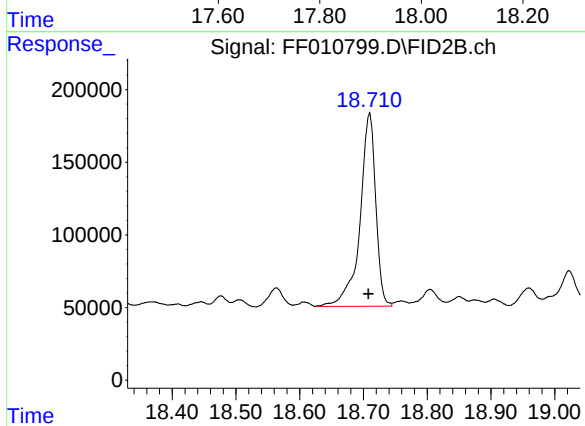

#14 N-DOTRIACONTANE


R.T.: 18.709 min
Delta R.T.: 0.002 min
Response: 2281480
Conc: 18.80 ug/ml

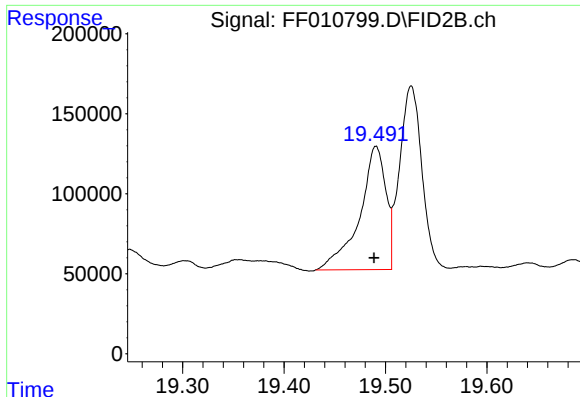

#15 N-TETRATRIACONTANE


R.T.: 19.491 min
Delta R.T.: 0.002 min
Response: 1388588
Conc: 13.36 ug/ml

Instrument :
FID_F
ClientSampleId :

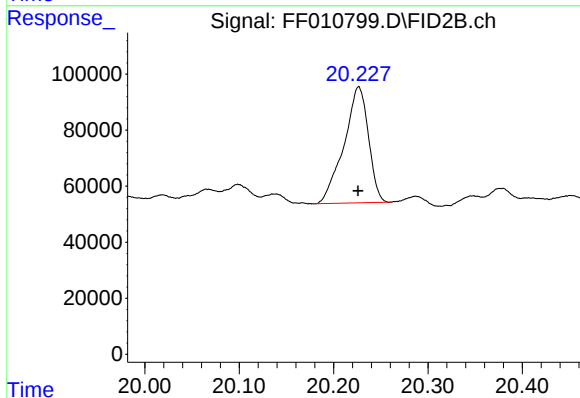


#16 N-HEXATRIACONTANE

R.T.: 20.227 min
Delta R.T.: 0.000 min
Response: 745800
Conc: 8.67 ug/ml

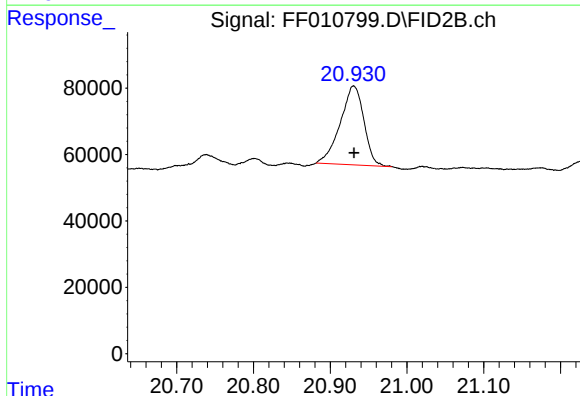

#17 N-OCTATRIACONTANE

R.T.: 20.931 min
Delta R.T.: 0.000 min
Response: 507046
Conc: 6.62 ug/ml

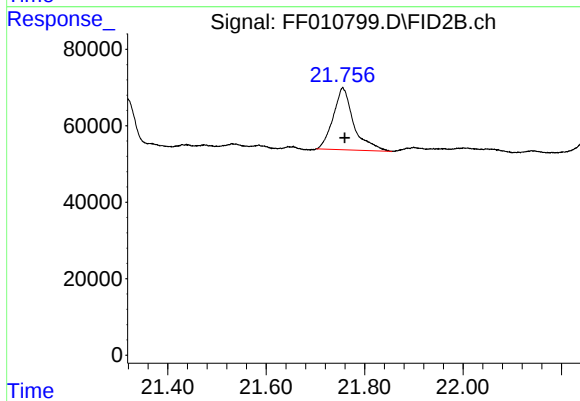

#18 N-TETRACONTANE

R.T.: 21.756 min
Delta R.T.: -0.004 min
Response: 466773
Conc: 5.97 ug/ml