

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
 Data File : FF010800.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jun 2022 18:17
 Operator : AJ\MA
 Sample : N3373-13
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 17 23:21:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.821	1236626	10.940 ug/ml
Target Compounds			
7) N-EICOSANE	12.723	95663	0.756 ug/ml
8) N-DOCOSANE	13.922	297683	2.357 ug/ml
10) N-TETRACOSANE	15.022	552220	4.406 ug/ml
11) N-HEXACOSANE	16.044	1940182	15.317 ug/ml
12) N-OCTACOSANE	16.994	3166196	25.944 ug/ml
13) N-TRIACONTANE	17.879	2210629	18.037 ug/ml
14) N-DOTRIACONTANE	18.708	971324	8.005 ug/ml
15) N-TETRATRIACONTANE	19.489	407445	3.920 ug/ml
16) N-HEXATRIACONTANE	20.227	182554	2.123 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
Data File : FF010800.D
Signal(s) : FID2B.ch
Acq On : 17 Jun 2022 18:17
Operator : AJ\MA
Sample : N3373-13
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 17 23:21:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

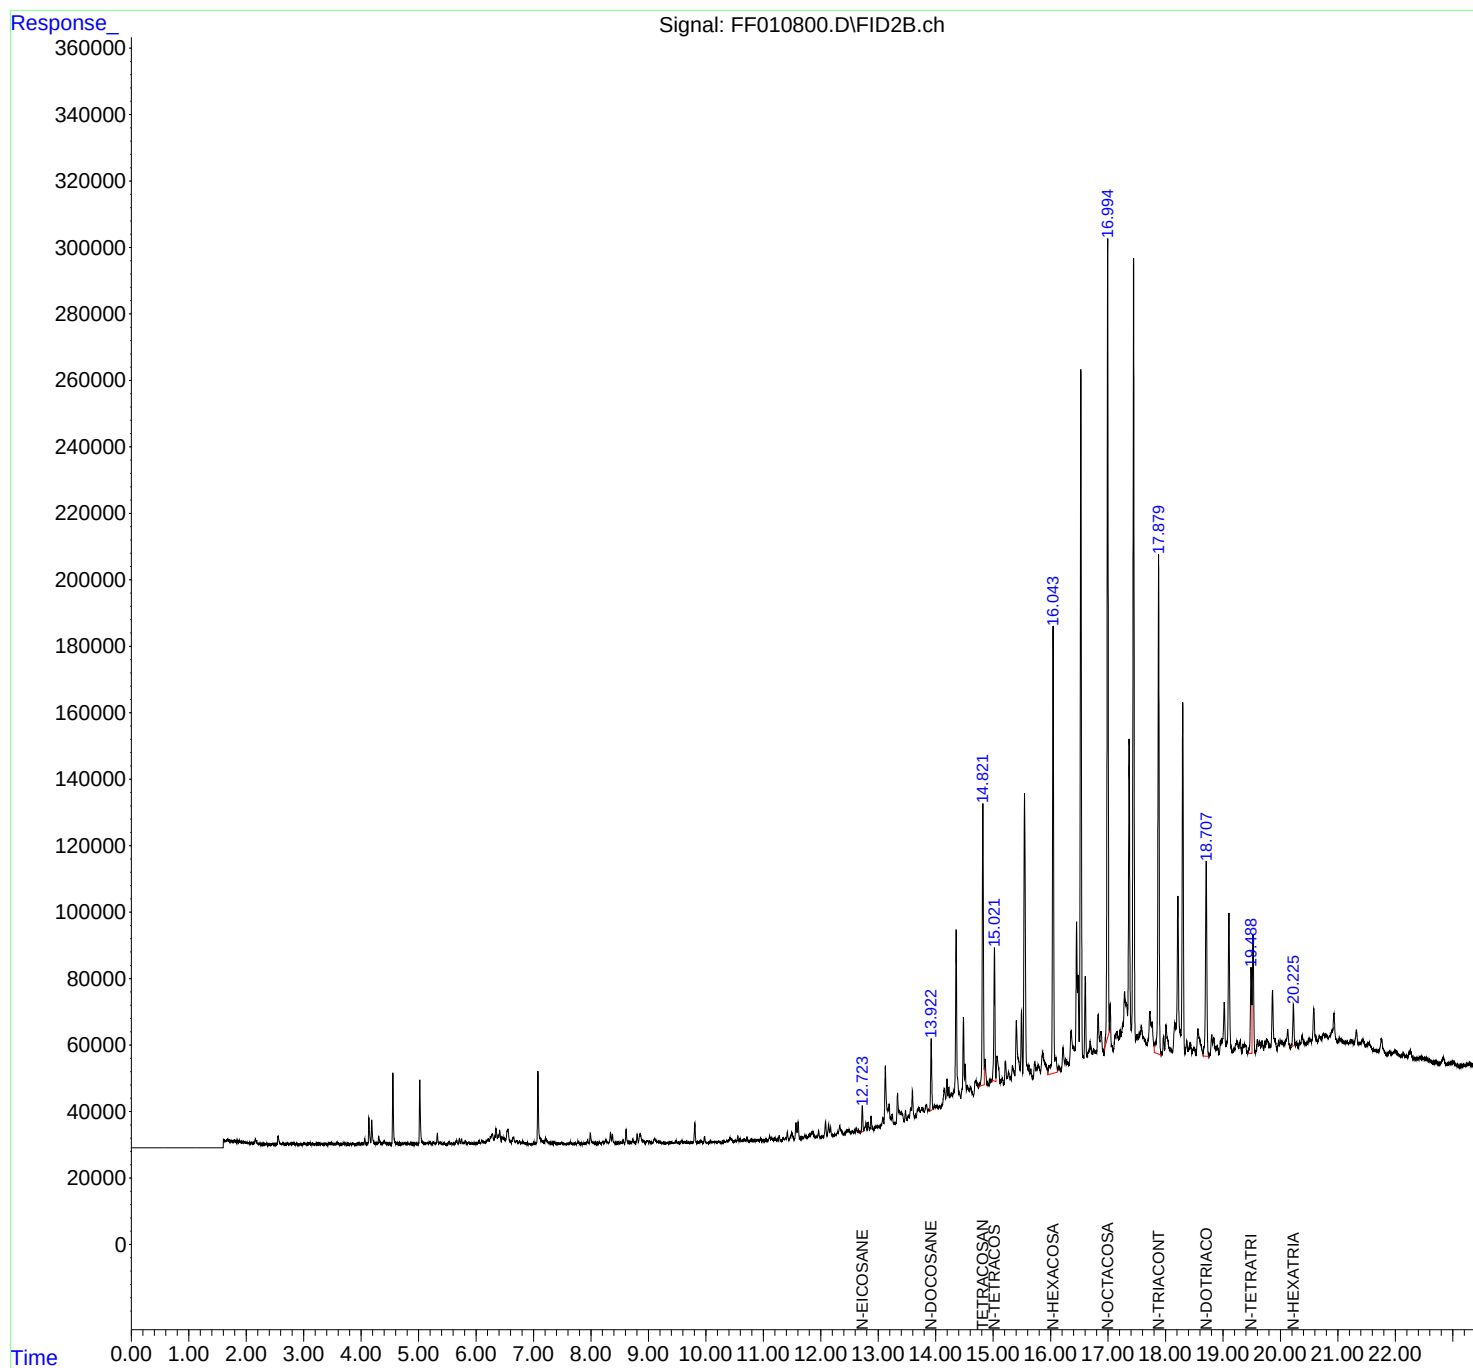


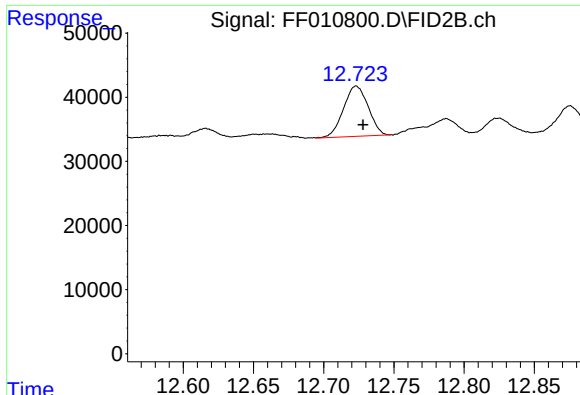

#7 N-EICOSANE


R.T.: 12.723 min
Delta R.T.: -0.005 min
Response: 95663
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

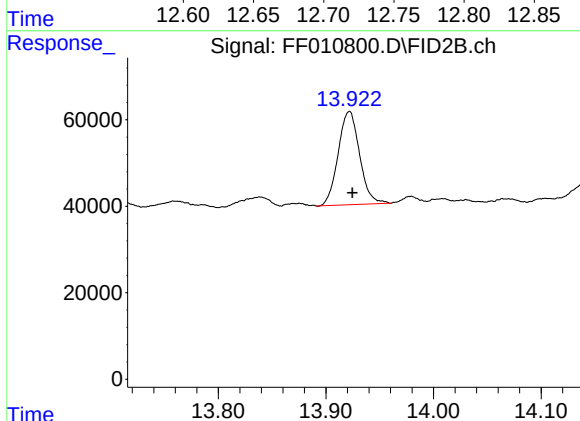


#8 N-DOCOSANE

R.T.: 13.922 min
Delta R.T.: -0.003 min
Response: 297683
Conc: 2.36 ug/ml

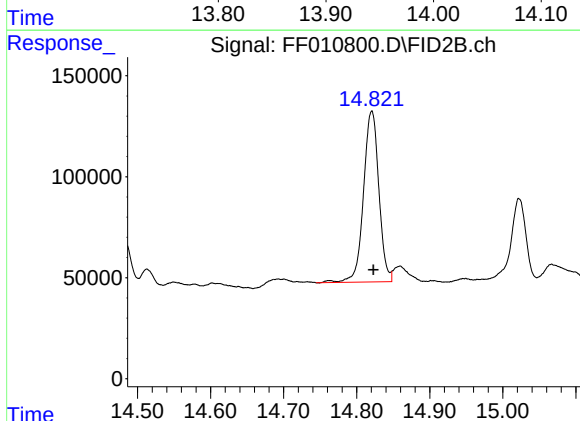


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.821 min
Delta R.T.: -0.002 min
Response: 1236626
Conc: 10.94 ug/ml

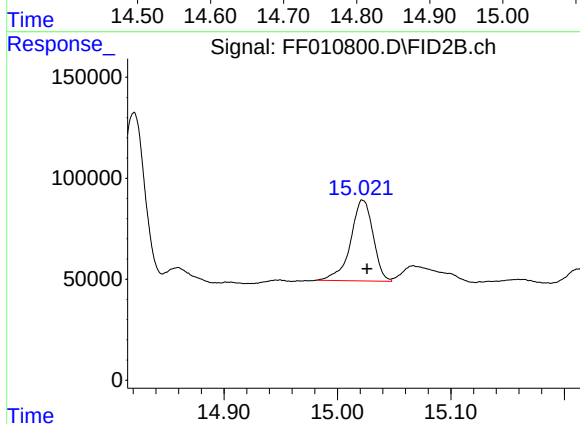

#10 N-TETRACOSANE


R.T.: 15.022 min
Delta R.T.: -0.004 min
Response: 552220
Conc: 4.41 ug/ml

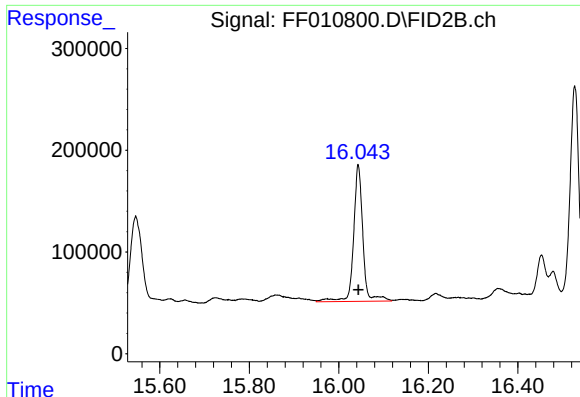

#11 N-HEXACOSANE


R.T.: 16.044 min
Delta R.T.: 0.000 min
Response: 1940182
Conc: 15.32 ug/ml

Instrument :
FID_F
ClientSampleId :

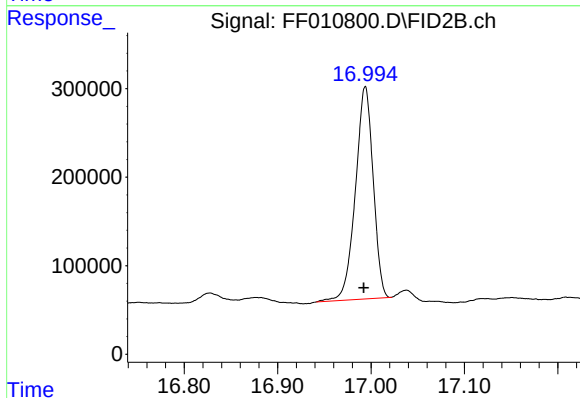


#12 N-OCTACOSANE

R.T.: 16.994 min
Delta R.T.: 0.002 min
Response: 3166196
Conc: 25.94 ug/ml

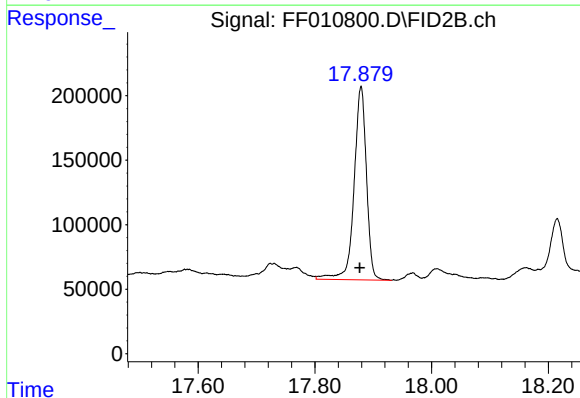


#13 N-TRIACONTANE

R.T.: 17.879 min
Delta R.T.: 0.002 min
Response: 2210629
Conc: 18.04 ug/ml

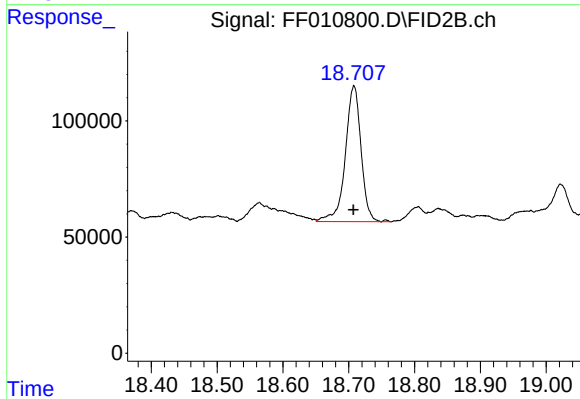

#14 N-DOTRIACONTANE


R.T.: 18.708 min
Delta R.T.: 0.000 min
Response: 971324
Conc: 8.00 ug/ml

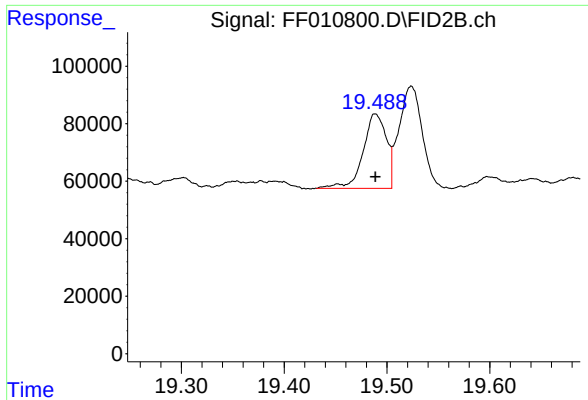

#15 N-TETRATRIACONTANE

R.T.: 19.489 min
Delta R.T.: 0.000 min
Response: 407445
Conc: 3.92 ug/ml

Instrument :
FID_F
ClientSampleId :

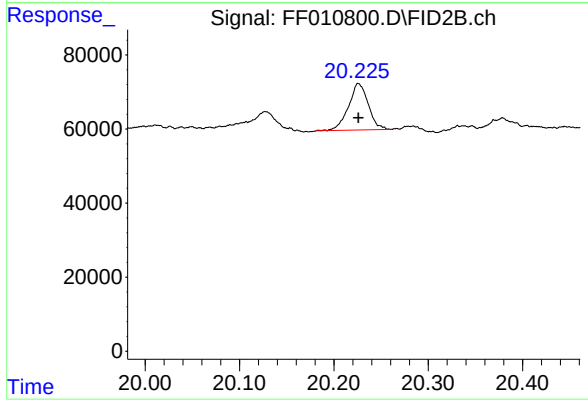

#16 N-HEXATRIACONTANE

R.T.: 20.227 min
Delta R.T.: 0.000 min
Response: 182554
Conc: 2.12 ug/ml