

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
 Data File : FF010796.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jun 2022 15:57
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: Sample.e
 Quant Time: Jun 17 23:19:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
 Quant Title :
 QLast Update : Tue Jun 07 09:12:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3)	N-DODECANE	6.553	3072082 25.279 ug/ml
12)	N-OCTACOSANE	16.993	3134472 25.684 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061722\
Data File : FF010796.D
Signal(s) : FID2B.ch
Acq On : 17 Jun 2022 15:57
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Jun 17 23:19:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 09:12:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

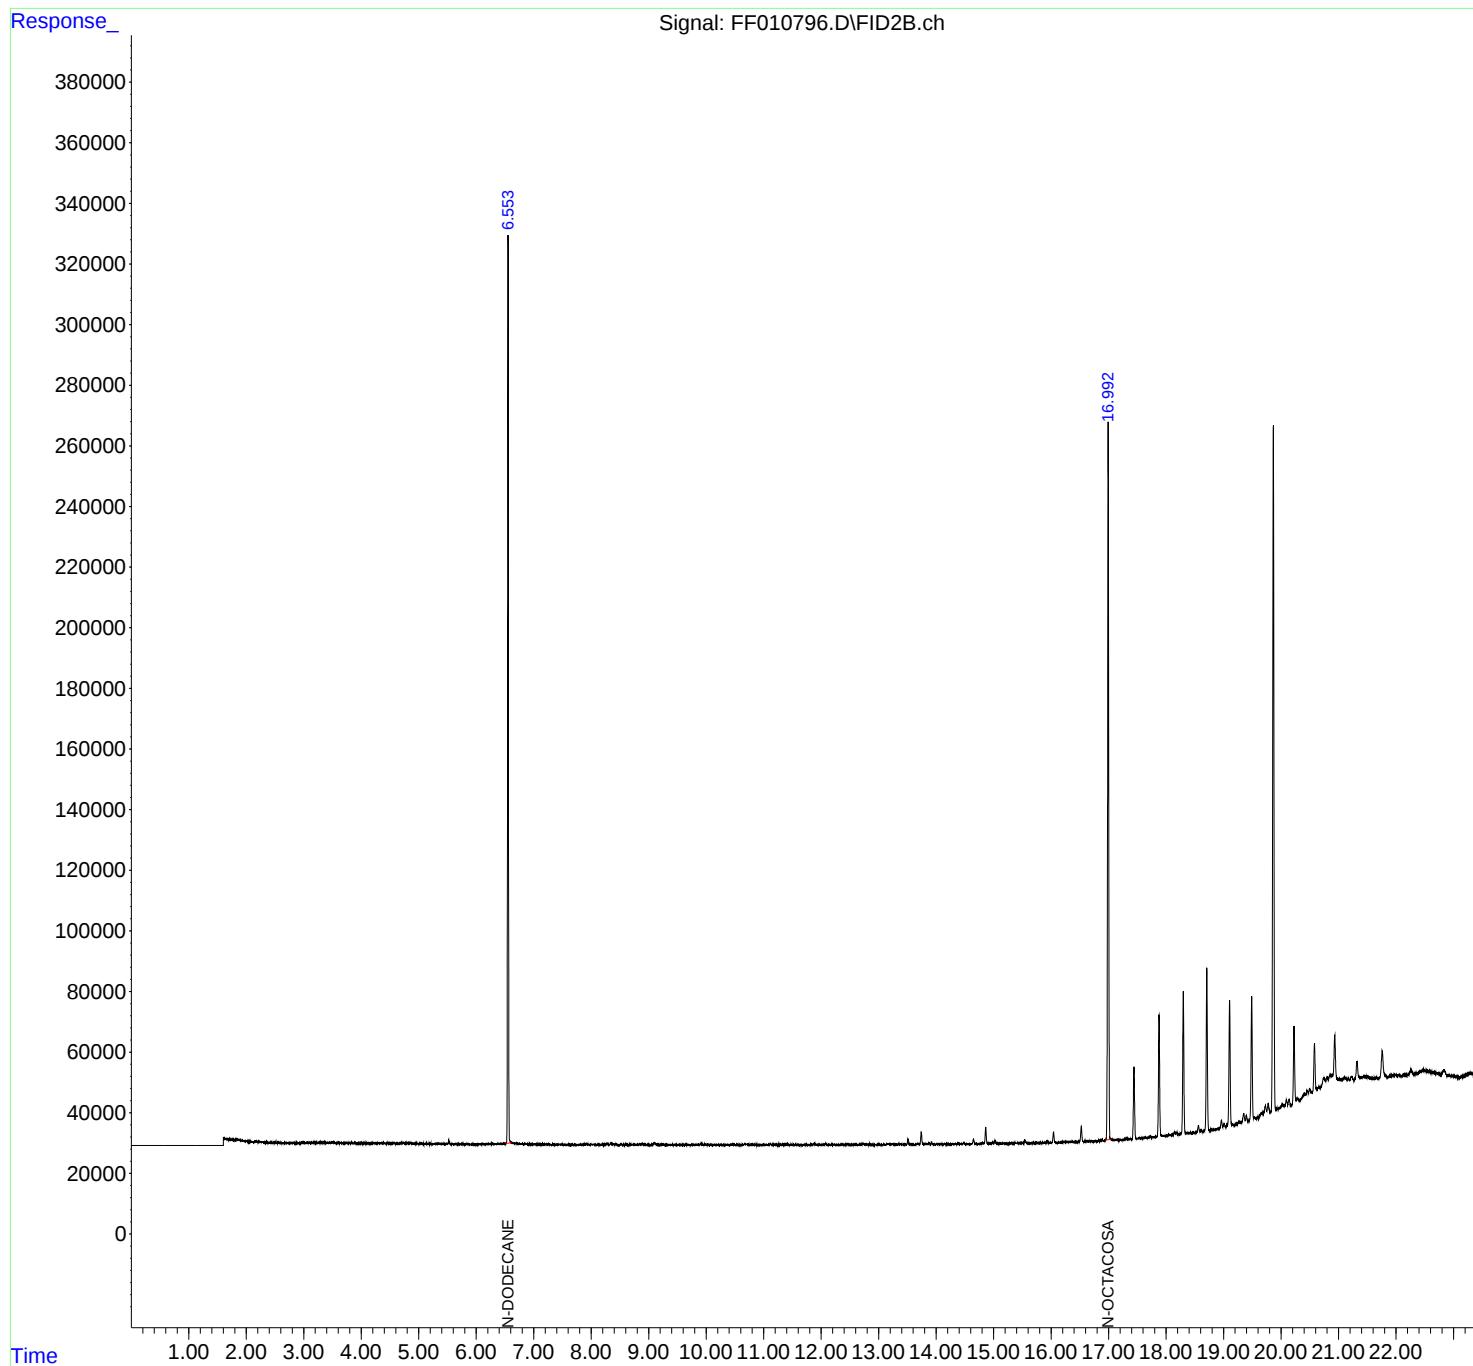


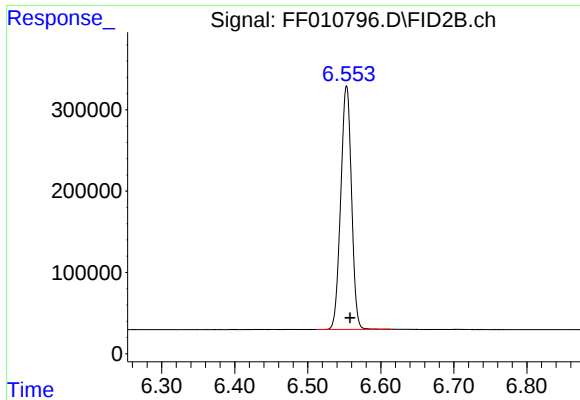

#3 N-DODECANE


R.T.: 6.553 min
Delta R.T.: -0.005 min
Response: 3072082
Conc: 25.28 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

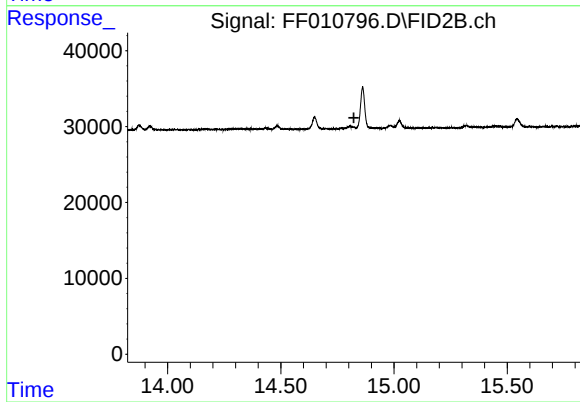

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.823 min
Response: 0
Conc: N.D.

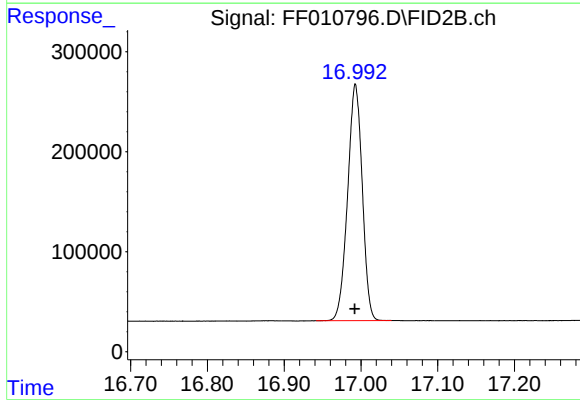

#12 N-OCTACOSANE

R.T.: 16.993 min
Delta R.T.: 0.000 min
Response: 3134472
Conc: 25.68 ug/ml