

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000976.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 12:00
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:17:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.257	3363807	24.001 ug/ml
12)	N-OCTACOSANE	16.653	3136878	24.669 ug/ml
13)	N-TRIACONTANE	17.537	201058	1.592 ug/ml
14)	N-DOTRIACONTANE	18.368	272295	2.220 ug/ml
15)	N-TETRATRIACONTANE	19.152	192240	1.602 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000976.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 12:00
Operator : UA\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:17:08 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

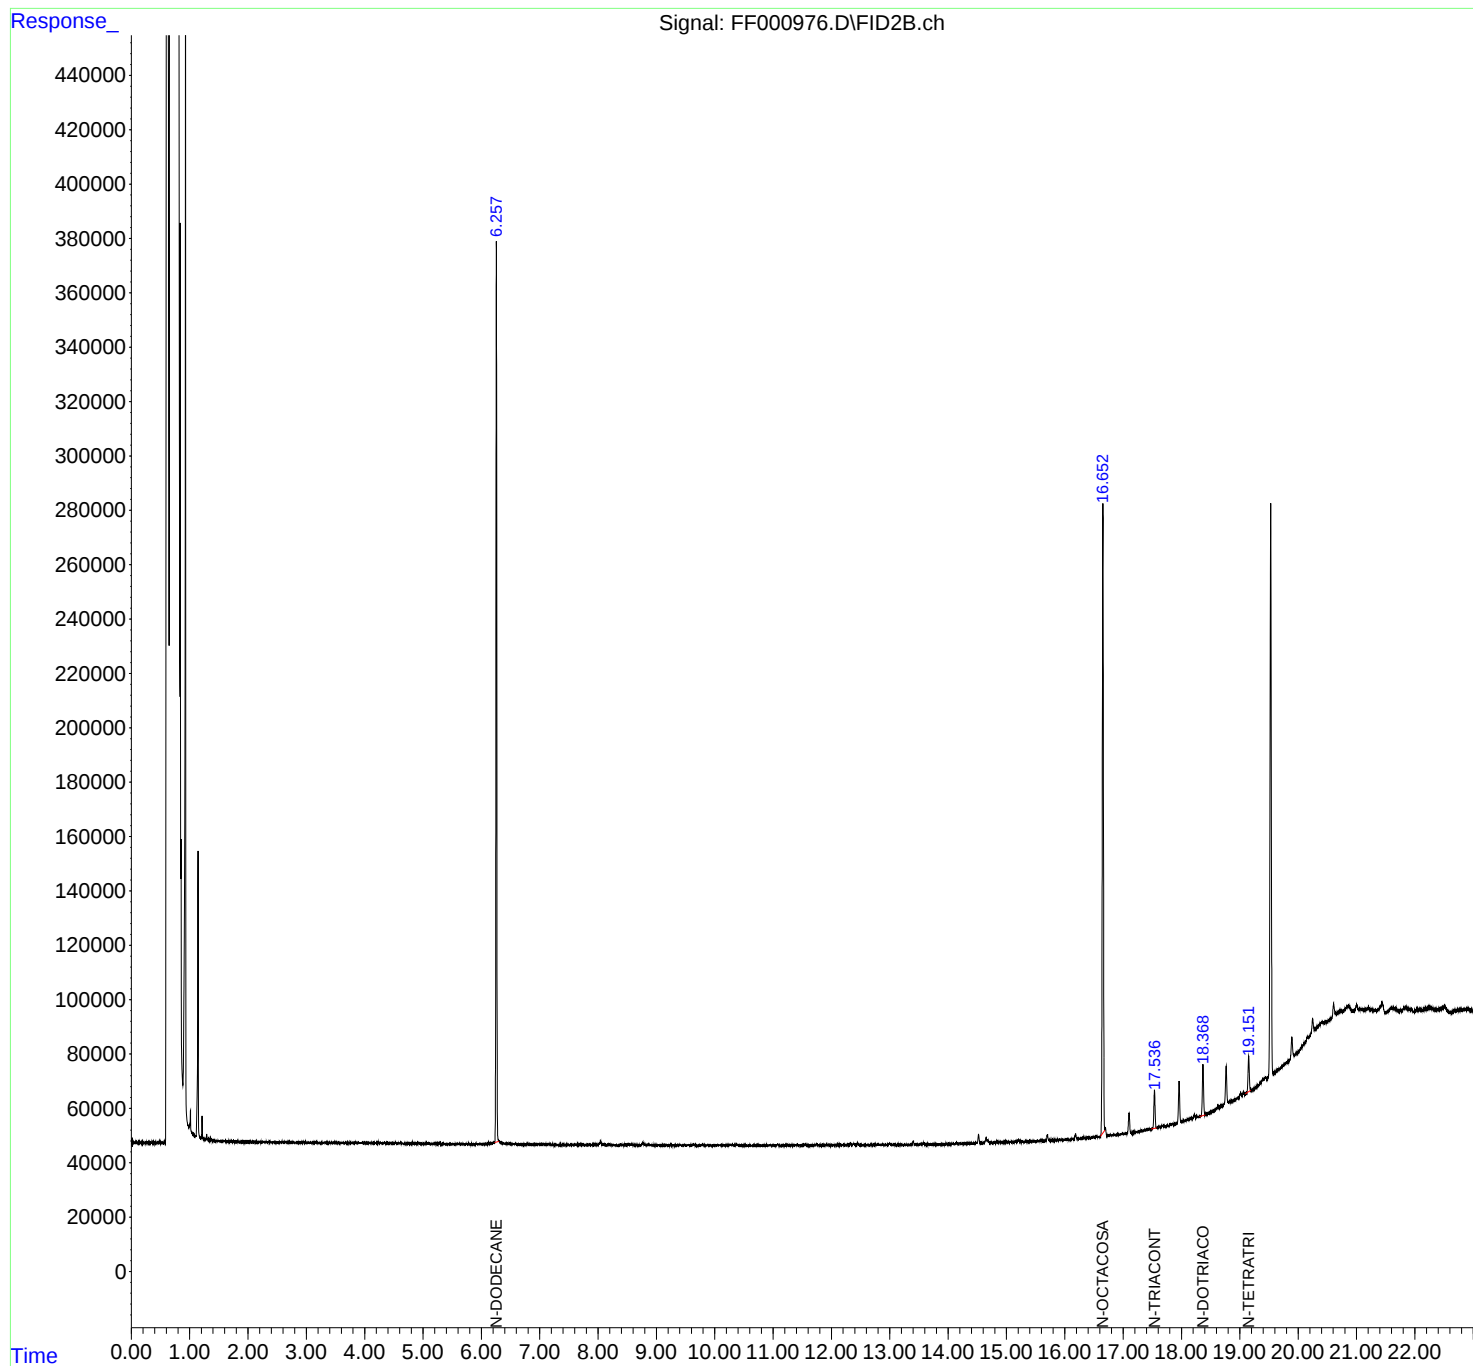


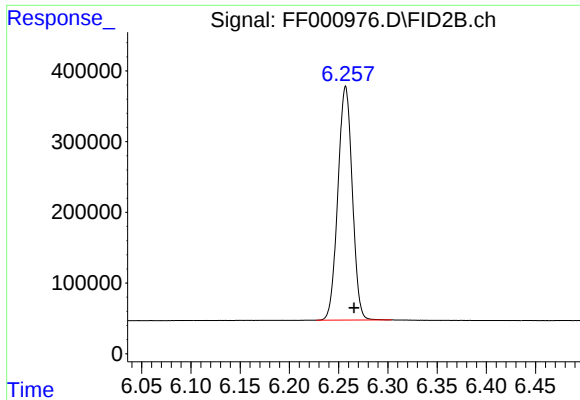

#3 N-DODECANE


R.T.: 6.257 min
Delta R.T.: -0.009 min
Response: 3363807
Conc: 24.00 ug/ml

Instrument :
FID_F
ClientSampleId :

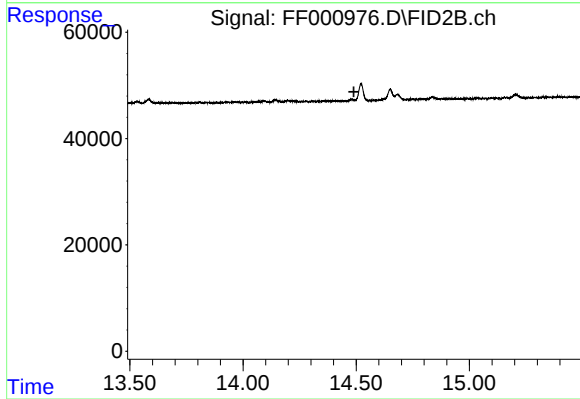


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.490 min
Response: 0
Conc: N.D.

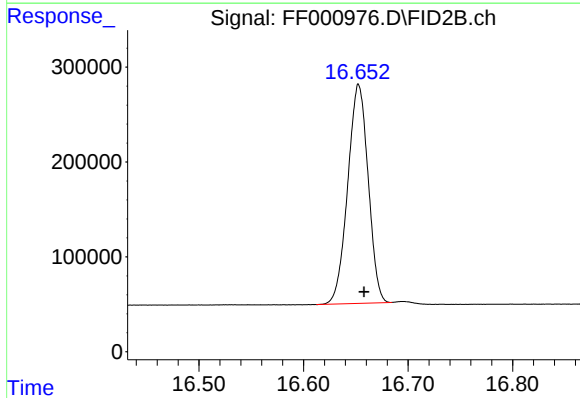


#12 N-OCTACOSANE

R.T.: 16.653 min
Delta R.T.: -0.005 min
Response: 3136878
Conc: 24.67 ug/ml

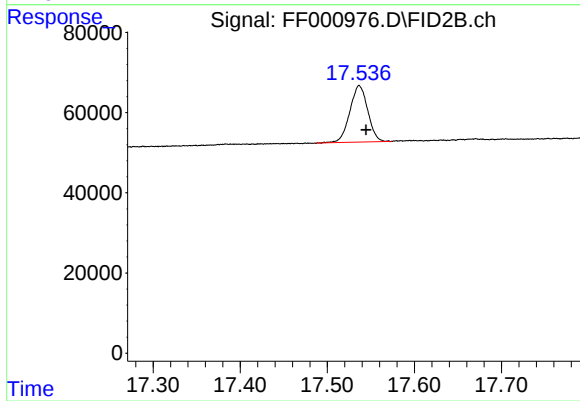

#13 N-TRIACONTANE


R.T.: 17.537 min
Delta R.T.: -0.008 min
Response: 201058
Conc: 1.59 ug/ml

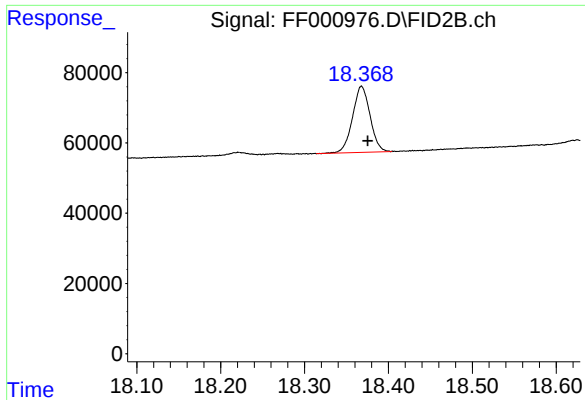

#14 N-DOTRIACONTANE

R.T.: 18.368 min
Delta R.T.: -0.008 min
Response: 272295
Conc: 2.22 ug/ml

Instrument :
FID_F
ClientSampleId :

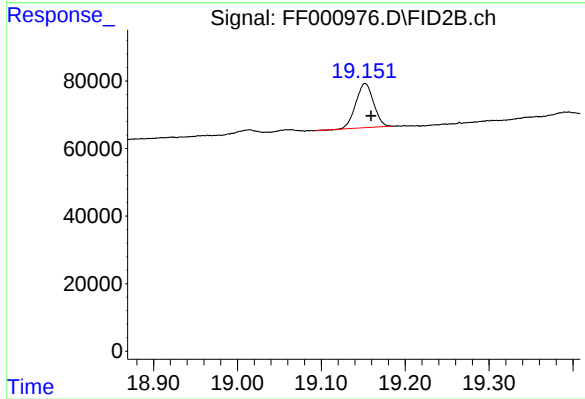

#15 N-TETRATRIACONTANE

R.T.: 19.152 min
Delta R.T.: -0.007 min
Response: 192240
Conc: 1.60 ug/ml