

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF000980.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2018 14:21
 Operator : UA\AJ
 Sample : J3240-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:18:10 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.483	1627712	14.114 ug/ml
Target Compounds			
4) N-TETRADECANE	8.100	977638	7.022 ug/ml
5) N-HEXADECANE	9.639	235146	1.705 ug/ml
6) N-OCTADECANE	11.078	199323	1.460 ug/ml
7) N-EICOSANE	12.385	210334	1.570 ug/ml
8) N-DOCOSANE	13.586	137710	1.041 ug/ml
10) N-TETRACOSANE	14.650	767226	5.915 ug/ml
12) N-OCTACOSANE	16.657	437080	3.437 ug/ml
13) N-TRIACONTANE	17.549	936965	7.420 ug/ml
14) N-DOTRIACONTANE	18.370	1104249	9.003 ug/ml
15) N-TETRATRIACONTANE	19.180	1135438	9.461 ug/ml
16) N-HEXATRIACONTANE	19.910	409819	3.589 ug/ml
18) N-TETRACONTANE	21.467	330260	3.225 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000980.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 14:21
Operator : UA\AJ
Sample : J3240-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:18:10 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

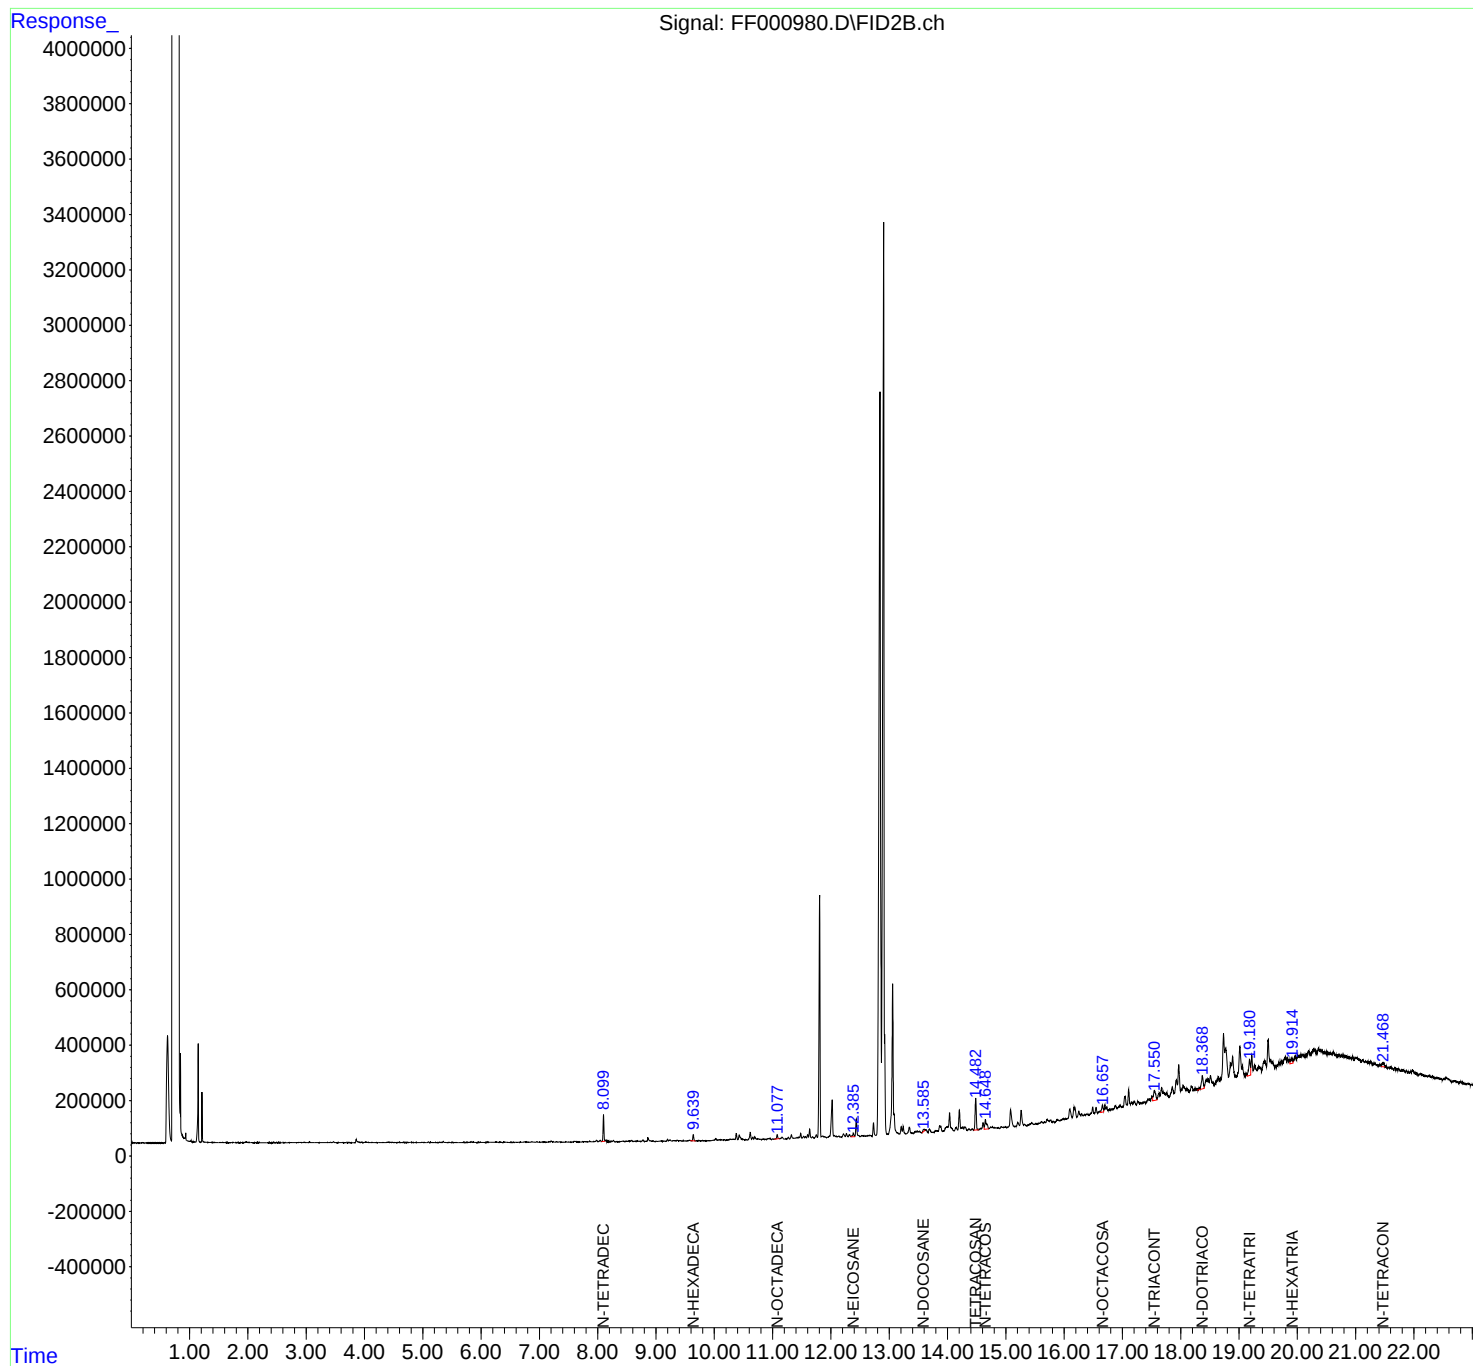


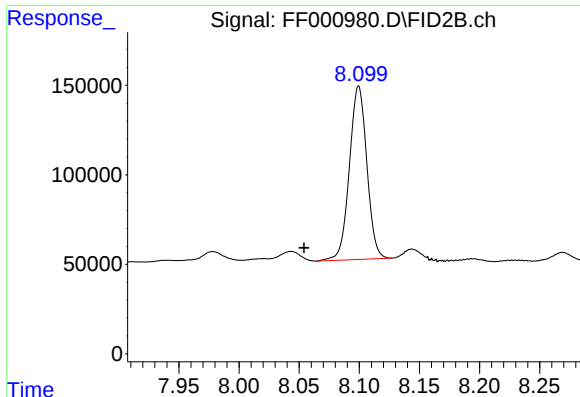

#4 N-TETRADECANE


R.T.: 8.100 min
Delta R.T.: 0.045 min
Response: 977638
Conc: 7.02 ug/ml

Instrument :
FID_F
ClientSampleId :

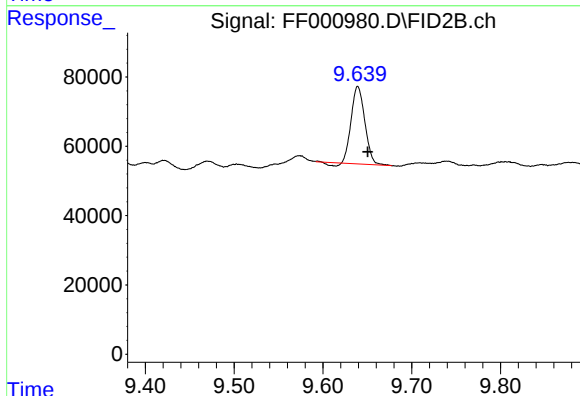


#5 N-HEXADECANE

R.T.: 9.639 min
Delta R.T.: -0.011 min
Response: 235146
Conc: 1.71 ug/ml

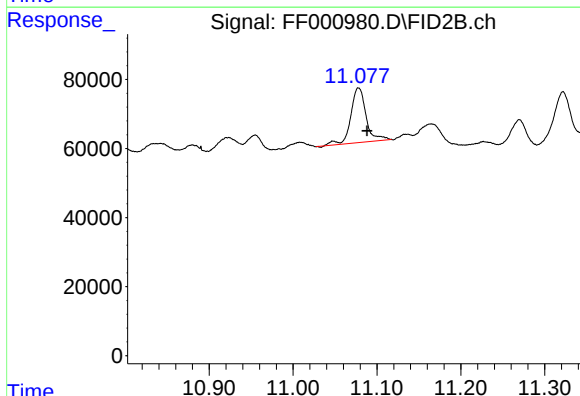


#6 N-OCTADECANE

R.T.: 11.078 min
Delta R.T.: -0.010 min
Response: 199323
Conc: 1.46 ug/ml

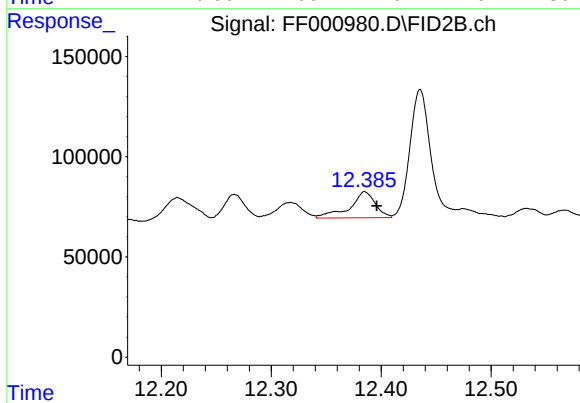

#7 N-EICOSANE


R.T.: 12.385 min
Delta R.T.: -0.011 min
Response: 210334
Conc: 1.57 ug/ml

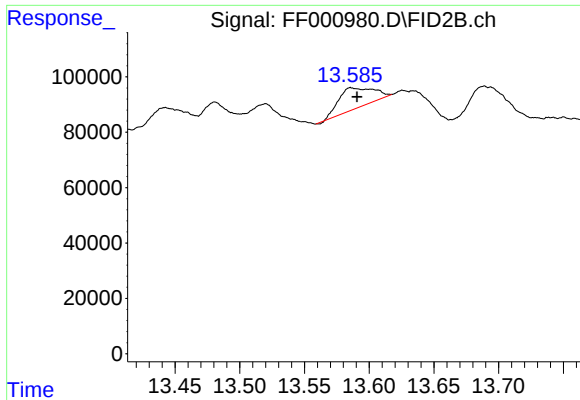

#8 N-DOCOSANE


R.T.: 13.586 min
Delta R.T.: -0.004 min
Response: 137710
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :

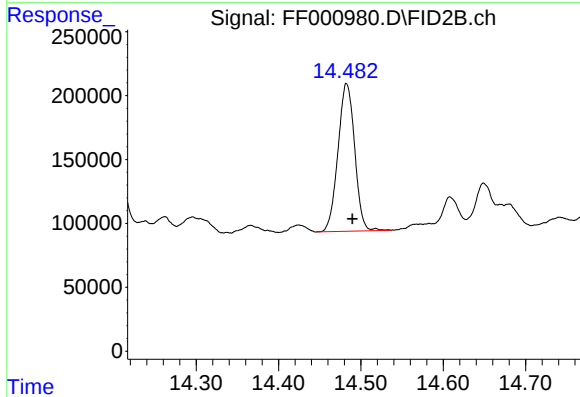


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.483 min
Delta R.T.: -0.007 min
Response: 1627712
Conc: 14.11 ug/ml

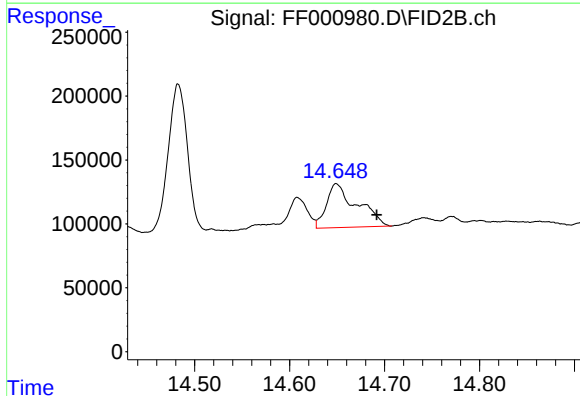


#10 N-TETRACOSANE

R.T.: 14.650 min
Delta R.T.: -0.042 min
Response: 767226
Conc: 5.91 ug/ml

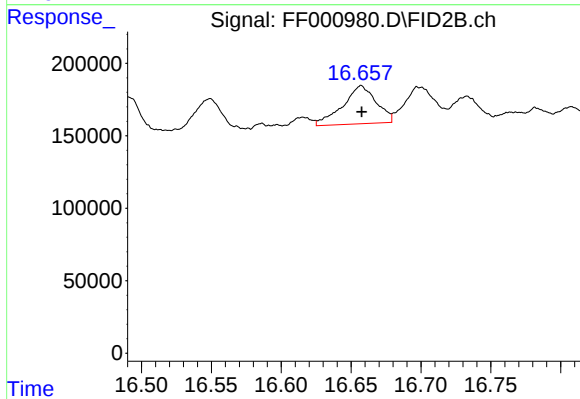

#12 N-OCTACOSANE


R.T.: 16.657 min
Delta R.T.: 0.000 min
Response: 437080
Conc: 3.44 ug/ml

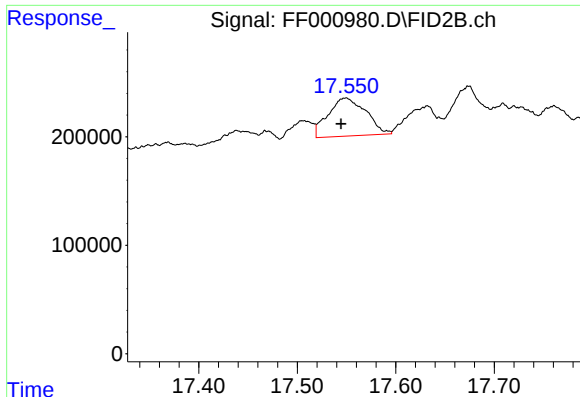

#13 N-TRIACONTANE


R.T.: 17.549 min
Delta R.T.: 0.004 min
Response: 936965
Conc: 7.42 ug/ml

Instrument :
FID_F
ClientSampleId :

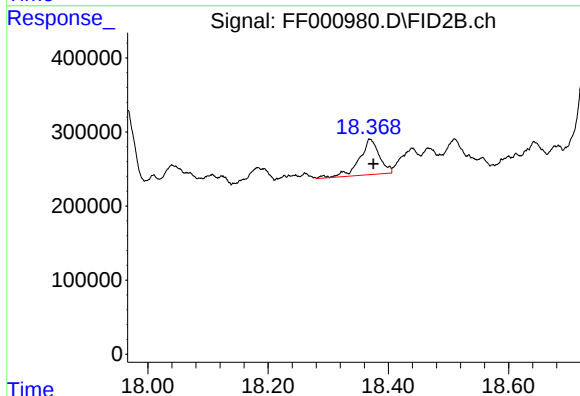


#14 N-DOTRIACONTANE

R.T.: 18.370 min
Delta R.T.: -0.005 min
Response: 1104249
Conc: 9.00 ug/ml

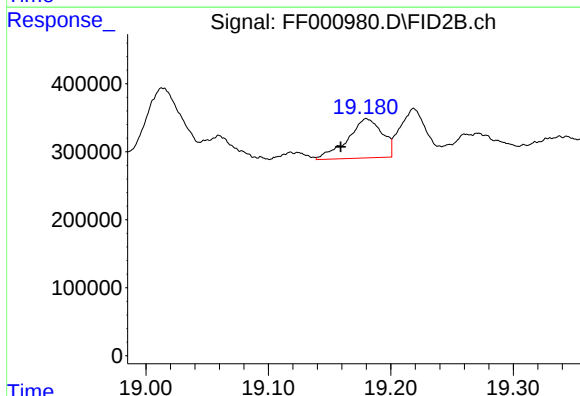


#15 N-TETRATRIACONTANE

R.T.: 19.180 min
Delta R.T.: 0.021 min
Response: 1135438
Conc: 9.46 ug/ml

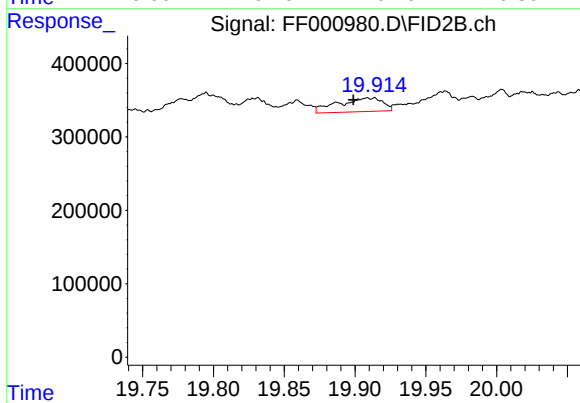

#16 N-HEXATRIACONTANE

R.T.: 19.910 min
Delta R.T.: 0.011 min
Response: 409819
Conc: 3.59 ug/ml

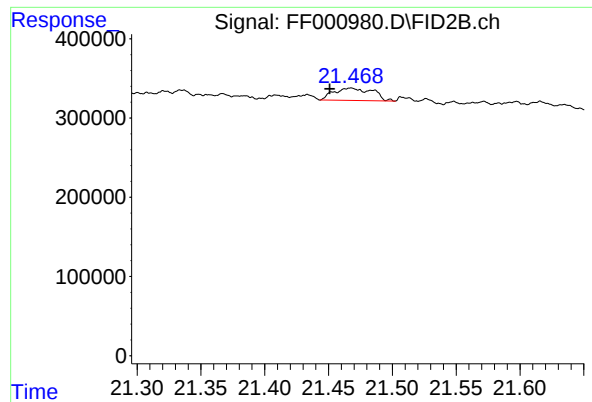

#18 N-TETRACONTANE

R.T.: 21.467 min
Delta R.T.: 0.016 min
Response: 330260
Conc: 3.22 ug/ml

Instrument :
FID_F
ClientSampleId :