

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF000981.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2018 14:51
 Operator : UA\AJ
 Sample : J3244-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:18:27 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.484	1922508	16.670 ug/ml
Target Compounds			
4) N-TETRADECANE	8.101	1003564	7.208 ug/ml
5) N-HEXADECANE	9.641	220611	1.600 ug/ml
7) N-EICOSANE	12.436	2257265	16.848 ug/ml
8) N-DOCOSANE	13.588	252023	1.906 ug/ml
10) N-TETRACOSANE	14.651	979664	7.553 ug/ml
11) N-HEXACOSANE	15.655f	125461	0.977 ug/ml
12) N-OCTACOSANE	16.652	566094	4.452 ug/ml
13) N-TRIACONTANE	17.542	754960	5.979 ug/ml
14) N-DOTRIACONTANE	18.357	1131141	9.222 ug/ml
15) N-TETRATRIACONTANE	19.175	587037	4.892 ug/ml
16) N-HEXATRIACONTANE	19.904	237639	2.081 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000981.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 14:51
Operator : UA\AJ
Sample : J3244-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 19 09:18:27 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

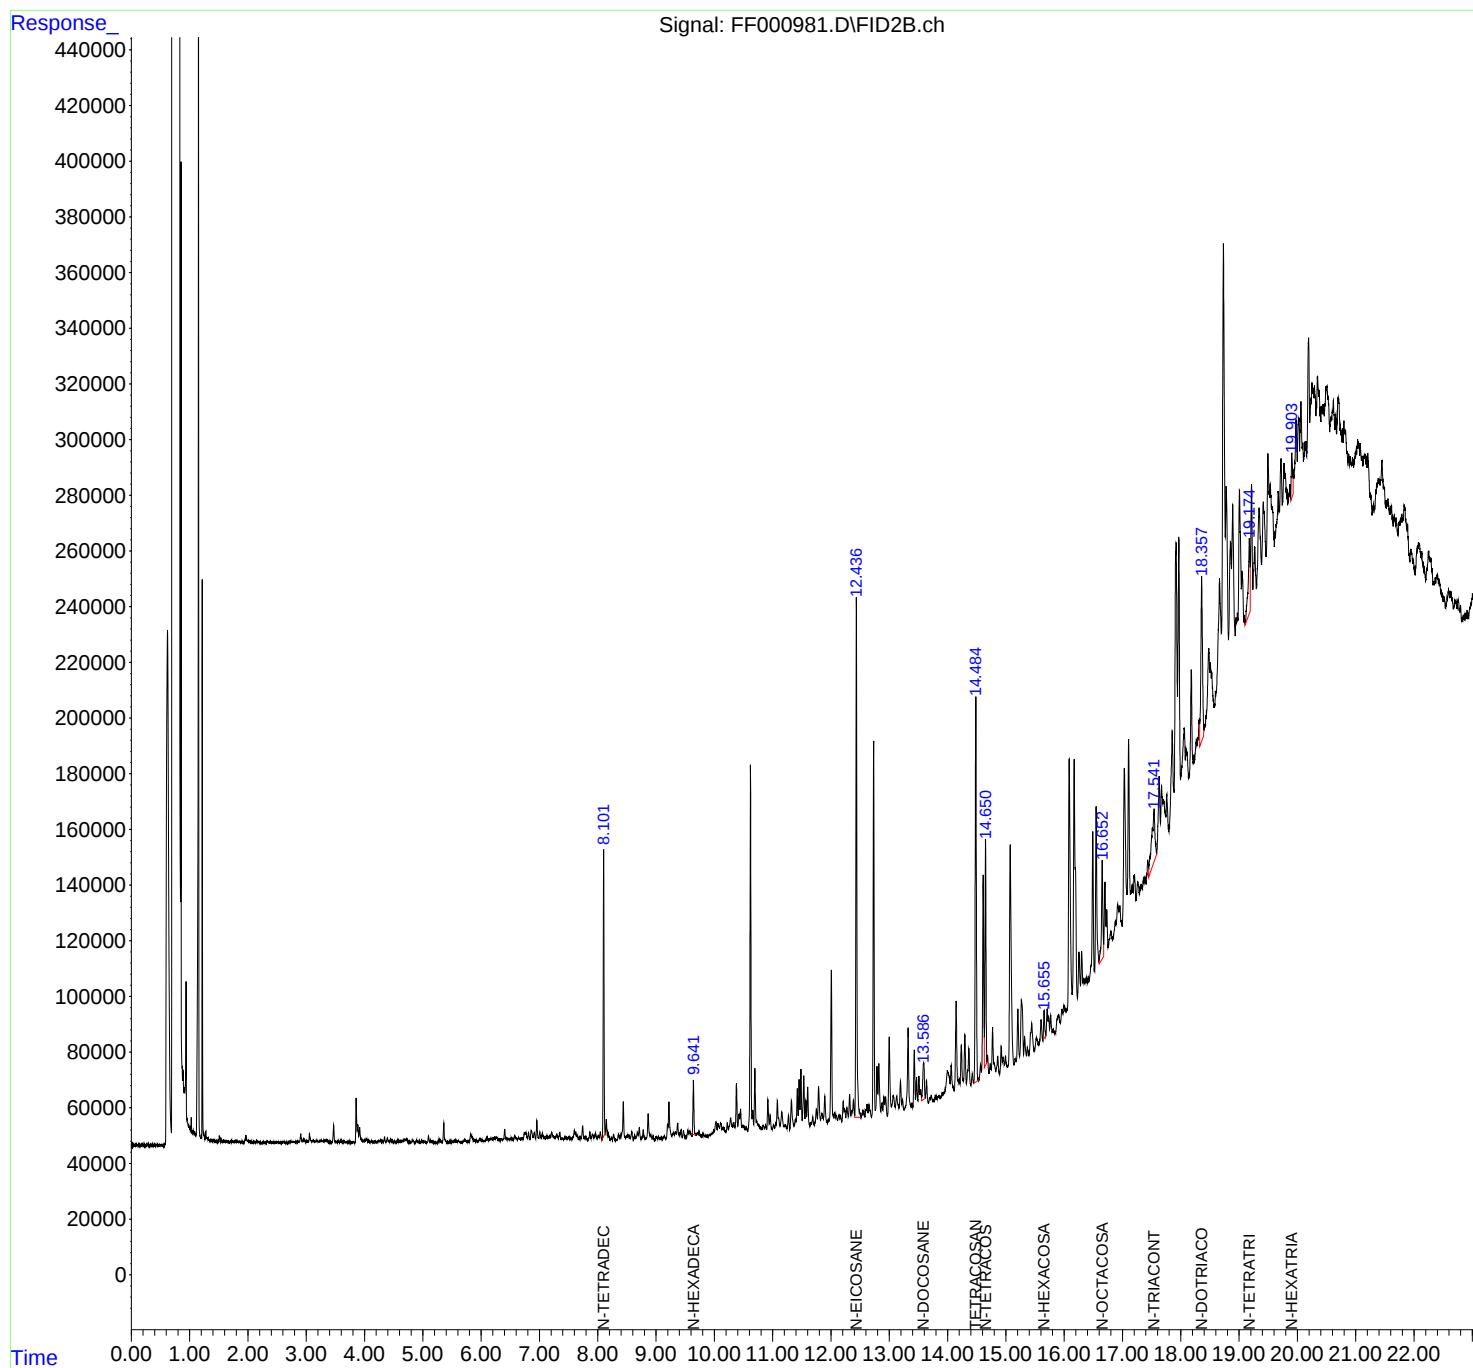


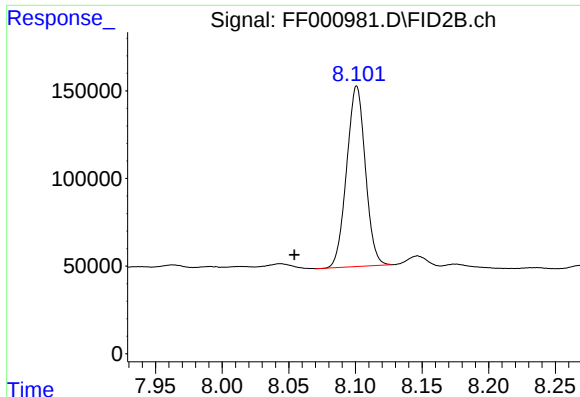

#4 N-TETRADECANE


R.T.: 8.101 min
Delta R.T.: 0.047 min
Response: 1003564
Conc: 7.21 ug/ml

Instrument :
FID_F
ClientSampleId :

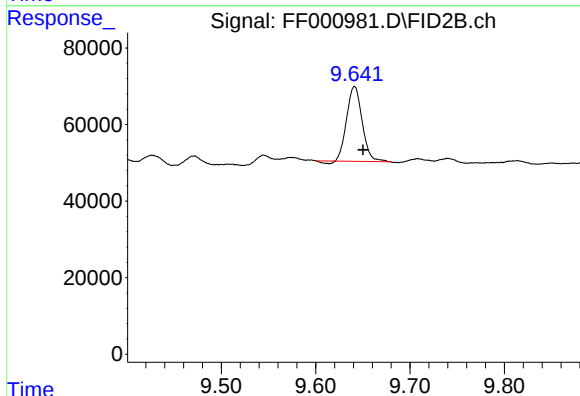


#5 N-HEXADECANE

R.T.: 9.641 min
Delta R.T.: -0.009 min
Response: 220611
Conc: 1.60 ug/ml

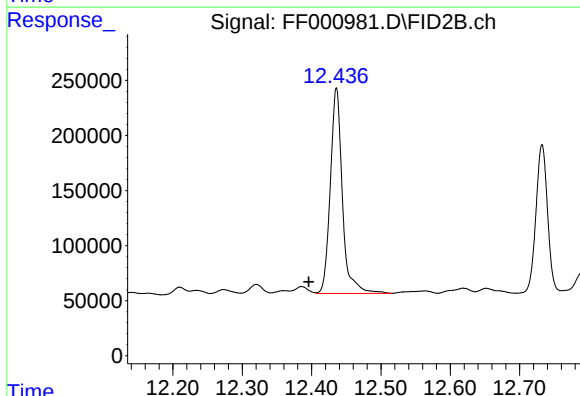


#7 N-EICOSANE

R.T.: 12.436 min
Delta R.T.: 0.040 min
Response: 2257265
Conc: 16.85 ug/ml

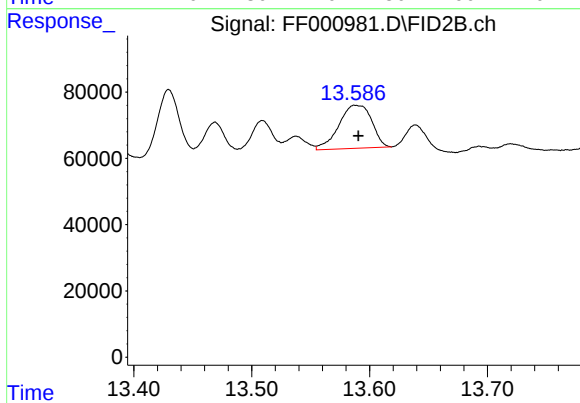

#8 N-DOCOSANE


R.T.: 13.588 min
Delta R.T.: -0.003 min
Response: 252023
Conc: 1.91 ug/ml

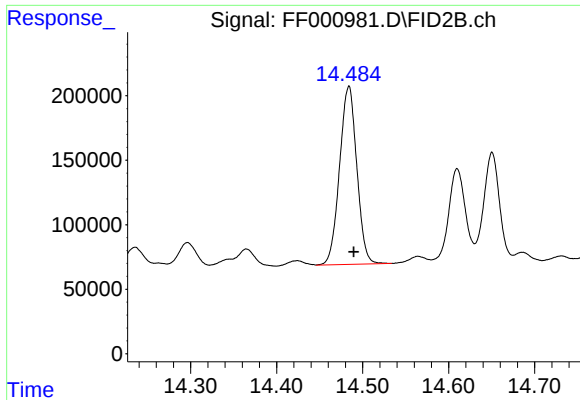

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.484 min
Delta R.T.: -0.006 min
Response: 1922508
Conc: 16.67 ug/ml

Instrument :
FID_F
ClientSampleId :

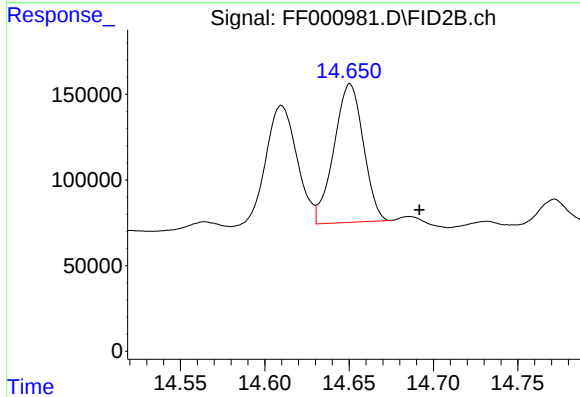


#10 N-TETRACOSANE

R.T.: 14.651 min
Delta R.T.: -0.041 min
Response: 979664
Conc: 7.55 ug/ml

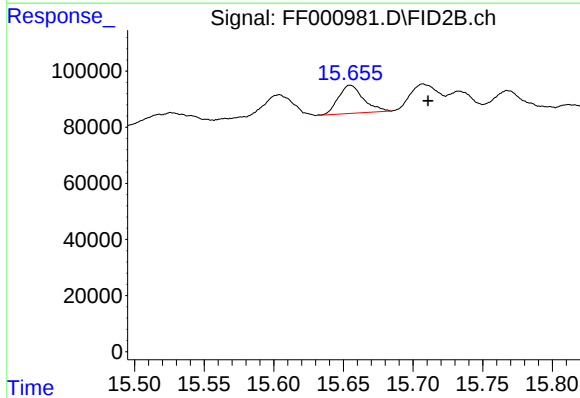


#11 N-HEXACOSANE

R.T.: 15.655 min
Delta R.T.: -0.056 min
Response: 125461
Conc: 0.98 ug/ml

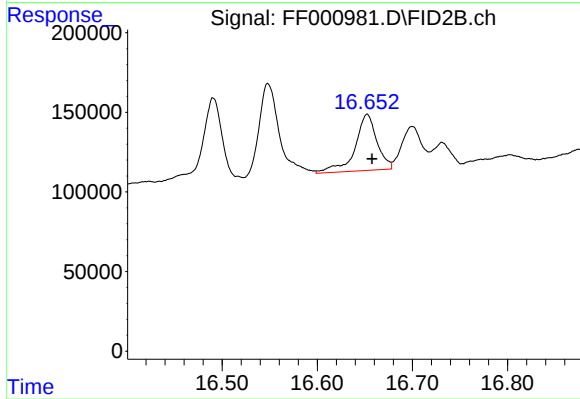

#12 N-OCTACOSANE


R.T.: 16.652 min
Delta R.T.: -0.005 min
Response: 566094
Conc: 4.45 ug/ml

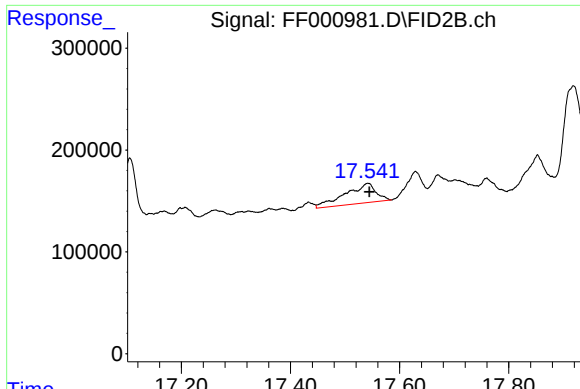

#13 N-TRIACONTANE


R.T.: 17.542 min
Delta R.T.: -0.003 min
Response: 754960
Conc: 5.98 ug/ml

Instrument :
FID_F
ClientSampleId :

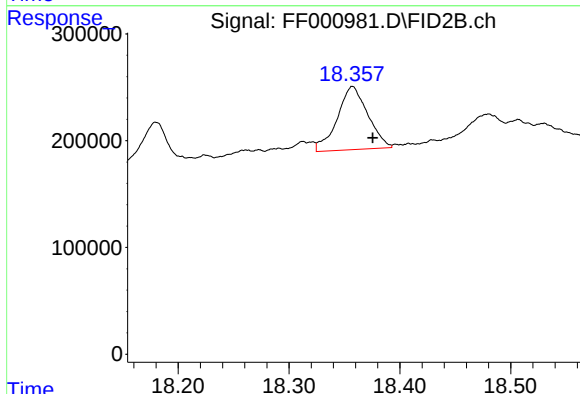


#14 N-DOTRIACONTANE

R.T.: 18.357 min
Delta R.T.: -0.018 min
Response: 1131141
Conc: 9.22 ug/ml

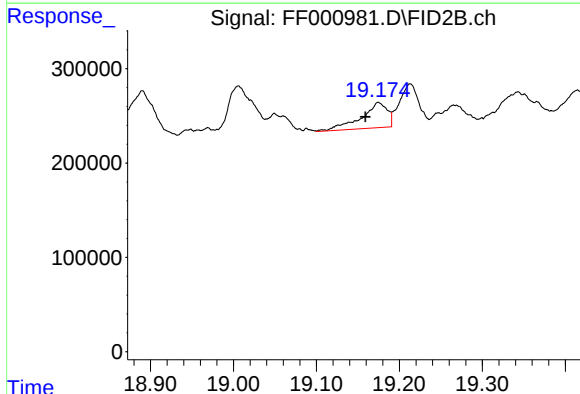

#15 N-TETRATRIACONTANE

R.T.: 19.175 min
Delta R.T.: 0.016 min
Response: 587037
Conc: 4.89 ug/ml

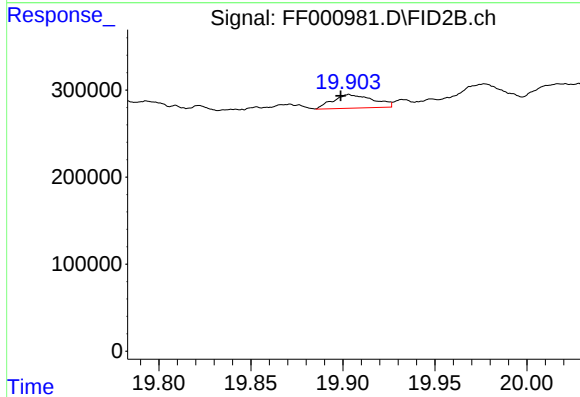

#16 N-HEXATRIACONTANE

R.T.: 19.904 min
Delta R.T.: 0.005 min
Response: 237639
Conc: 2.08 ug/ml