

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF000982.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2018 15:21
 Operator : UA\AJ
 Sample : J3566-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:18:43 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.483	1436734	12.458 ug/ml
Target Compounds			
4) N-TETRADECANE	8.045	155270	1.115 ug/ml
5) N-HEXADECANE	9.642	330416	2.396 ug/ml
6) N-OCTADECANE	11.080	201381	1.475 ug/ml
15) N-TETRATRIACONTANE	19.205	213496	1.779 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000982.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 15:21
Operator : UA\AJ
Sample : J3566-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:18:43 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

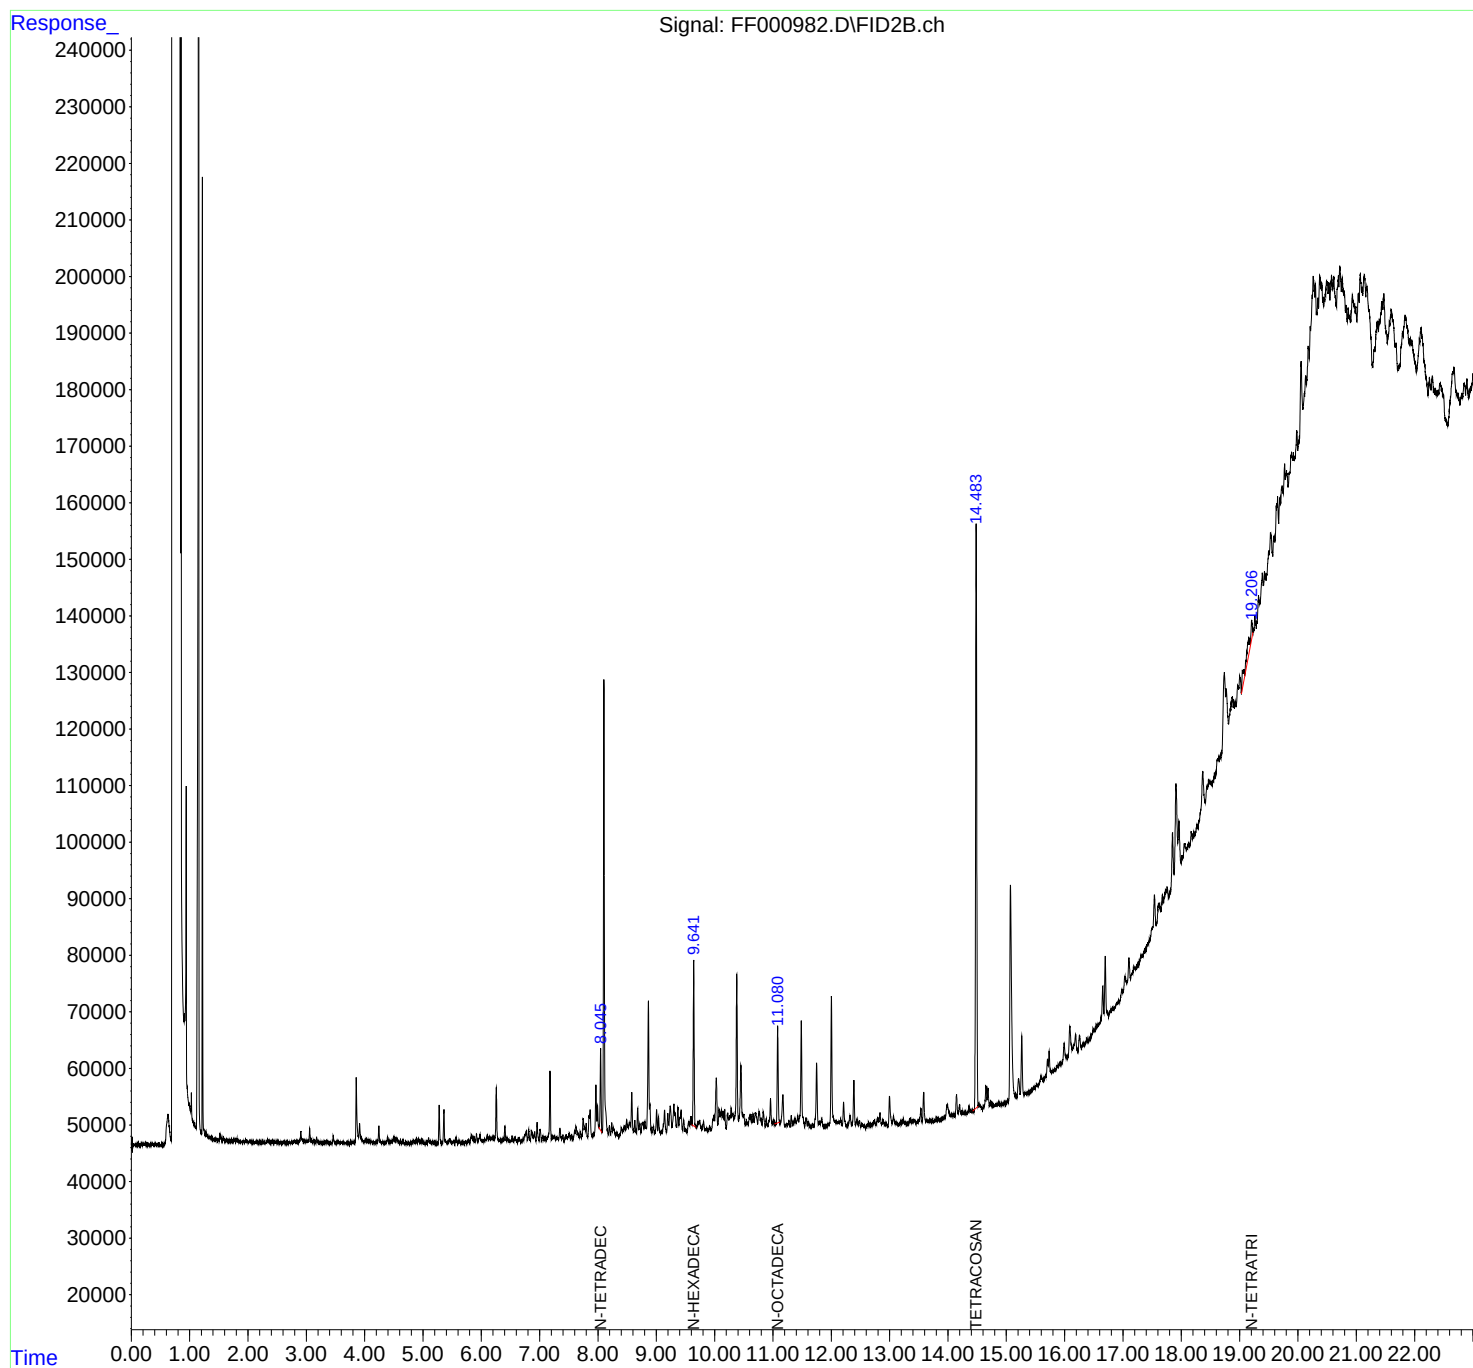


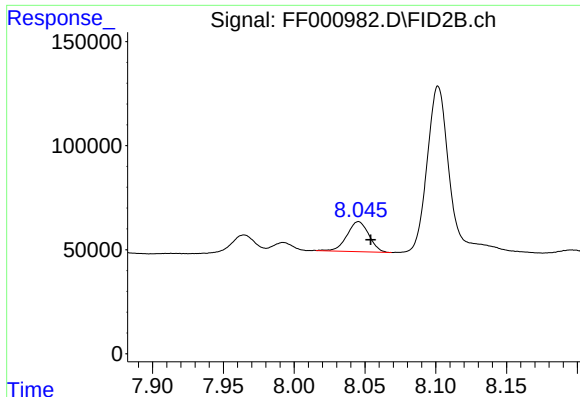

#4 N-TETRADECANE


R.T.: 8.045 min
Delta R.T.: -0.009 min
Response: 155270
Conc: 1.12 ug/ml

Instrument :
FID_F
ClientSampleId :

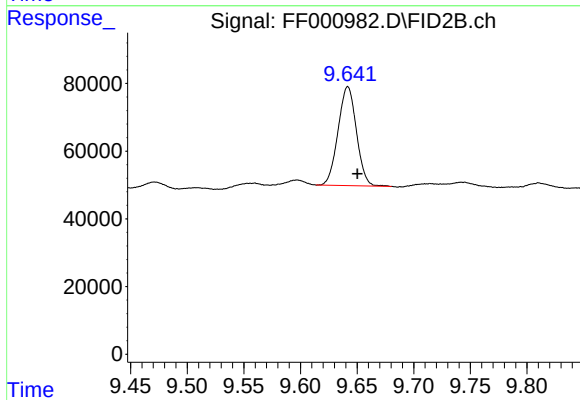


#5 N-HEXADECANE

R.T.: 9.642 min
Delta R.T.: -0.008 min
Response: 330416
Conc: 2.40 ug/ml

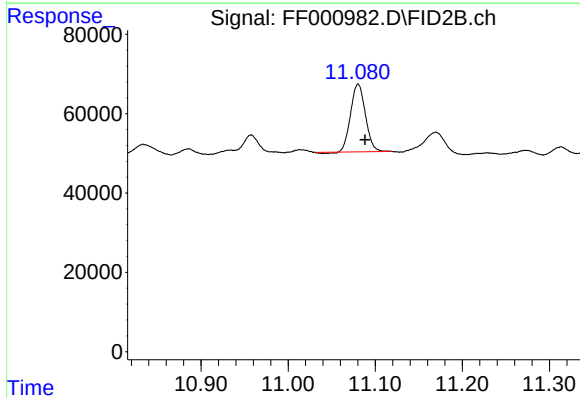


#6 N-OCTADECANE

R.T.: 11.080 min
Delta R.T.: -0.008 min
Response: 201381
Conc: 1.47 ug/ml

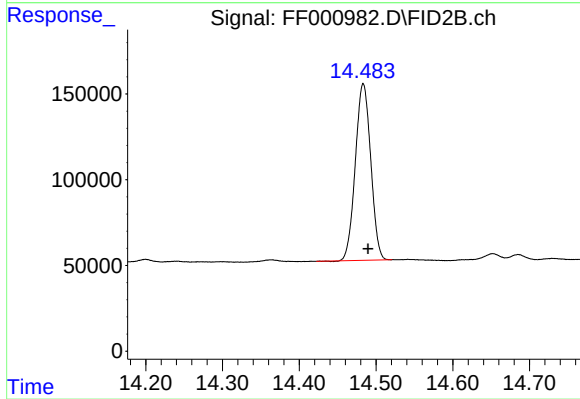

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.483 min
Delta R.T.: -0.006 min
Response: 1436734
Conc: 12.46 ug/ml

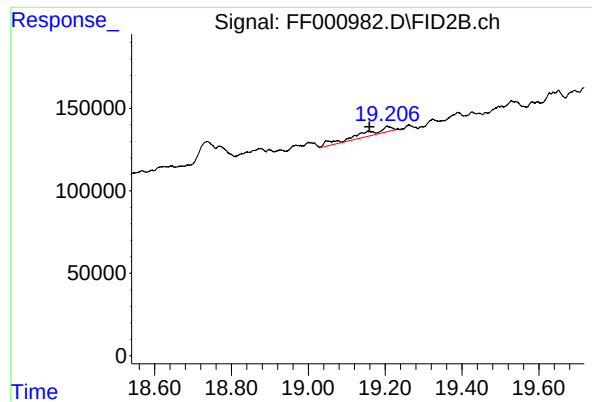

#15 N-TETRATRIACONTANE

R.T.: 19.205 min
Delta R.T.: 0.046 min
Response: 213496
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :