

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF000984.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2018 16:22
 Operator : UA\AJ
 Sample : J3566-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:19:10 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.484	1715961	14.879 ug/ml
Target Compounds			
4) N-TETRADECANE	8.102	987583	7.093 ug/ml
5) N-HEXADECANE	9.641	153653	1.114 ug/ml
16) N-HEXATRIACONTANE	19.903	45205	0.396 ug/ml
17) N-OCTATRIACONTANE	20.612	626408	6.087 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000984.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 16:22
Operator : UA\AJ
Sample : J3566-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:19:10 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

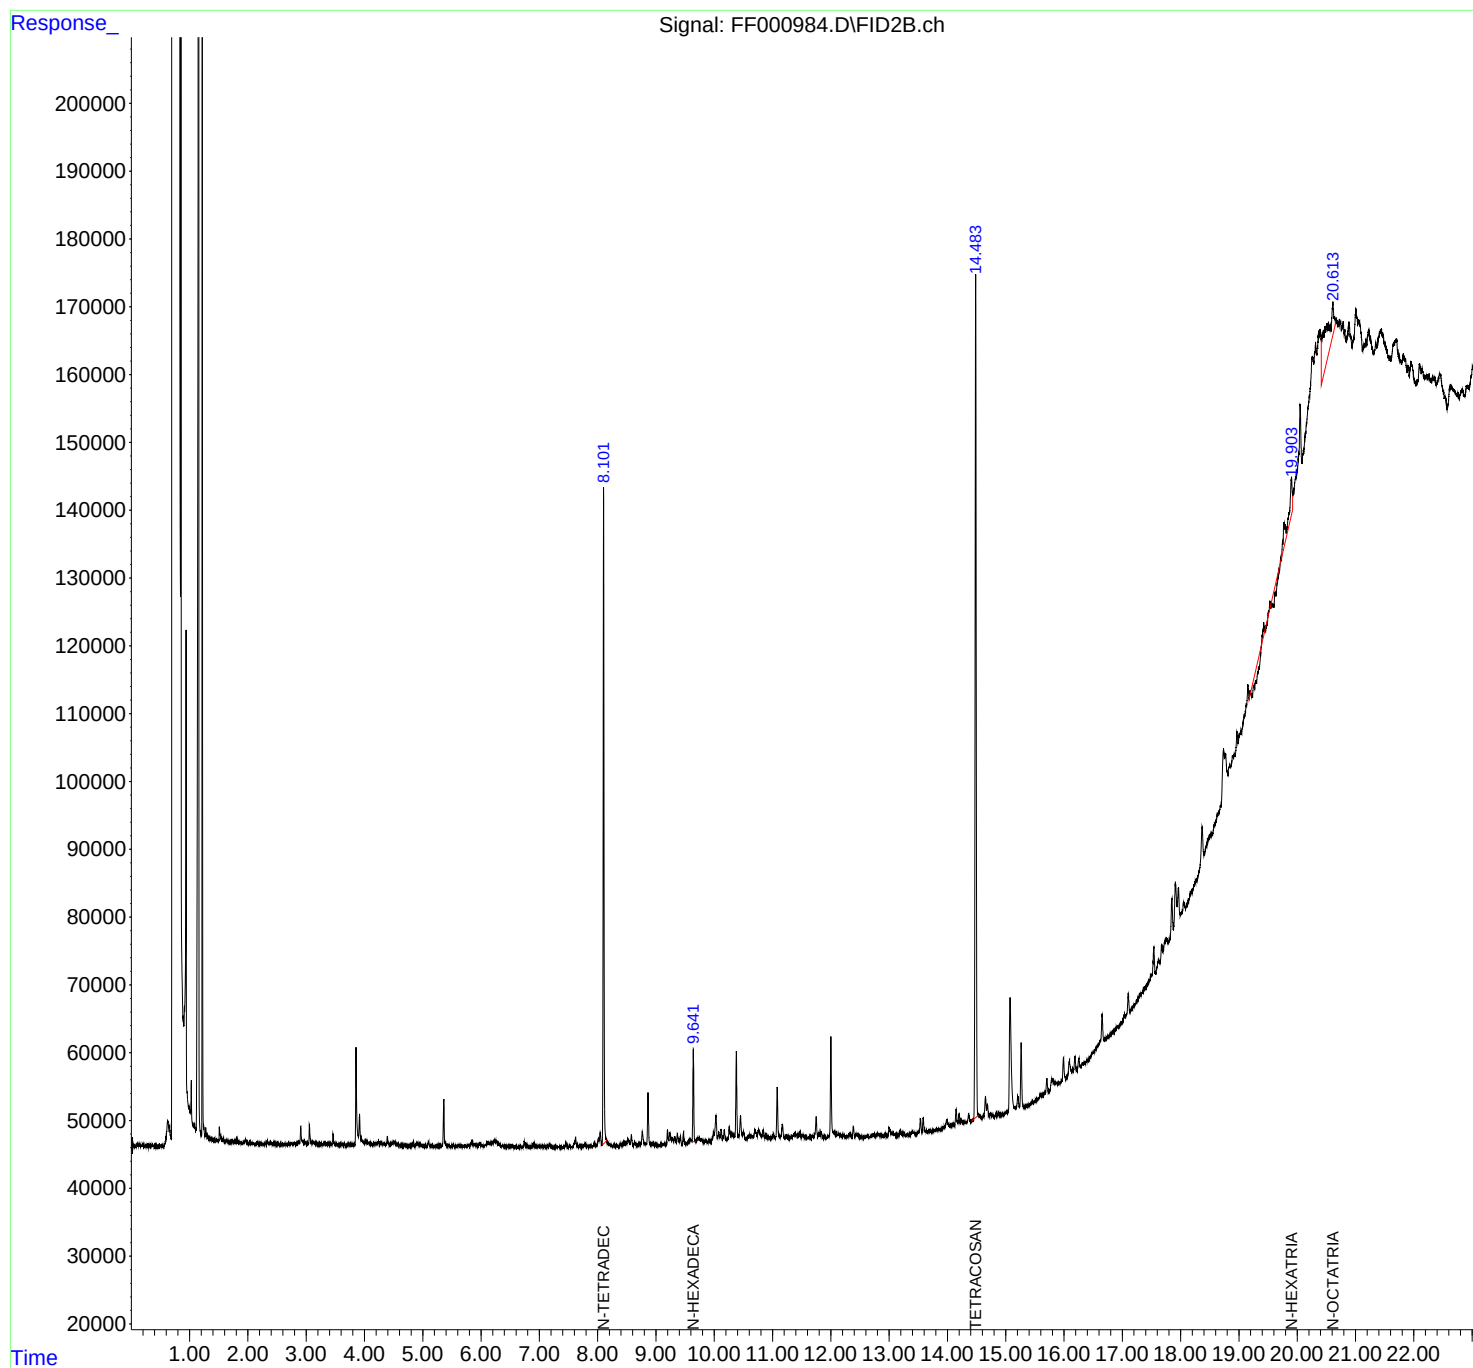


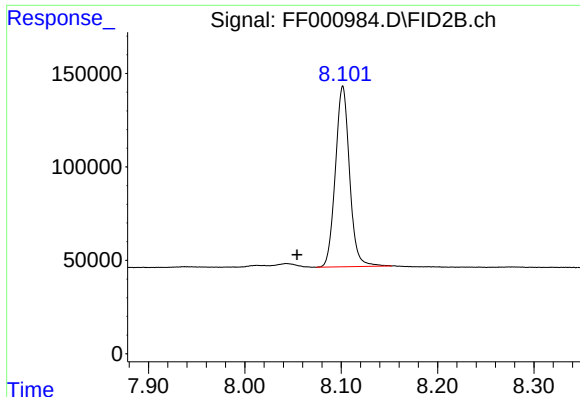

#4 N-TETRADECANE


R.T.: 8.102 min
Delta R.T.: 0.048 min
Response: 987583
Conc: 7.09 ug/ml

Instrument :
FID_F
ClientSampleId :

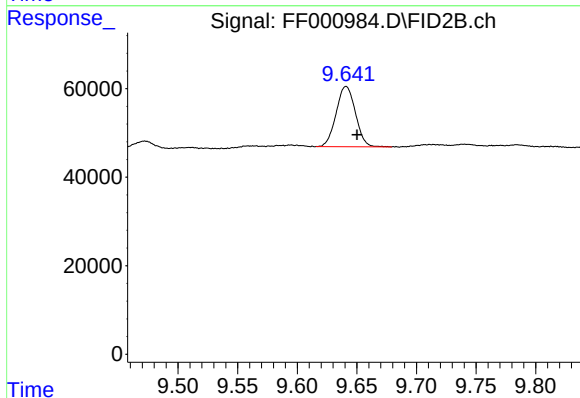


#5 N-HEXADECANE

R.T.: 9.641 min
Delta R.T.: -0.009 min
Response: 153653
Conc: 1.11 ug/ml

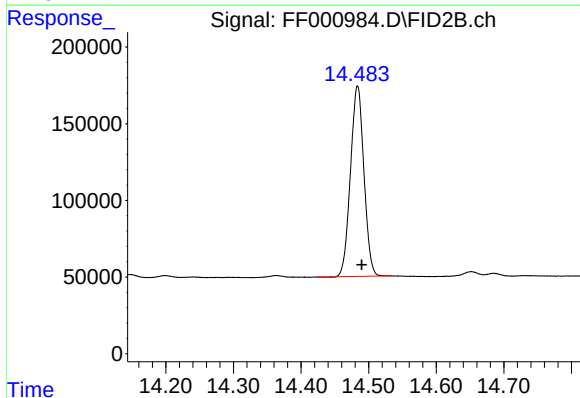


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.484 min
Delta R.T.: -0.006 min
Response: 1715961
Conc: 14.88 ug/ml

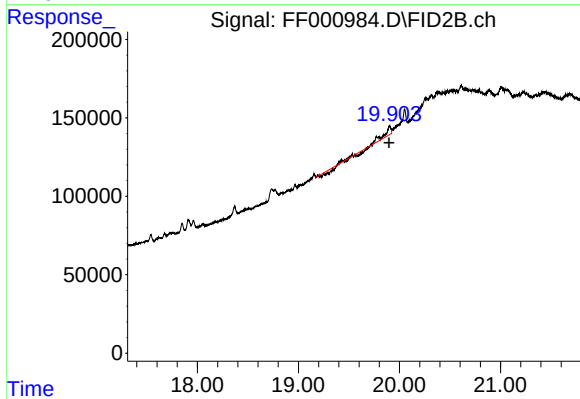

#16 N-HEXATRIACONTANE

R.T.: 19.903 min
Delta R.T.: 0.004 min
Response: 45205
Conc: 0.40 ug/ml

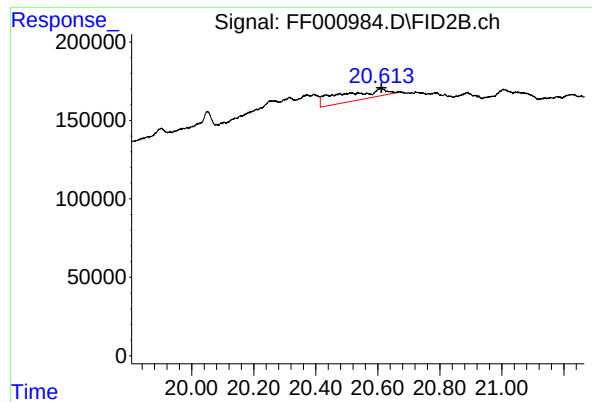

#17 N-OCTATRIACONTANE

R.T.: 20.612 min
Delta R.T.: 0.000 min
Response: 626408
Conc: 6.09 ug/ml

Instrument :
FID_F
ClientSampleId :