

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF000989.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2018 18:55
 Operator : UA\AJ
 Sample : J3566-10
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:20:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.482	1741099	15.097 ug/ml
Target Compounds			
4) N-TETRADECANE	8.100	996109	7.154 ug/ml
5) N-HEXADECANE	9.641	400748	2.907 ug/ml
7) N-EICOSANE	12.437	3180548	23.739 ug/ml
8) N-DOCOSANE	13.594	372118	2.814 ug/ml
10) N-TETRACOSANE	14.649	1317758	10.159 ug/ml
12) N-OCTACOSANE	16.650	373008	2.933 ug/ml
13) N-TRIACONTANE	17.538	254075	2.012 ug/ml
14) N-DOTRIACONTANE	18.371	146049	1.191 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000989.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 18:55
Operator : UA\AJ
Sample : J3566-10
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:20:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

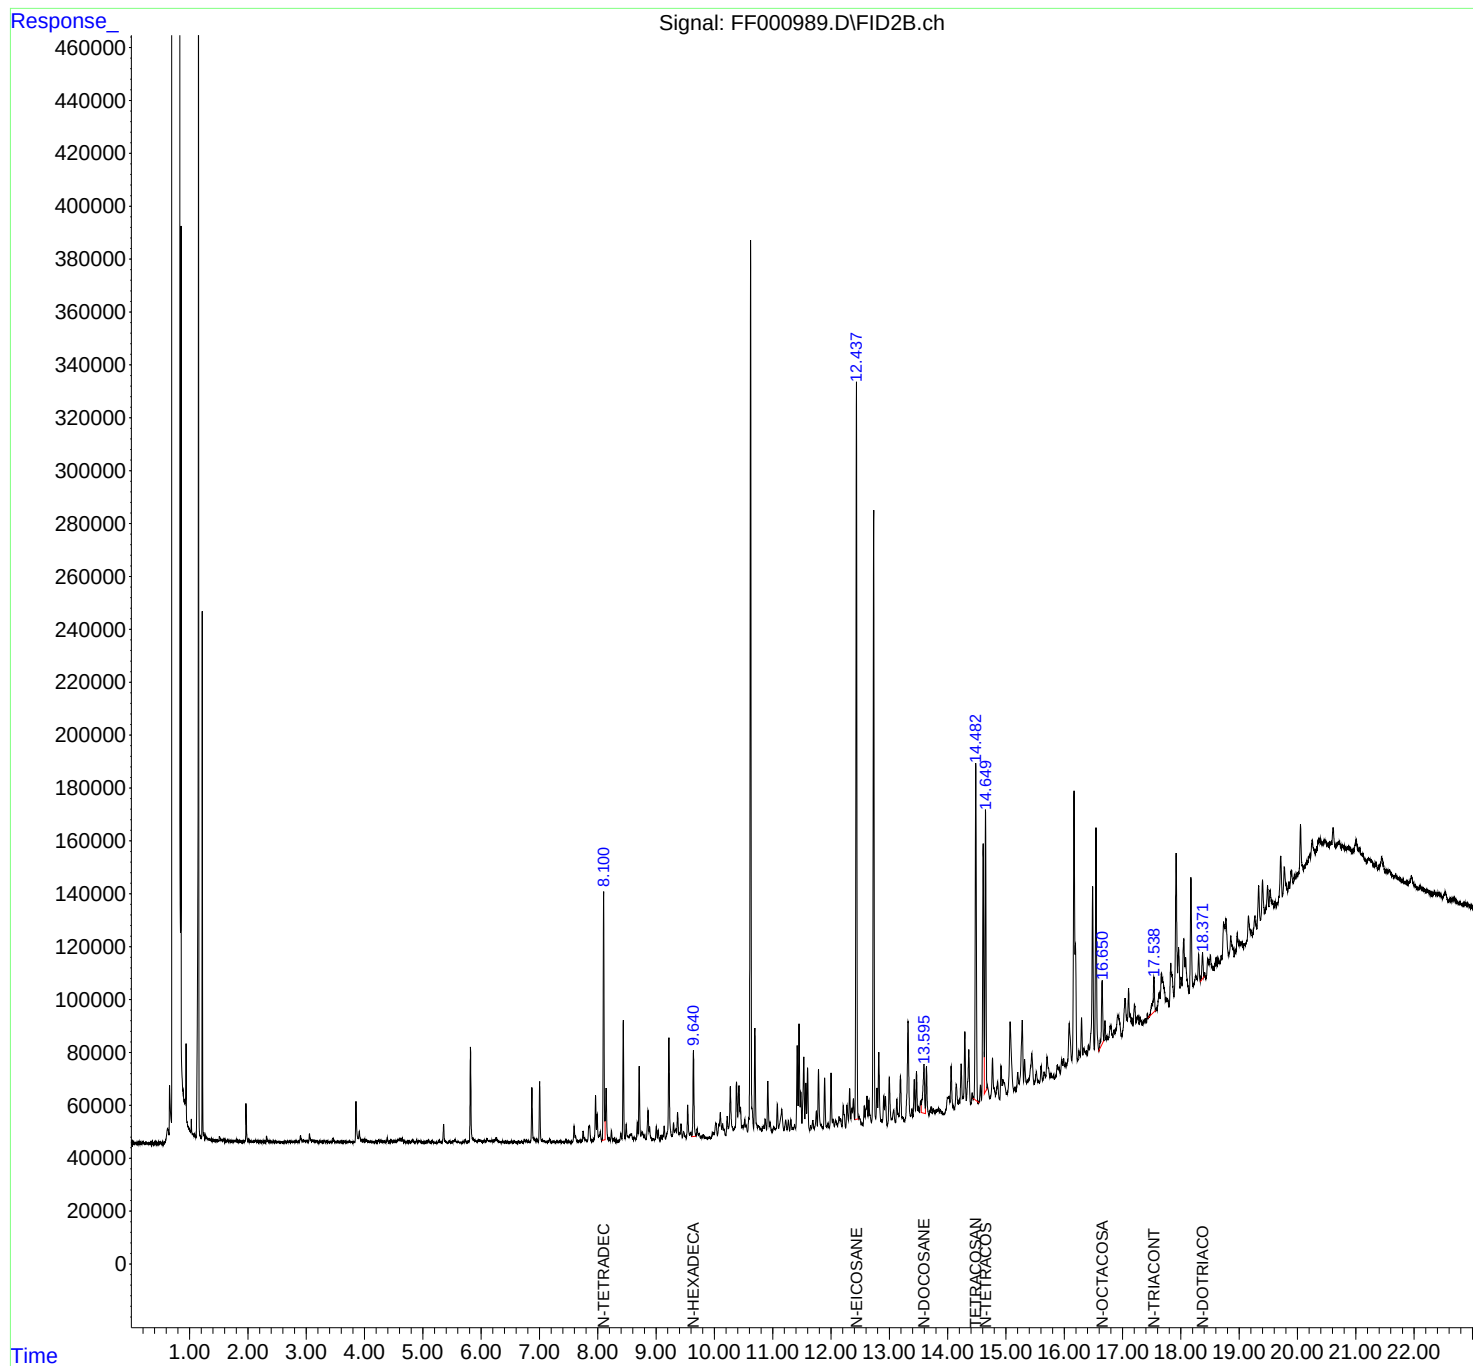


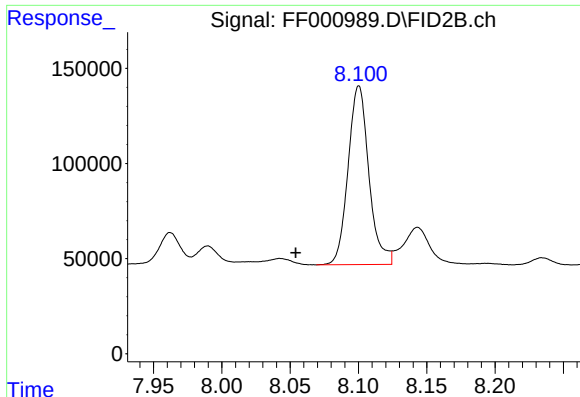

#4 N-TETRADECANE


R.T.: 8.100 min
Delta R.T.: 0.046 min
Response: 996109
Conc: 7.15 ug/ml

Instrument :
FID_F
ClientSampleId :

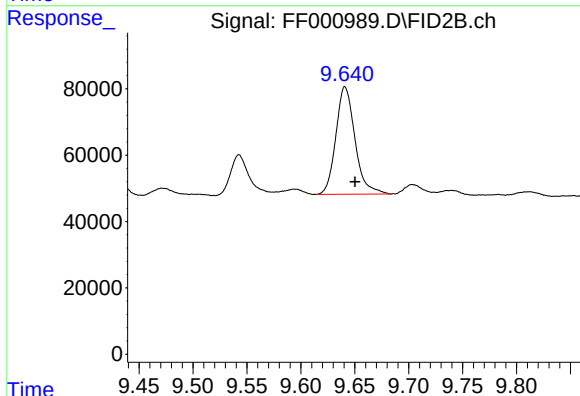


#5 N-HEXADECANE

R.T.: 9.641 min
Delta R.T.: -0.009 min
Response: 400748
Conc: 2.91 ug/ml

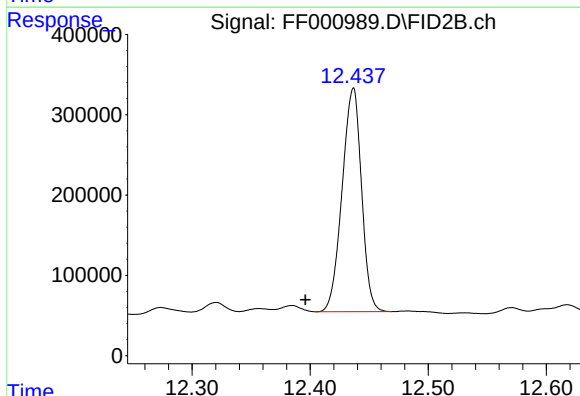


#7 N-EICOSANE

R.T.: 12.437 min
Delta R.T.: 0.041 min
Response: 3180548
Conc: 23.74 ug/ml

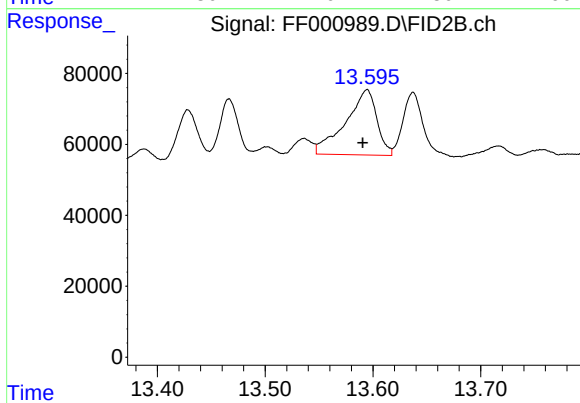

#8 N-DOCOSANE


R.T.: 13.594 min
Delta R.T.: 0.004 min
Response: 372118
Conc: 2.81 ug/ml

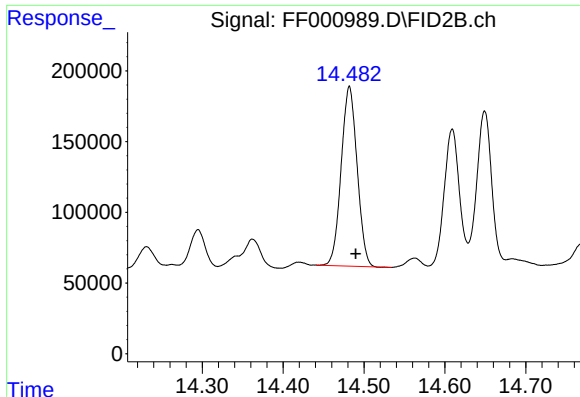

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.482 min
Delta R.T.: -0.008 min
Response: 1741099
Conc: 15.10 ug/ml

Instrument :
FID_F
ClientSampleId :

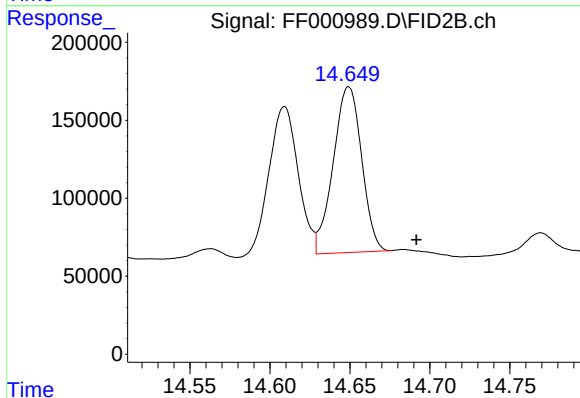


#10 N-TETRACOSANE

R.T.: 14.649 min
Delta R.T.: -0.042 min
Response: 1317758
Conc: 10.16 ug/ml

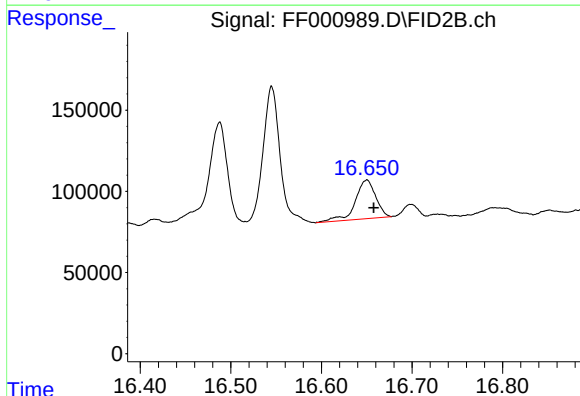


#12 N-OCTACOSANE

R.T.: 16.650 min
Delta R.T.: -0.008 min
Response: 373008
Conc: 2.93 ug/ml

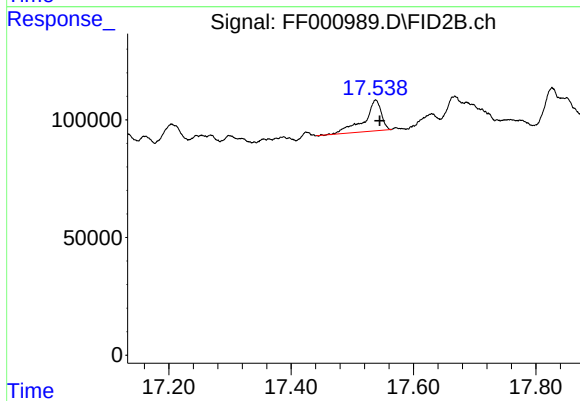

#13 N-TRIACONTANE

R.T.: 17.538 min
Delta R.T.: -0.006 min
Response: 254075
Conc: 2.01 ug/ml

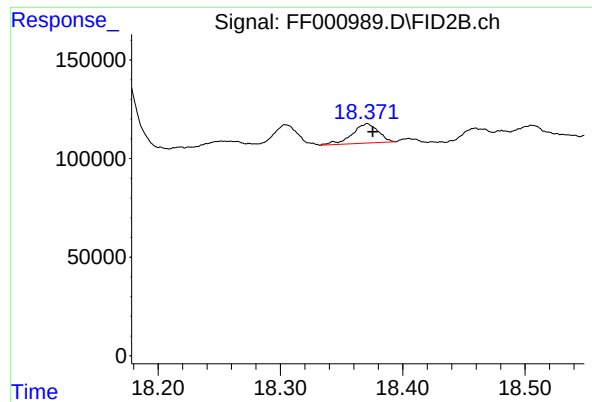

#14 N-DOTRIACONTANE

R.T.: 18.371 min
Delta R.T.: -0.004 min
Response: 146049
Conc: 1.19 ug/ml

Instrument :
FID_F
ClientSampleId :