

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000995.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 21:59
Operator : UA\AJ
Sample : J3567-02
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:21:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.481	1668344	14.467 ug/ml
Target Compounds			
4) N-TETRADECANE	8.099	922593	6.626 ug/ml
5) N-HEXADECANE	9.640	208017	1.509 ug/ml
13) N-TRIACONTANE	17.537	236661	1.874 ug/ml
14) N-DOTRIACONTANE	18.366	167424	1.365 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF000995.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2018 21:59
Operator : UA\AJ
Sample : J3567-02
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:21:42 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

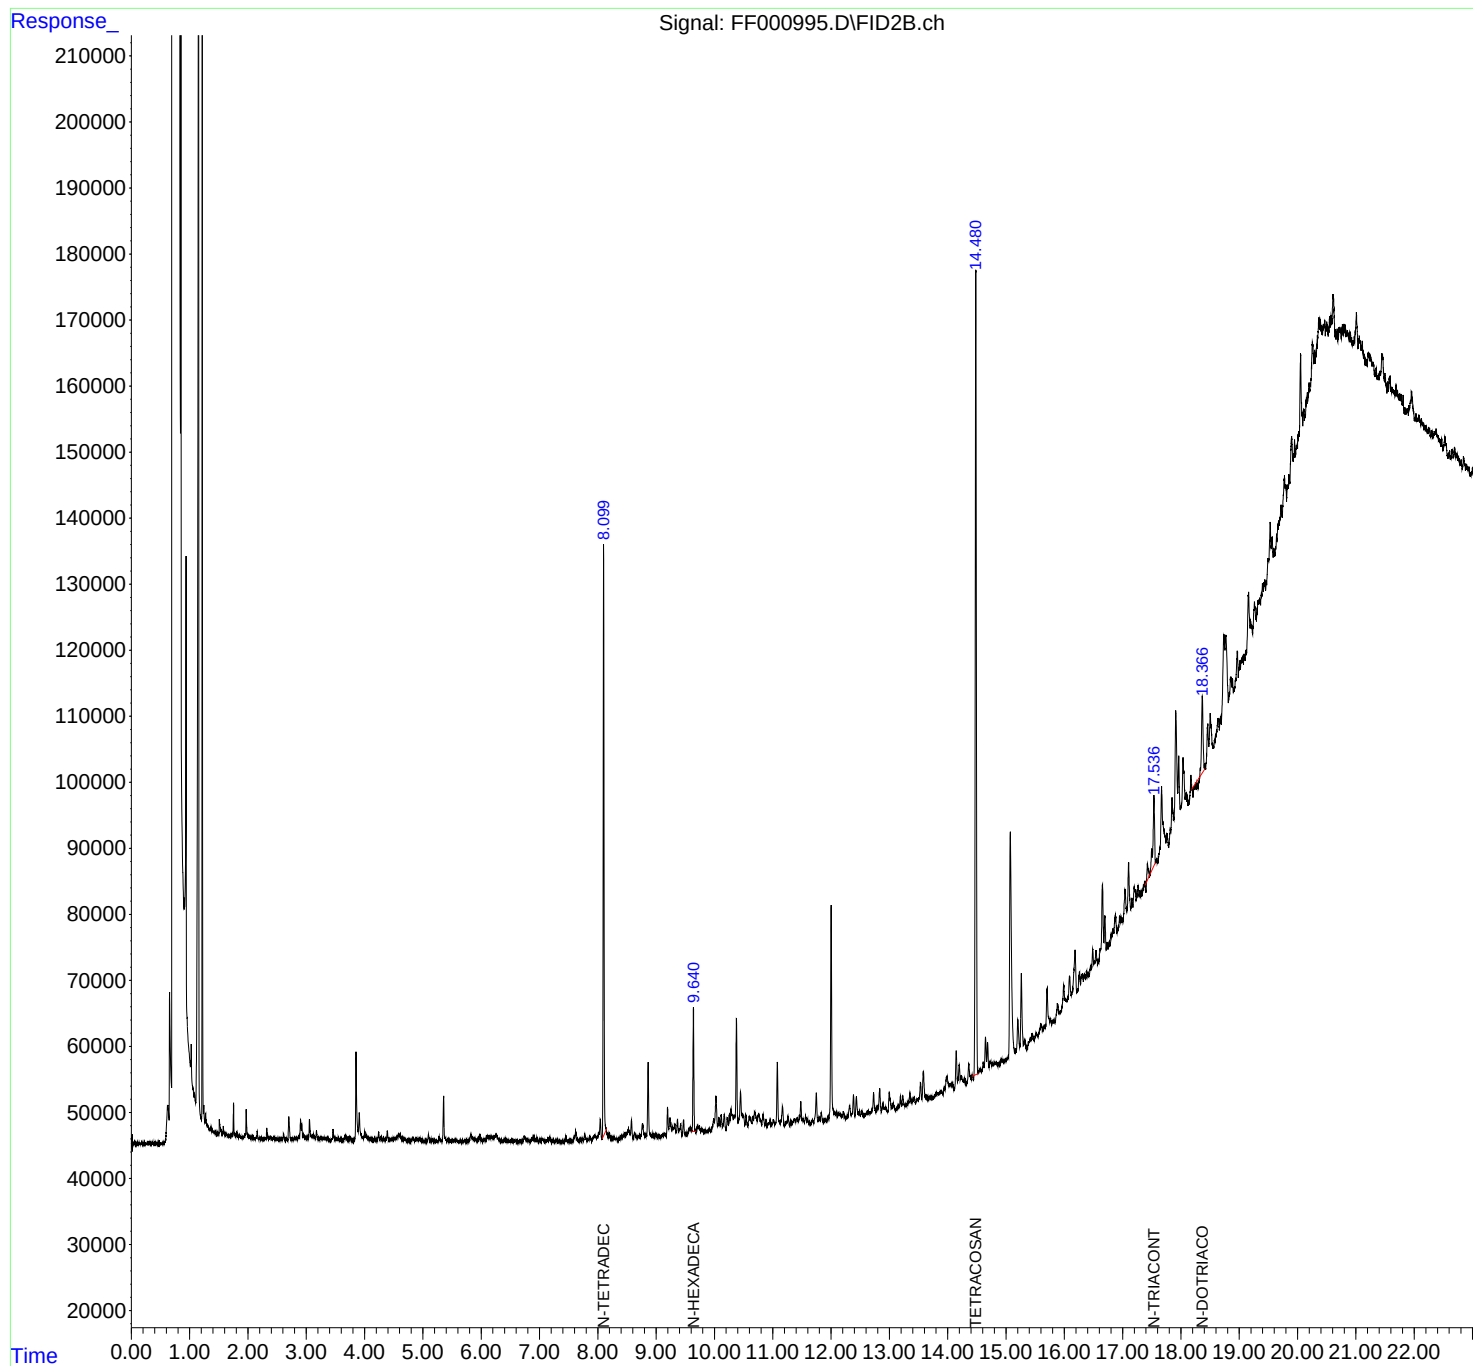


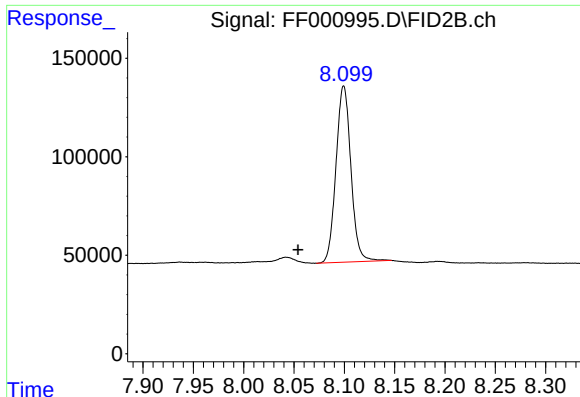

#4 N-TETRADECANE


R.T.: 8.099 min
Delta R.T.: 0.045 min
Response: 922593
Conc: 6.63 ug/ml

Instrument :
FID_F
ClientSampleId :

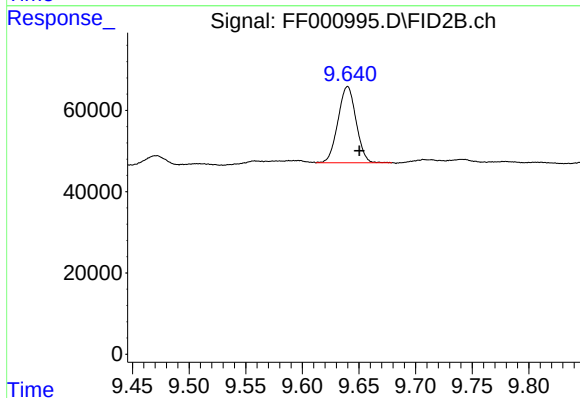


#5 N-HEXADECANE

R.T.: 9.640 min
Delta R.T.: -0.010 min
Response: 208017
Conc: 1.51 ug/ml

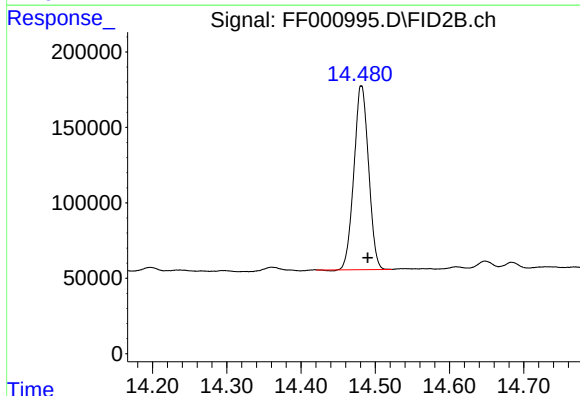


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.481 min
Delta R.T.: -0.009 min
Response: 1668344
Conc: 14.47 ug/ml

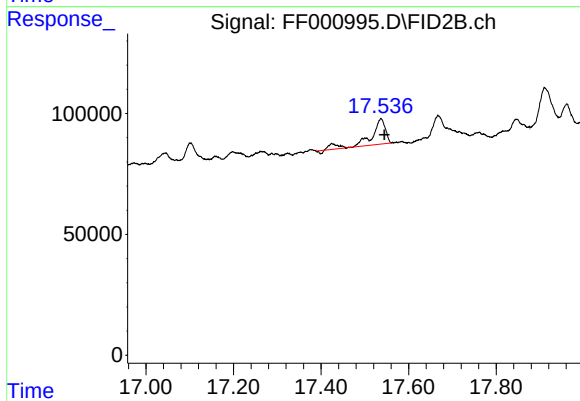

#13 N-TRIACONTANE

R.T.: 17.537 min
Delta R.T.: -0.007 min
Response: 236661
Conc: 1.87 ug/ml

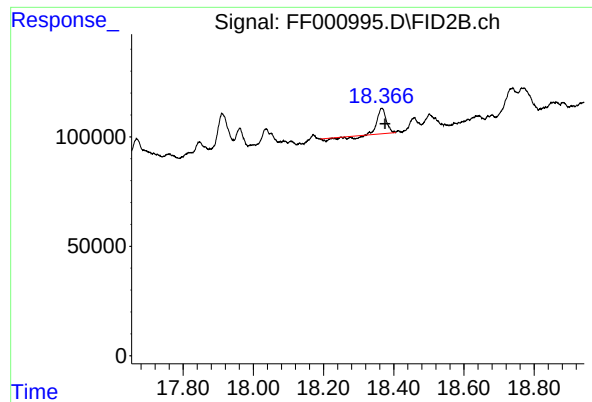

#14 N-DOTRIACONTANE

R.T.: 18.366 min
Delta R.T.: -0.010 min
Response: 167424
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :