

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF001000.D
 Signal(s) : FID2B.ch
 Acq On : 19 Jun 2018 00:30
 Operator : UA\AJ
 Sample : J3567-10MS
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:22:46 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.480	1881567	16.315 ug/ml
Target Compounds			
1) N-OCTANE	2.160	1479151	10.496 ug/ml
2) N-DECANE	4.242	2169044	15.480 ug/ml
3) N-DODECANE	6.256	2236340	15.956 ug/ml
4) N-TETRADECANE	8.045	2260492	16.236 ug/ml
5) N-HEXADECANE	9.640	2338518	16.961 ug/ml
6) N-OCTADECANE	11.079	2284054	16.726 ug/ml
7) N-EICOSANE	12.386	2164189	16.153 ug/ml
8) N-DOCOSANE	13.582	2112127	15.973 ug/ml
10) N-TETRACOSANE	14.682	2124604	16.380 ug/ml
11) N-HEXACOSANE	15.703	2103127	16.374 ug/ml
12) N-OCTACOSANE	16.652	2040821	16.049 ug/ml
13) N-TRIACONTANE	17.538	2174057	17.218 ug/ml
14) N-DOTRIACONTANE	18.369	2183864	17.805 ug/ml
15) N-TETRATRIACONTANE	19.153	2021535	16.845 ug/ml
16) N-HEXATRIACONTANE	19.895	1926400	16.872 ug/ml
17) N-OCTATRIACONTANE	20.608	1817047	17.658 ug/ml
18) N-TETRACONTANE	21.447	1889780	18.454 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF001000.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2018 00:30
Operator : UA\AJ
Sample : J3567-10MS
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:22:46 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

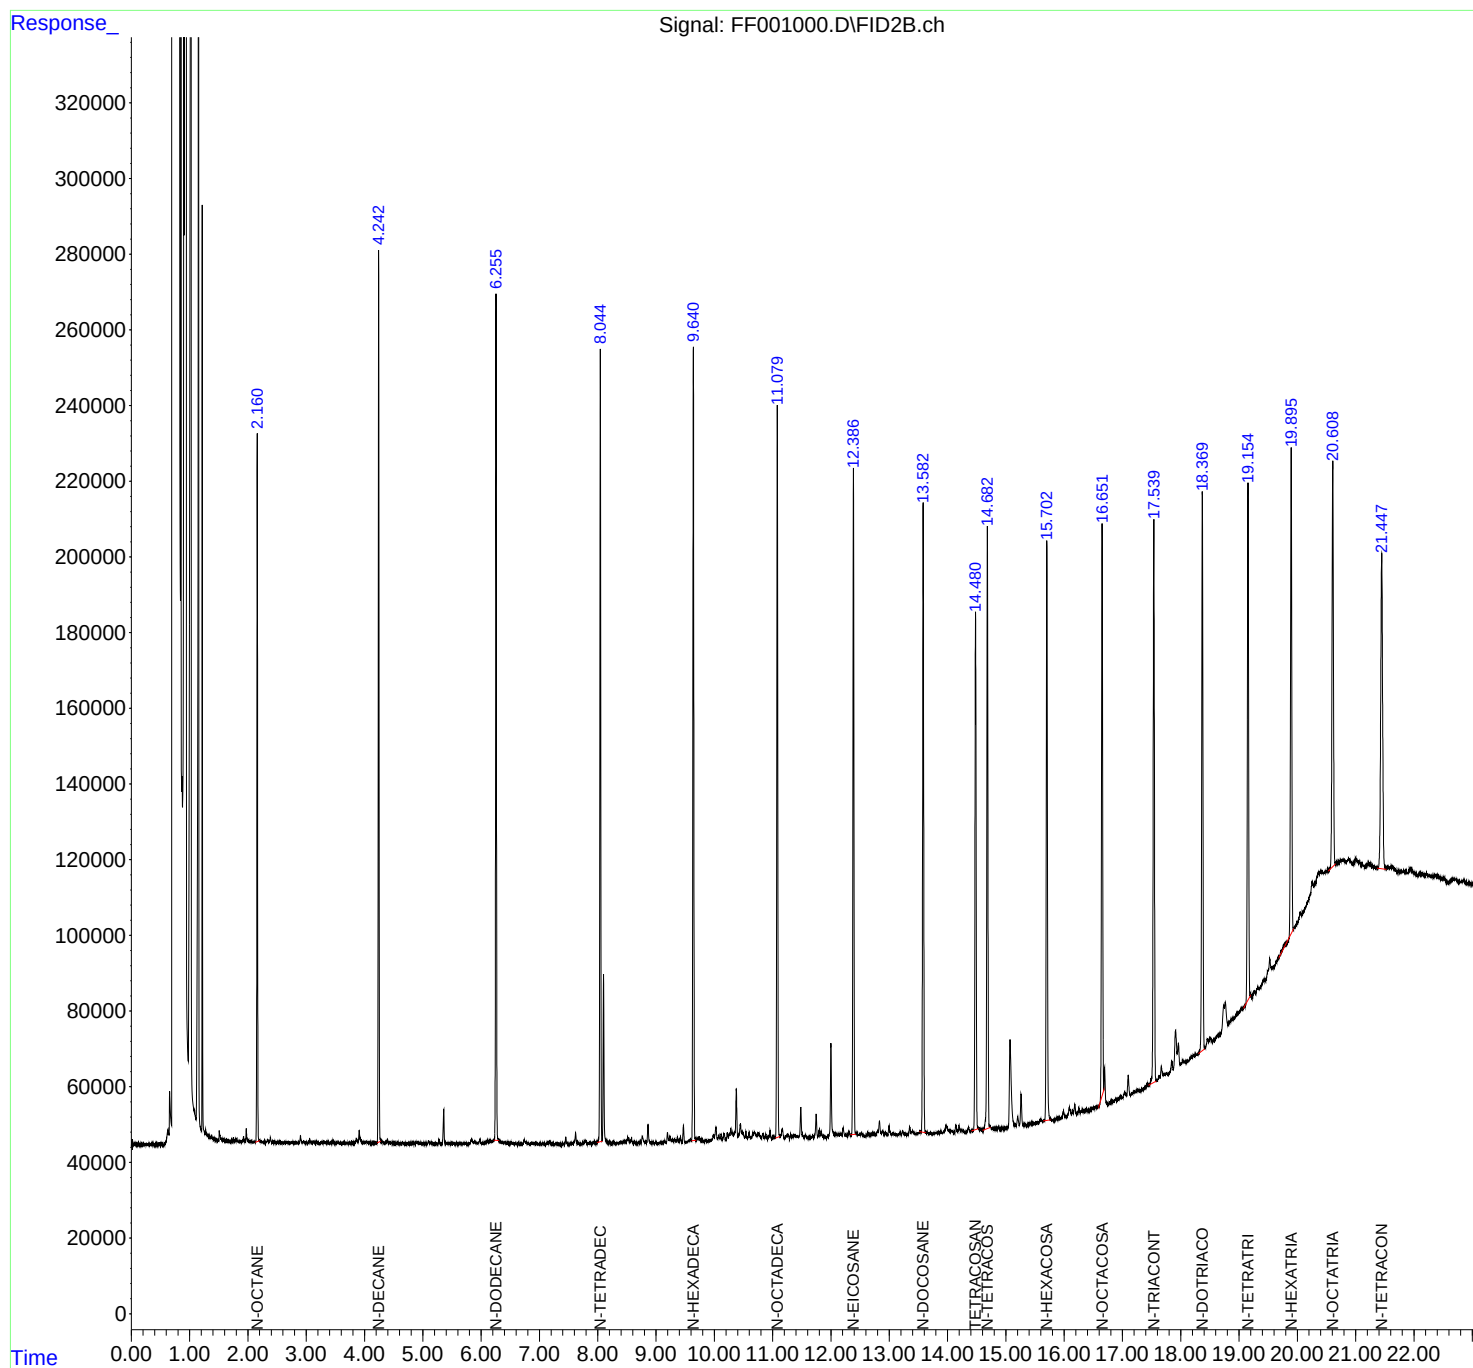


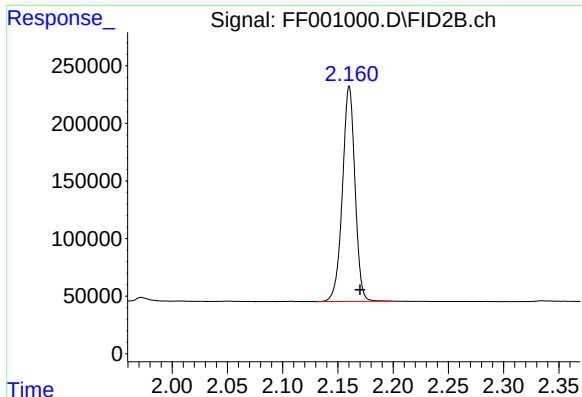

#1 N-OCTANE


R.T.: 2.160 min
Delta R.T.: -0.010 min
Response: 1479151
Conc: 10.50 ug/ml

Instrument :
FID_F
ClientSampleId :

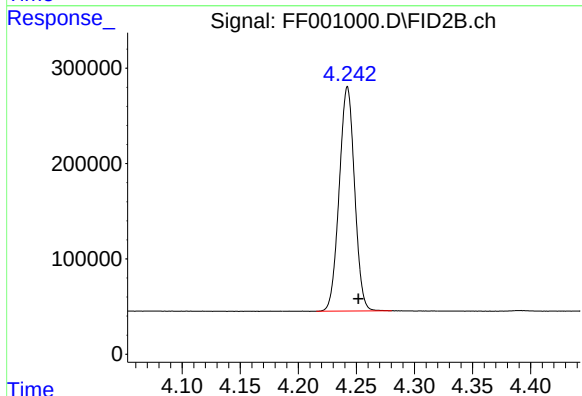


#2 N-DECANE

R.T.: 4.242 min
Delta R.T.: -0.009 min
Response: 2169044
Conc: 15.48 ug/ml

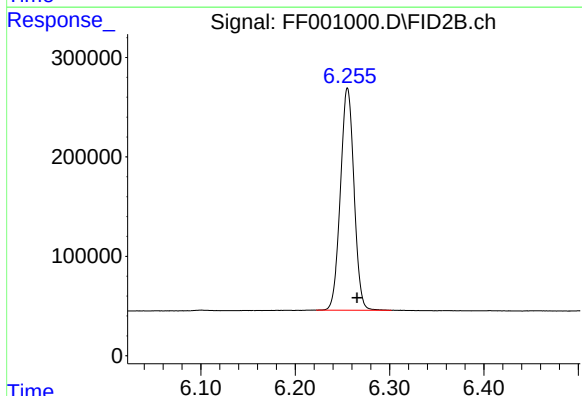


#3 N-DODECANE

R.T.: 6.256 min
Delta R.T.: -0.010 min
Response: 2236340
Conc: 15.96 ug/ml

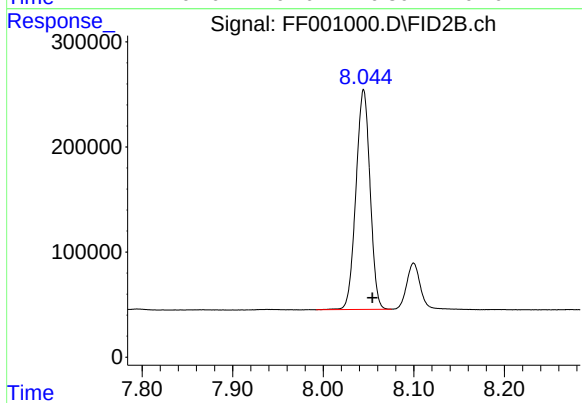

#4 N-TETRADECANE


R.T.: 8.045 min
Delta R.T.: -0.010 min
Response: 2260492
Conc: 16.24 ug/ml

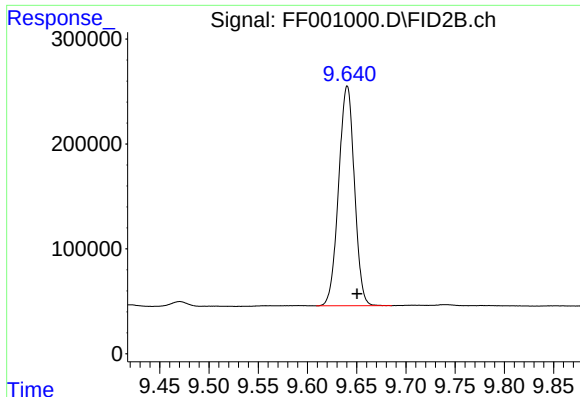

#5 N-HEXADECANE


R.T.: 9.640 min
Delta R.T.: -0.010 min
Response: 2338518
Conc: 16.96 ug/ml

Instrument :
FID_F
ClientSampleId :

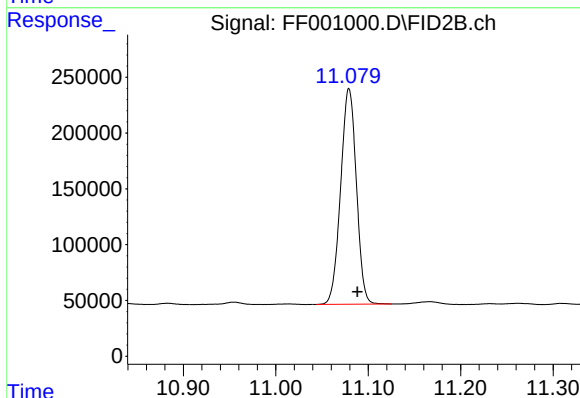


#6 N-OCTADECANE

R.T.: 11.079 min
Delta R.T.: -0.009 min
Response: 2284054
Conc: 16.73 ug/ml

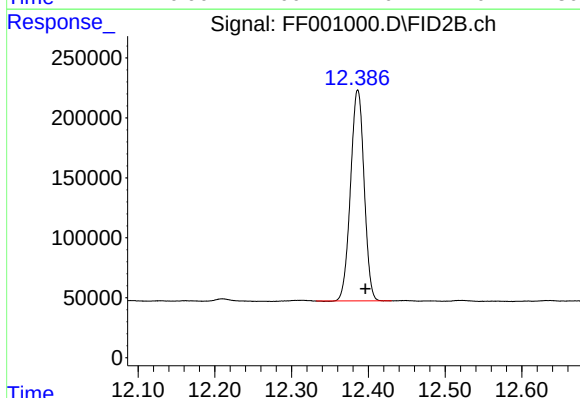


#7 N-EICOSANE

R.T.: 12.386 min
Delta R.T.: -0.010 min
Response: 2164189
Conc: 16.15 ug/ml

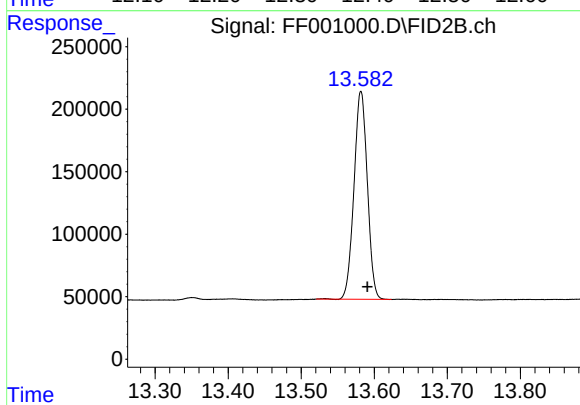

#8 N-DOCOSANE


R.T.: 13.582 min
Delta R.T.: -0.009 min
Response: 2112127
Conc: 15.97 ug/ml

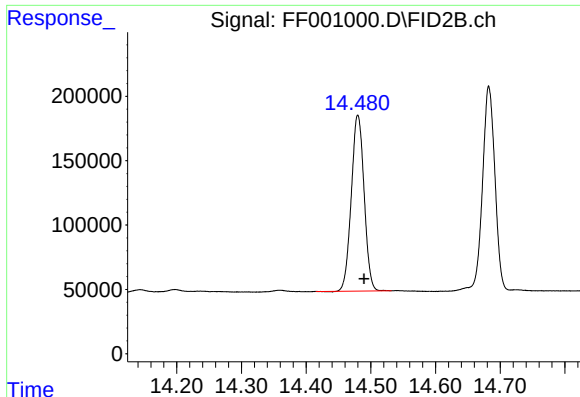

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.480 min
Delta R.T.: -0.010 min
Response: 1881567
Conc: 16.32 ug/ml

Instrument :
FID_F
ClientSampleId :

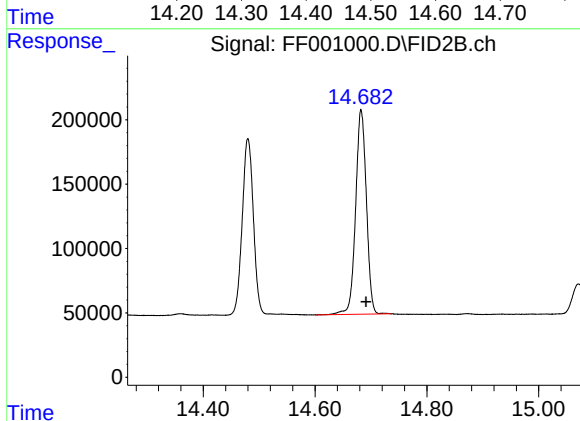


#10 N-TETRACOSANE

R.T.: 14.682 min
Delta R.T.: -0.009 min
Response: 2124604
Conc: 16.38 ug/ml

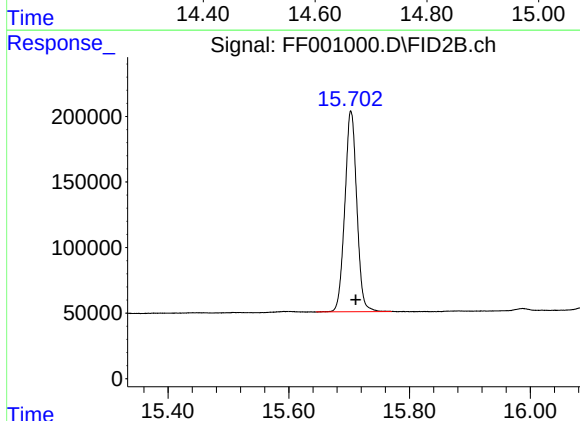


#11 N-HEXACOSANE

R.T.: 15.703 min
Delta R.T.: -0.008 min
Response: 2103127
Conc: 16.37 ug/ml

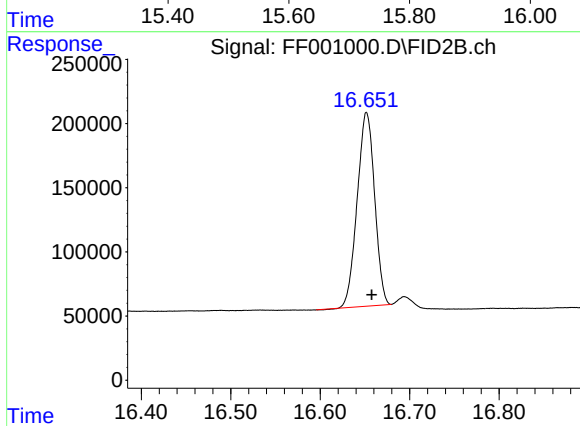

#12 N-OCTACOSANE


R.T.: 16.652 min
Delta R.T.: -0.006 min
Response: 2040821
Conc: 16.05 ug/ml

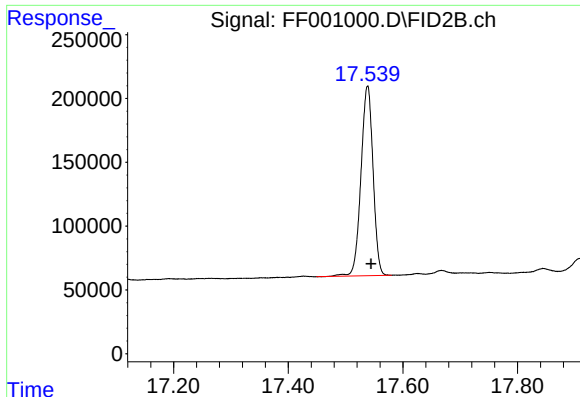

#13 N-TRIACONTANE


R.T.: 17.538 min
Delta R.T.: -0.006 min
Response: 2174057
Conc: 17.22 ug/ml

Instrument :
FID_F
ClientSampleId :

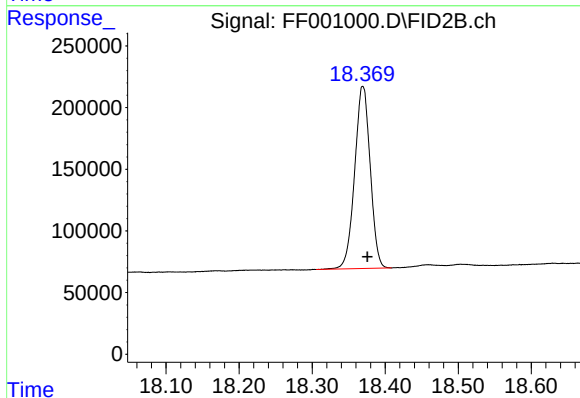


#14 N-DOTRIACONTANE

R.T.: 18.369 min
Delta R.T.: -0.006 min
Response: 2183864
Conc: 17.81 ug/ml

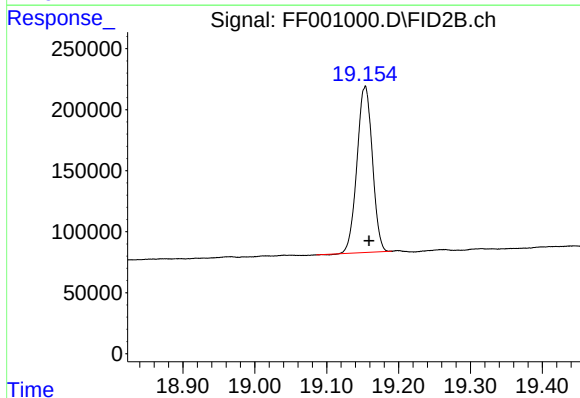


#15 N-TETRATRIACONTANE

R.T.: 19.153 min
Delta R.T.: -0.006 min
Response: 2021535
Conc: 16.84 ug/ml

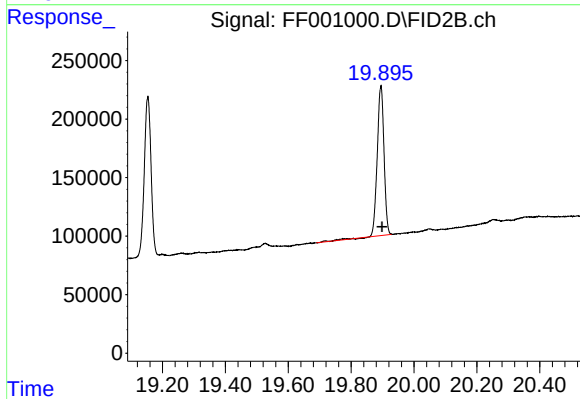

#16 N-HEXATRIACONTANE


R.T.: 19.895 min
Delta R.T.: -0.004 min
Response: 1926400
Conc: 16.87 ug/ml

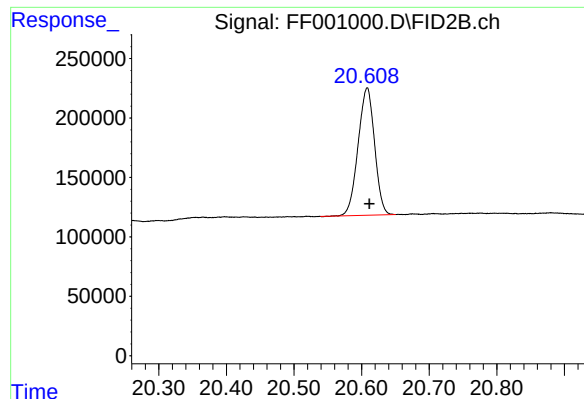

#17 N-OCTATRIACONTANE

R.T.: 20.608 min
Delta R.T.: -0.004 min
Response: 1817047
Conc: 17.66 ug/ml

Instrument :
FID_F
ClientSampleId :

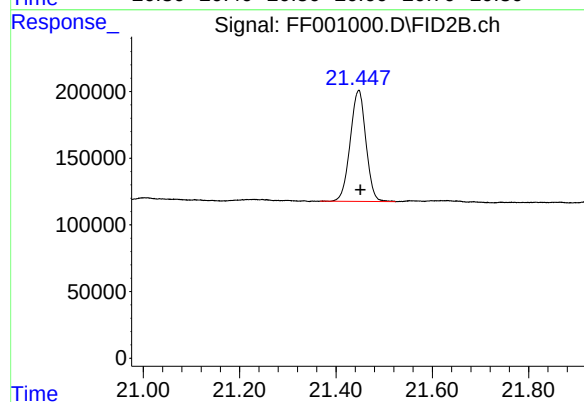

#18 N-TETRACONTANE

R.T.: 21.447 min
Delta R.T.: -0.004 min
Response: 1889780
Conc: 18.45 ug/ml