

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF001002.D
 Signal(s) : FID2B.ch
 Acq On : 19 Jun 2018 01:31
 Operator : UA\AJ
 Sample : J3240-03 5X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:23:24 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.479	309811	2.686 ug/ml
Target Compounds			
4) N-TETRADECANE	8.099	184342	1.324 ug/ml
13) N-TRIACONTANE	17.538	393226	3.114 ug/ml
14) N-DOTRIACONTANE	18.368	251702	2.052 ug/ml
15) N-TETRATRIACONTANE	19.163	269656	2.247 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF001002.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2018 01:31
Operator : UA\AJ
Sample : J3240-03 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:23:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

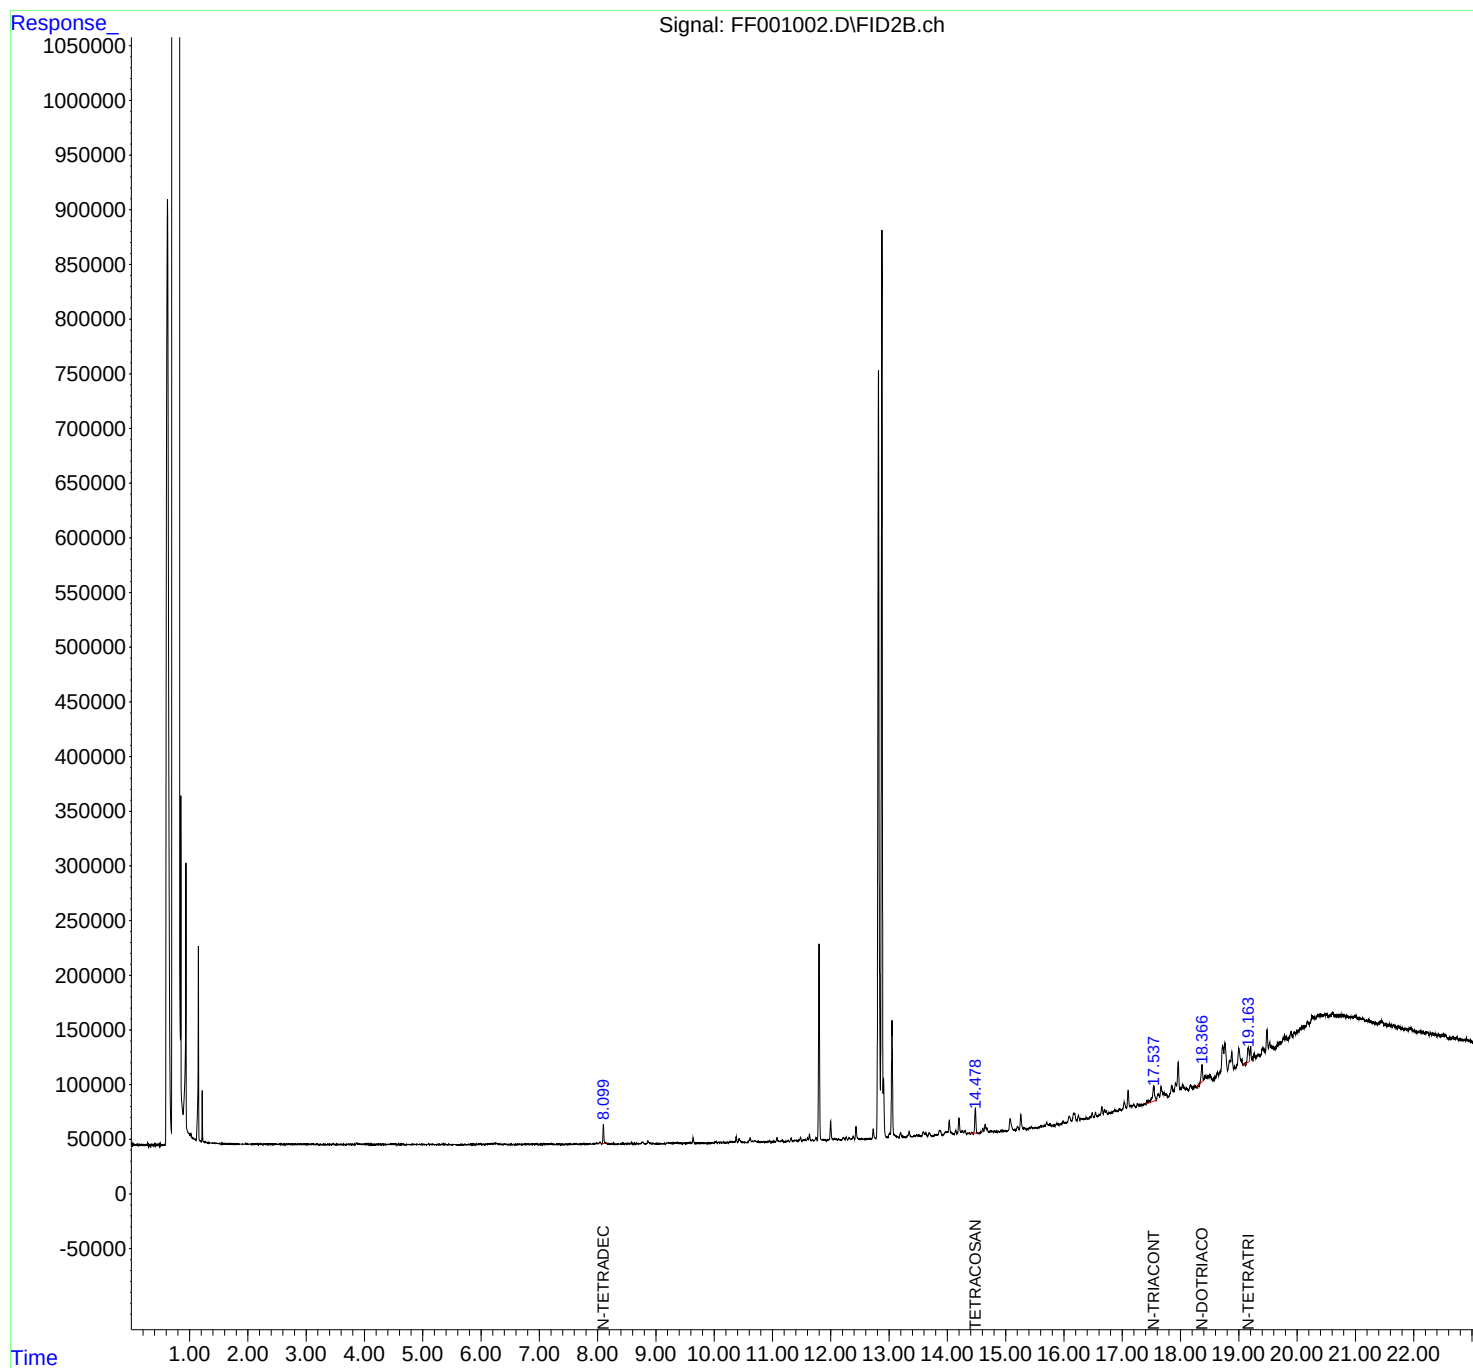


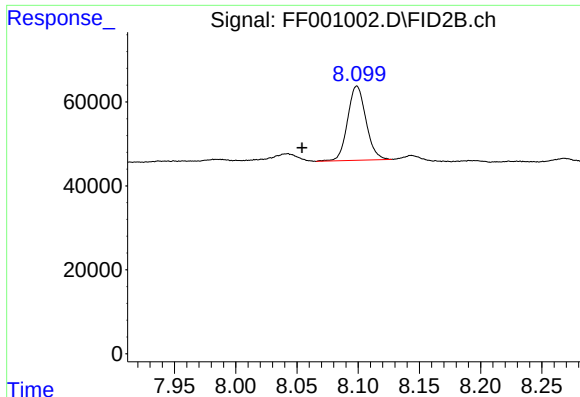

#4 N-TETRADECANE


R.T.: 8.099 min
Delta R.T.: 0.045 min
Response: 184342
Conc: 1.32 ug/ml

Instrument :
FID_F
ClientSampleId :

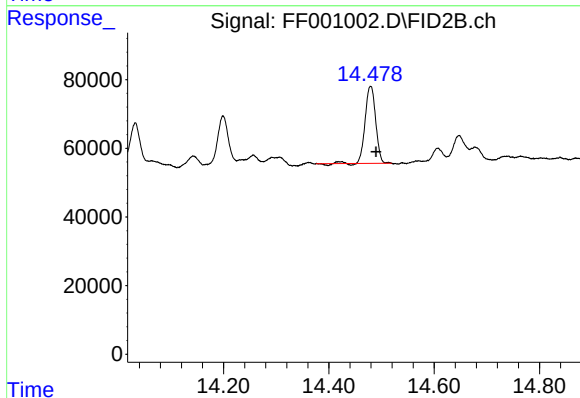


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.479 min
Delta R.T.: -0.010 min
Response: 309811
Conc: 2.69 ug/ml

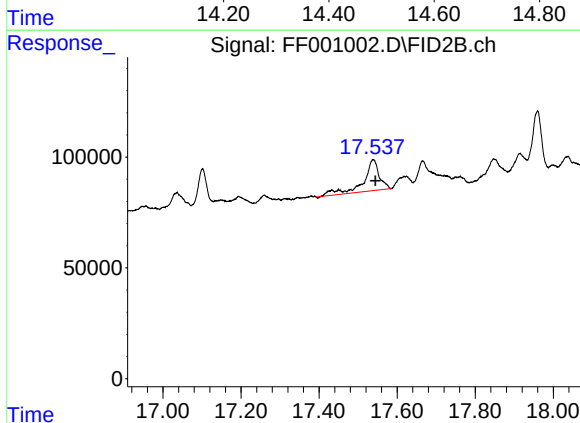


#13 N-TRIACONTANE

R.T.: 17.538 min
Delta R.T.: -0.006 min
Response: 393226
Conc: 3.11 ug/ml

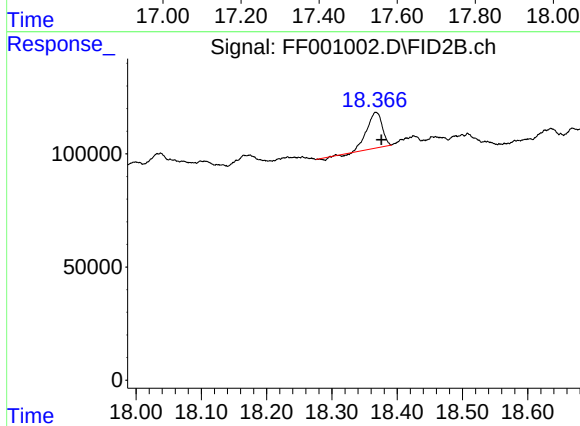

#14 N-DOTRIACONTANE

R.T.: 18.368 min
Delta R.T.: -0.008 min
Response: 251702
Conc: 2.05 ug/ml

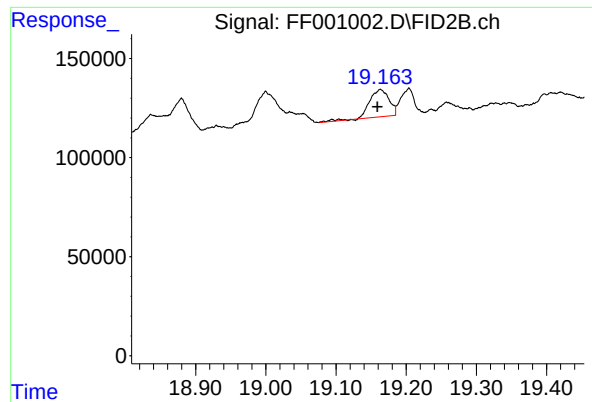

#15 N-TETRATRIACONTANE

R.T.: 19.163 min

Delta R.T.: 0.004 min

Response: 269656

Conc: 2.25 ug/ml

Instrument :
FID_F
ClientSampleId :