

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF001001.D
 Signal(s) : FID2B.ch
 Acq On : 19 Jun 2018 01:01
 Operator : UA\AJ
 Sample : J3567-10MSD
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:23:05 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.481	1910995	16.571 ug/ml
Target Compounds			
2) N-DECANE	4.242	2266228	16.174 ug/ml
3) N-DODECANE	6.255	2315761	16.523 ug/ml
4) N-TETRADECANE	8.044	2333486	16.760 ug/ml
5) N-HEXADECANE	9.640	2399571	17.404 ug/ml
6) N-OCTADECANE	11.078	2338372	17.124 ug/ml
7) N-EICOSANE	12.386	2202810	16.442 ug/ml
8) N-DOCOSANE	13.582	2147659	16.242 ug/ml
10) N-TETRACOSANE	14.683	2154437	16.610 ug/ml
11) N-HEXACOSANE	15.703	2133574	16.611 ug/ml
12) N-OCTACOSANE	16.652	2080341	16.360 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF001001.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2018 01:01
Operator : UA\AJ
Sample : J3567-10MSD
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:23:05 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

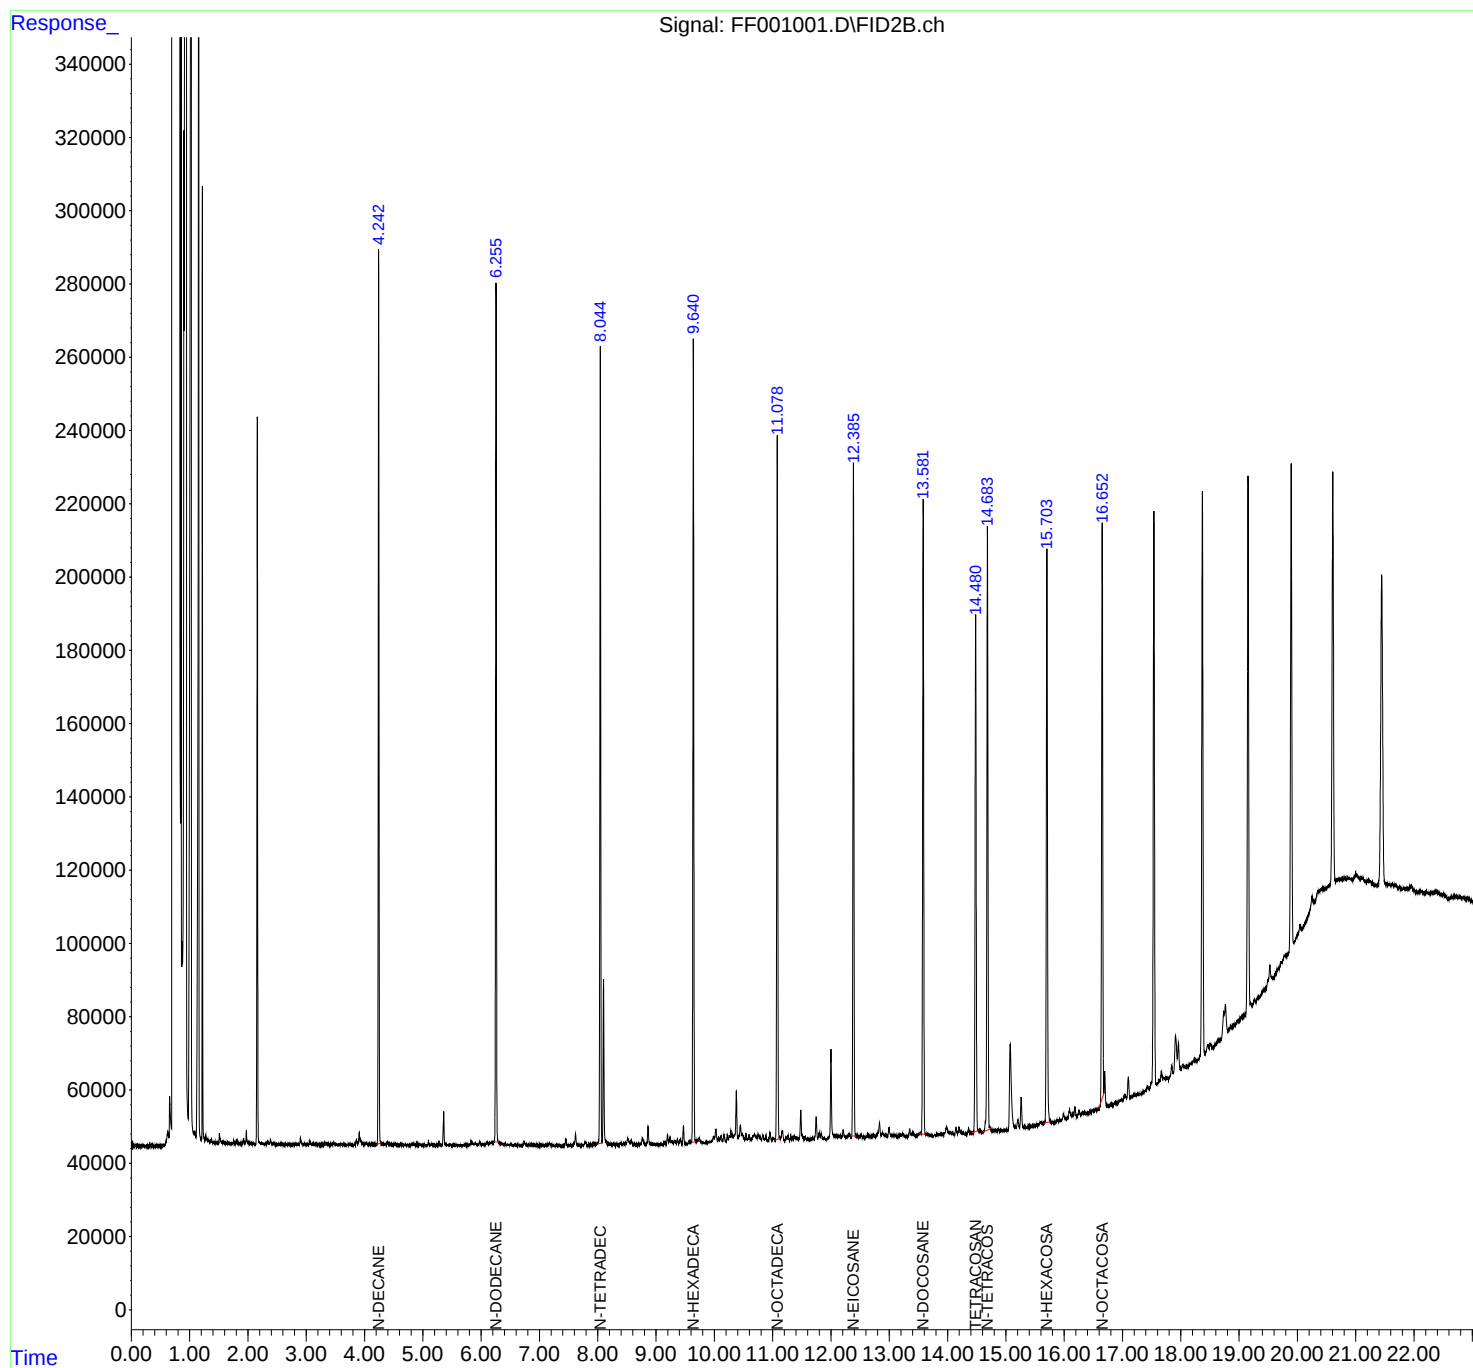


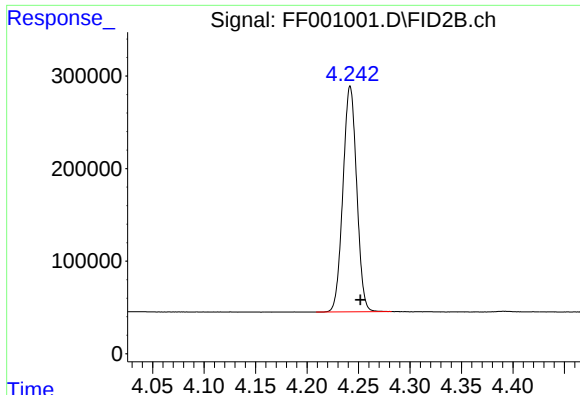

#2 N-DECANE


R.T.: 4.242 min
Delta R.T.: -0.010 min
Response: 2266228
Conc: 16.17 ug/ml

Instrument :
FID_F
ClientSampleId :

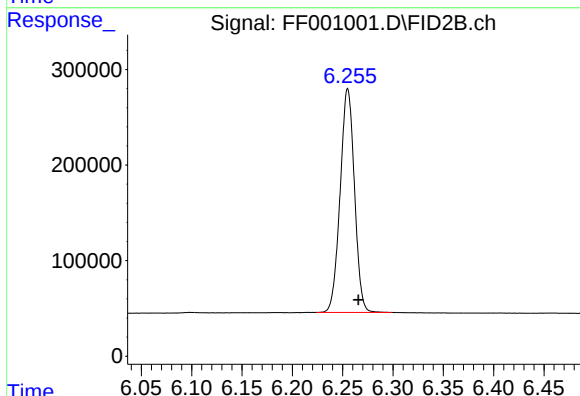


#3 N-DODECANE

R.T.: 6.255 min
Delta R.T.: -0.011 min
Response: 2315761
Conc: 16.52 ug/ml

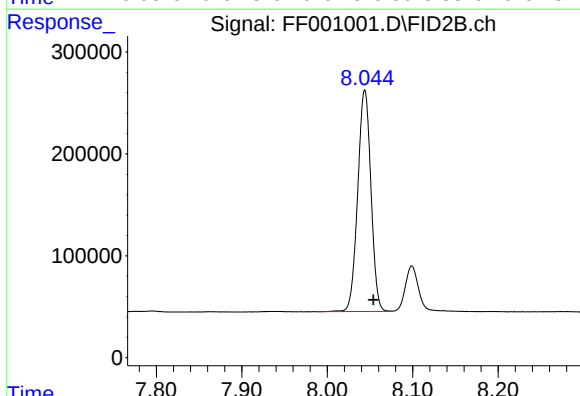


#4 N-TETRADECANE

R.T.: 8.044 min
Delta R.T.: -0.010 min
Response: 2333486
Conc: 16.76 ug/ml

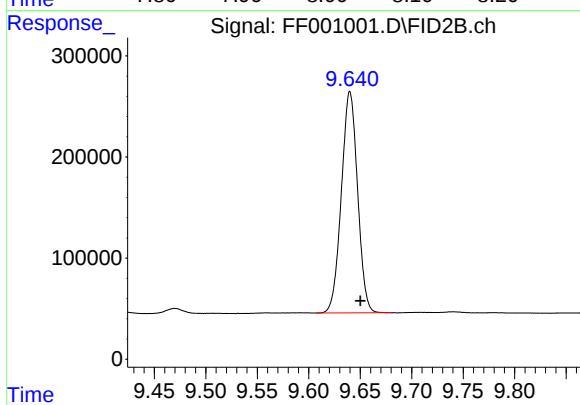

#5 N-HEXADECANE


R.T.: 9.640 min
Delta R.T.: -0.010 min
Response: 2399571
Conc: 17.40 ug/ml

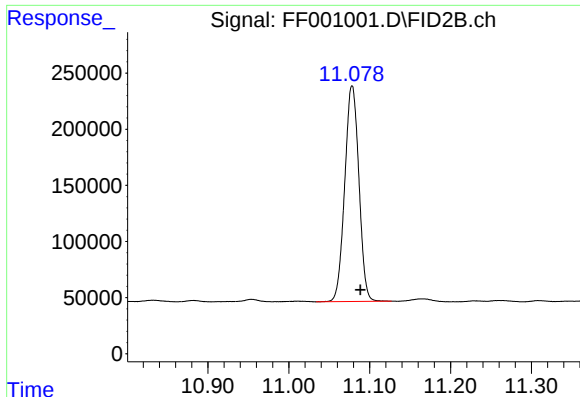

#6 N-OCTADECANE


R.T.: 11.078 min
Delta R.T.: -0.010 min
Response: 2338372
Conc: 17.12 ug/ml

Instrument :
FID_F
ClientSampleId :

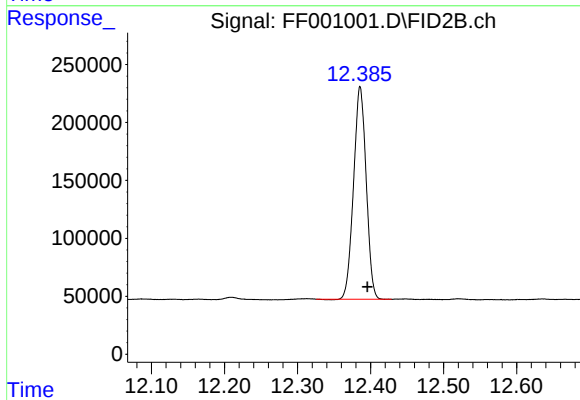


#7 N-EICOSANE

R.T.: 12.386 min
Delta R.T.: -0.010 min
Response: 2202810
Conc: 16.44 ug/ml

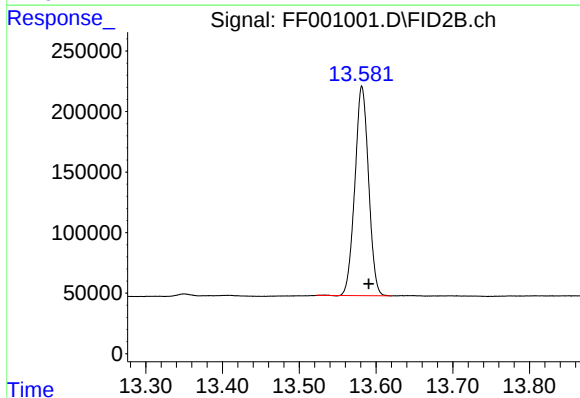


#8 N-DOCOSANE

R.T.: 13.582 min
Delta R.T.: -0.009 min
Response: 2147659
Conc: 16.24 ug/ml

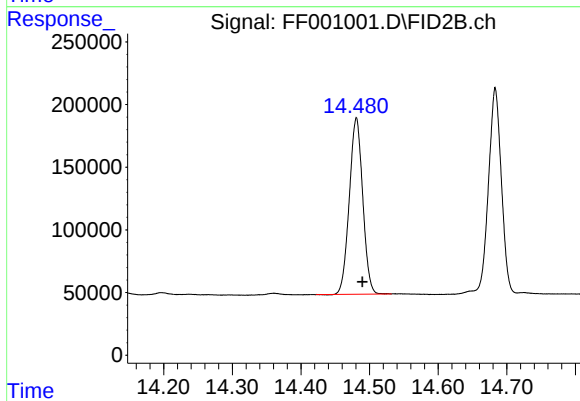

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.481 min
Delta R.T.: -0.009 min
Response: 1910995
Conc: 16.57 ug/ml

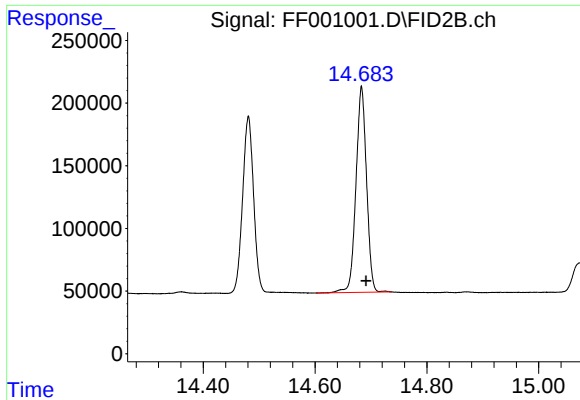

#10 N-TETRACOSANE


R.T.: 14.683 min
Delta R.T.: -0.008 min
Response: 2154437
Conc: 16.61 ug/ml

Instrument :
FID_F
ClientSampleId :

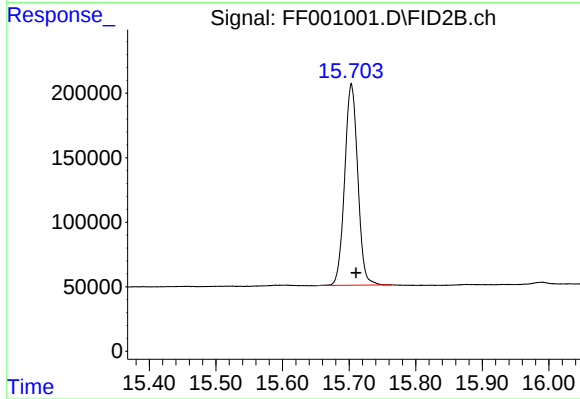

#11 N-HEXACOSANE

R.T.: 15.703 min
Delta R.T.: -0.007 min
Response: 2133574
Conc: 16.61 ug/ml

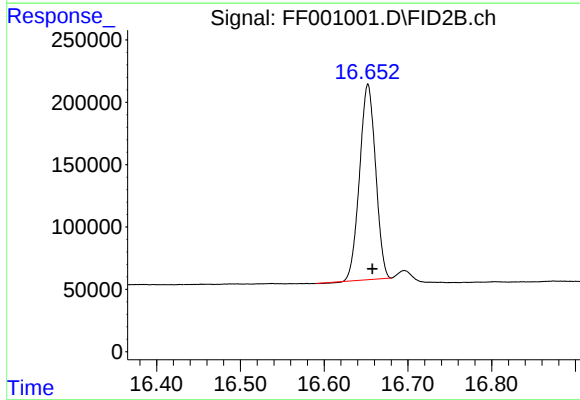

#12 N-OCTACOSANE

R.T.: 16.652 min
Delta R.T.: -0.005 min
Response: 2080341
Conc: 16.36 ug/ml