

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF001002.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2018 01:31
Operator : UA\AJ
Sample : J3240-03 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

UGO
6/19/2018 12:00:08 PM

Integration File: autoint1.e
Quant Time: Jun 19 09:23:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.478	329027	2.853 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF001002.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2018 01:31
Operator : UA\AJ
Sample : J3240-03 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :


Manual Integrations
APPROVED

UGO
6/19/2018 12:00:08 PM

Integration File: autoint1.e
Quant Time: Jun 19 09:23:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

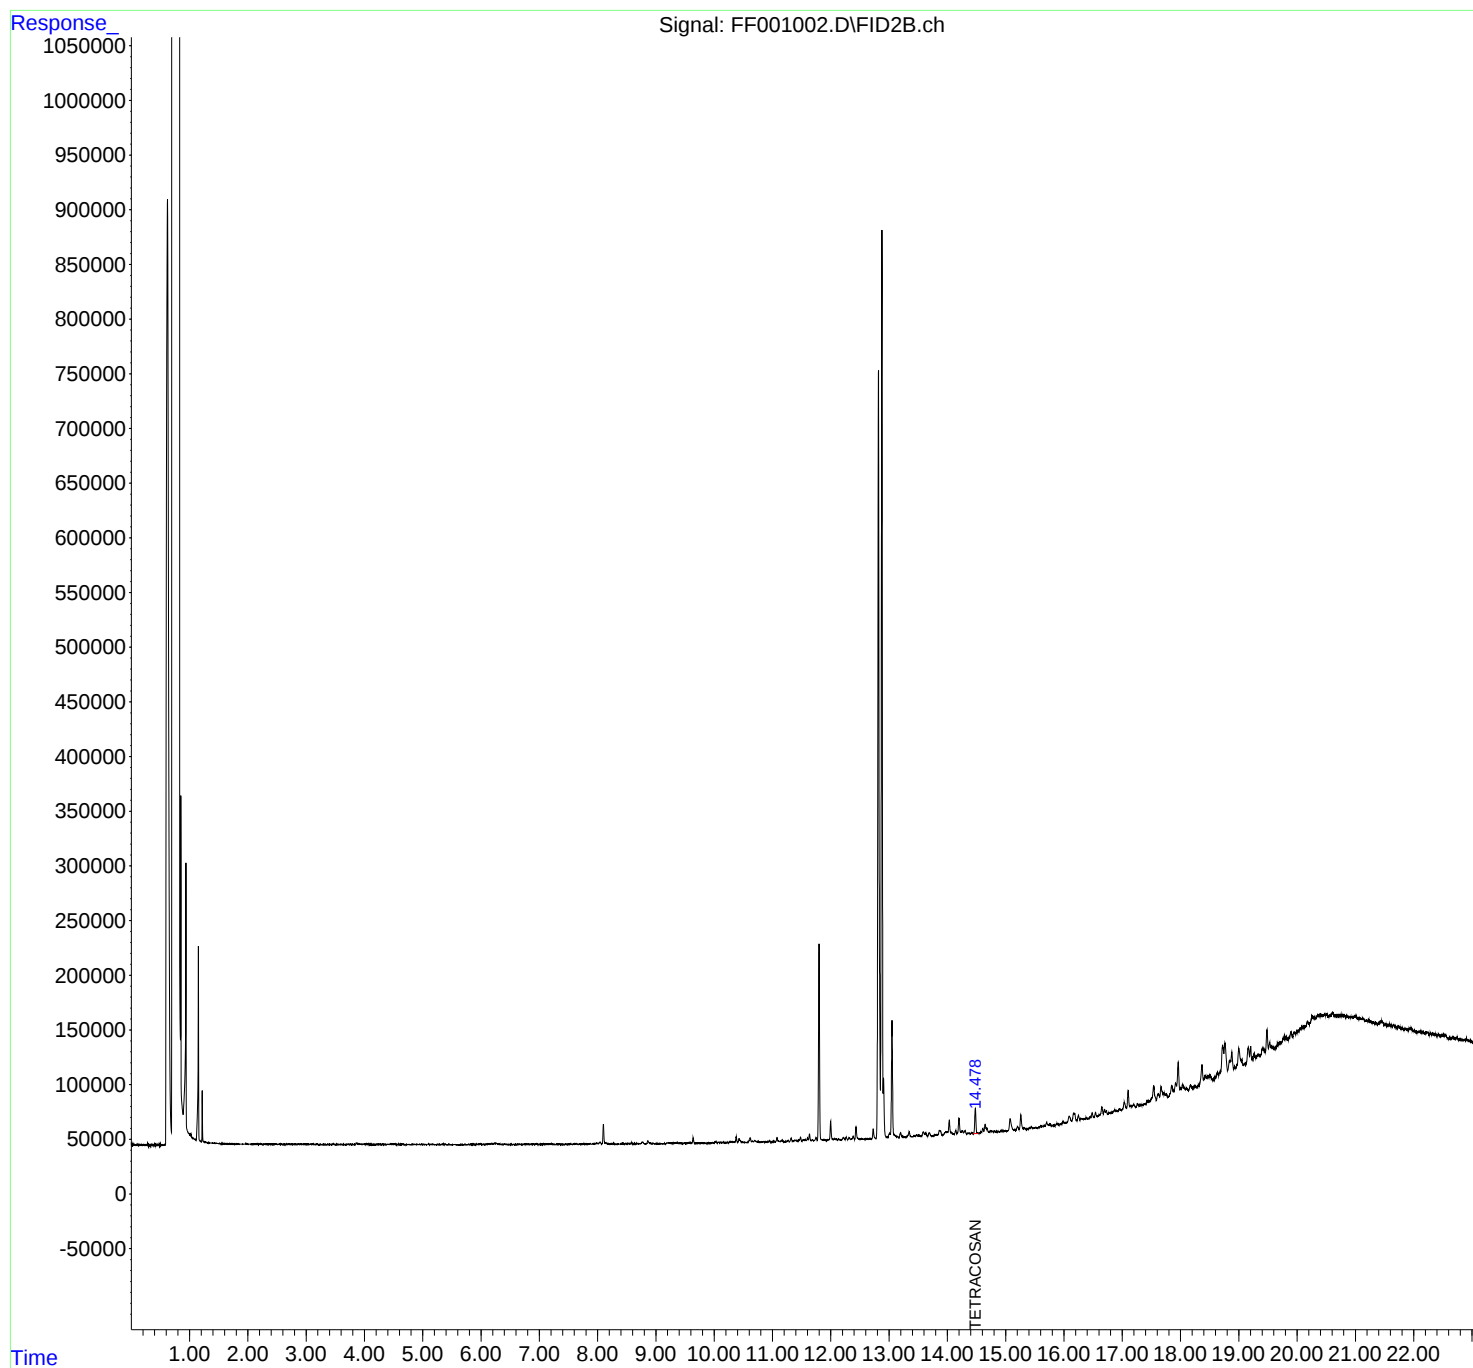

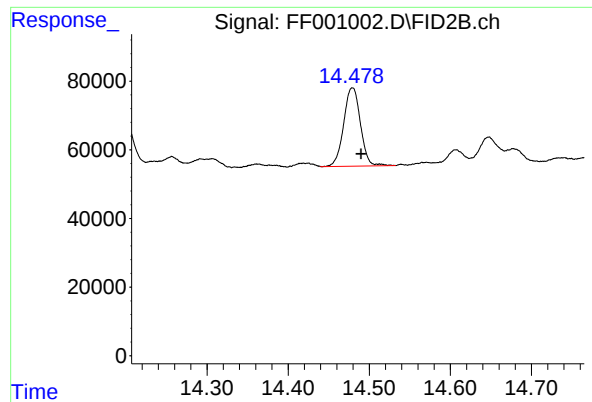

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.478 min
Delta R.T.: -0.011 min
Response: 329027
Conc: 2.85 ug/ml m

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

UGO
6/19/2018 12:00:08 PM