

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
 Data File : FF001004.D
 Signal(s) : FID2B.ch
 Acq On : 19 Jun 2018 02:32
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 19 09:23:50 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.484	5144951	44.613 ug/ml
Target Compounds			
2) N-DECANE	4.244	6742707	48.122 ug/ml
3) N-DODECANE	6.258	6597705	47.075 ug/ml
4) N-TETRADECANE	8.047	6460563	46.402 ug/ml
5) N-HEXADECANE	9.643	6319528	45.834 ug/ml
6) N-OCTADECANE	11.082	6193090	45.353 ug/ml
7) N-EICOSANE	12.389	6030097	45.008 ug/ml
8) N-DOCOSANE	13.586	5916350	44.744 ug/ml
10) N-TETRACOSANE	14.687	5865755	45.222 ug/ml
11) N-HEXACOSANE	15.707	5839281	45.461 ug/ml
12) N-OCTACOSANE	16.655	5885267	46.283 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061818\
Data File : FF001004.D
Signal(s) : FID2B.ch
Acq On : 19 Jun 2018 02:32
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 19 09:23:50 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

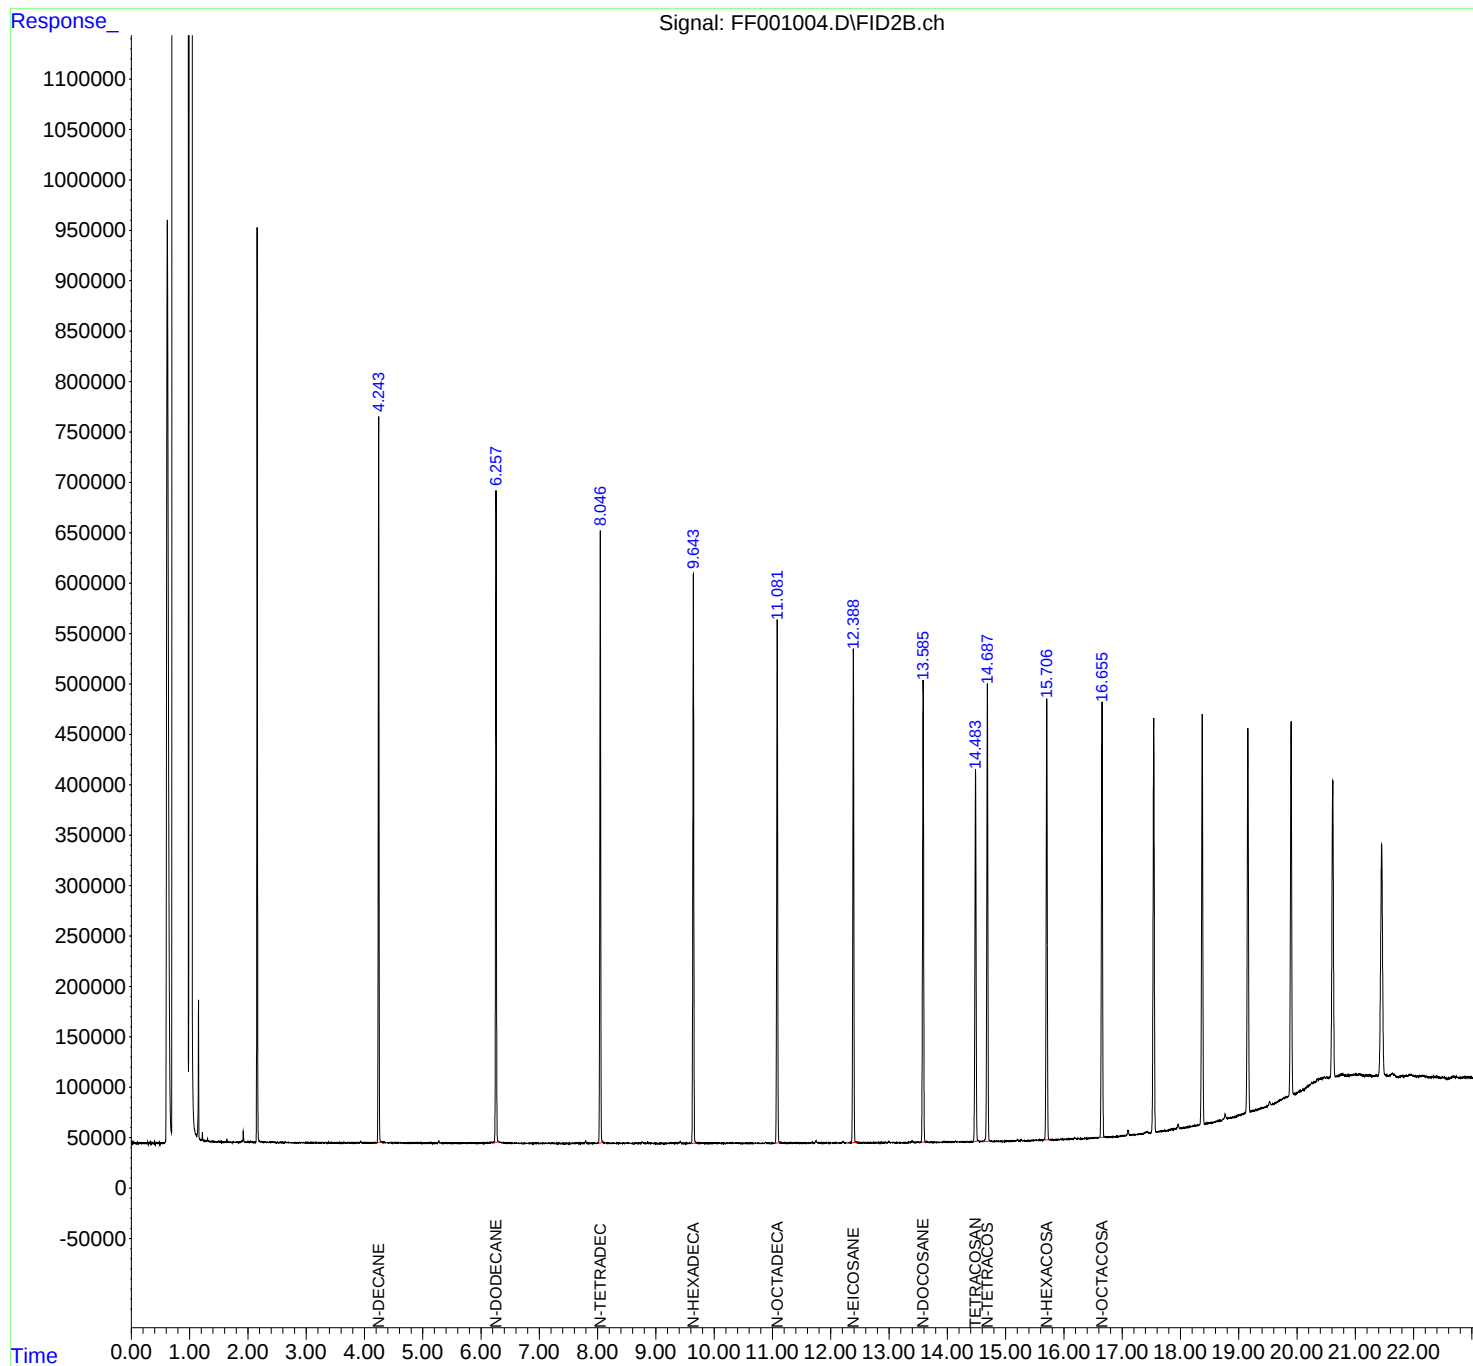


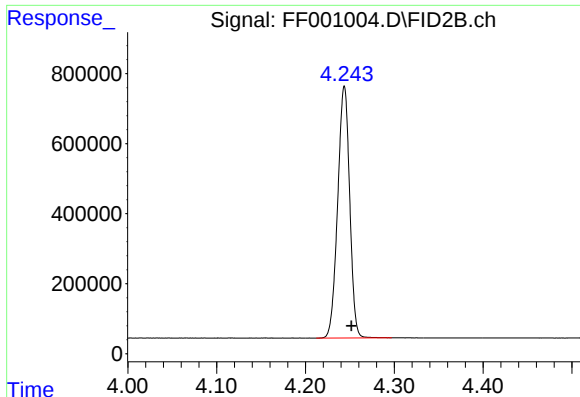

#2 N-DECANE


R.T.: 4.244 min
Delta R.T.: -0.008 min
Response: 6742707
Conc: 48.12 ug/ml

Instrument :
FID_F
ClientSampleId :

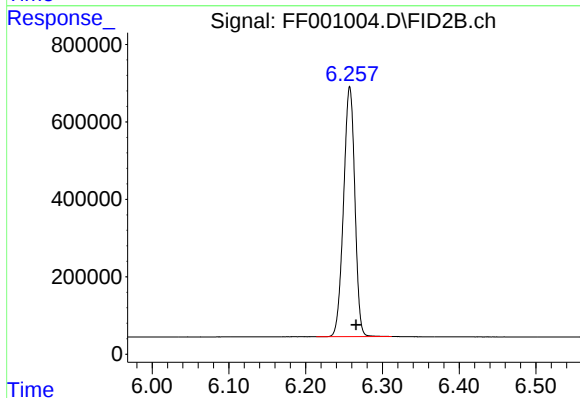


#3 N-DODECANE

R.T.: 6.258 min
Delta R.T.: -0.008 min
Response: 6597705
Conc: 47.08 ug/ml

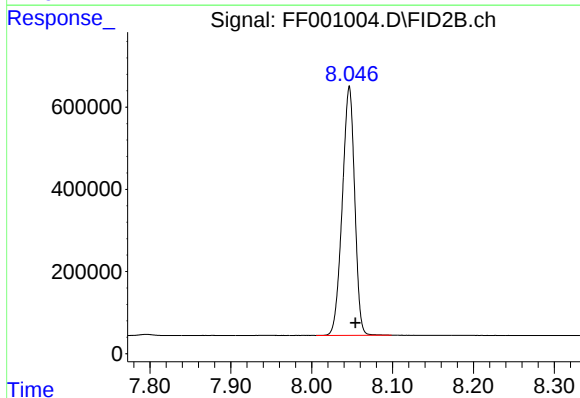


#4 N-TETRADECANE

R.T.: 8.047 min
Delta R.T.: -0.008 min
Response: 6460563
Conc: 46.40 ug/ml

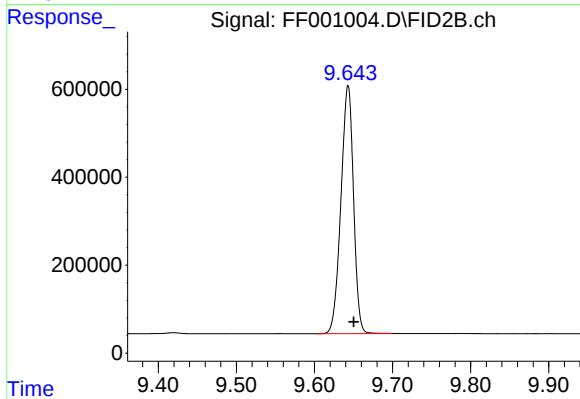

#5 N-HEXADECANE


R.T.: 9.643 min
Delta R.T.: -0.007 min
Response: 6319528
Conc: 45.83 ug/ml

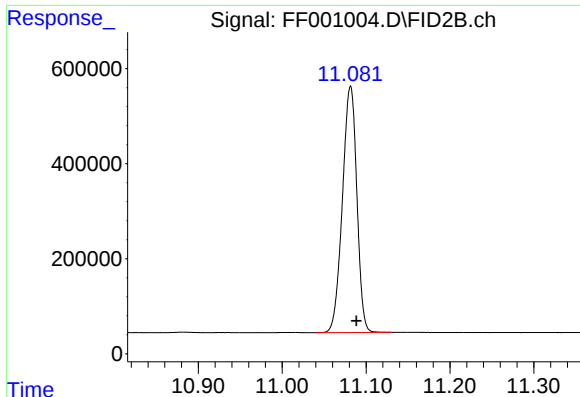

#6 N-OCTADECANE


R.T.: 11.082 min
Delta R.T.: -0.007 min
Response: 6193090
Conc: 45.35 ug/ml

Instrument :
FID_F
ClientSampleId :

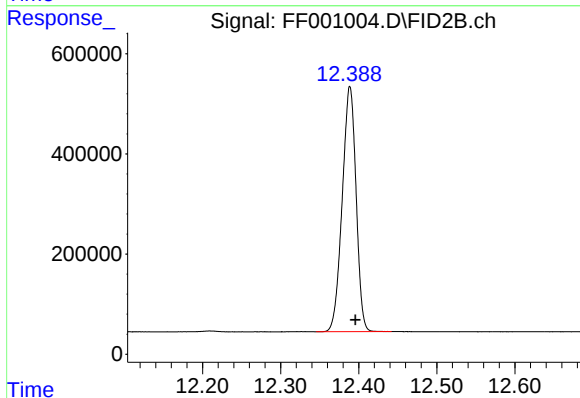


#7 N-EICOSANE

R.T.: 12.389 min
Delta R.T.: -0.007 min
Response: 6030097
Conc: 45.01 ug/ml

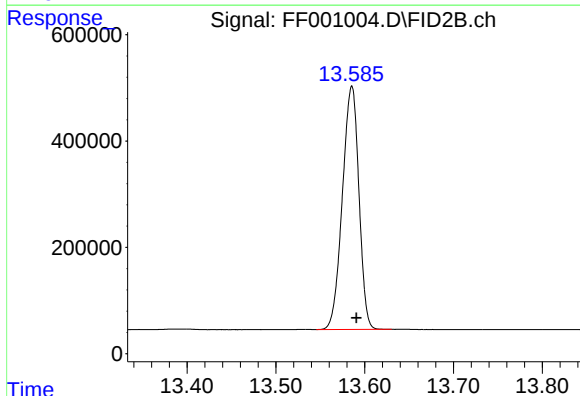


#8 N-DOCOSANE

R.T.: 13.586 min
Delta R.T.: -0.005 min
Response: 5916350
Conc: 44.74 ug/ml

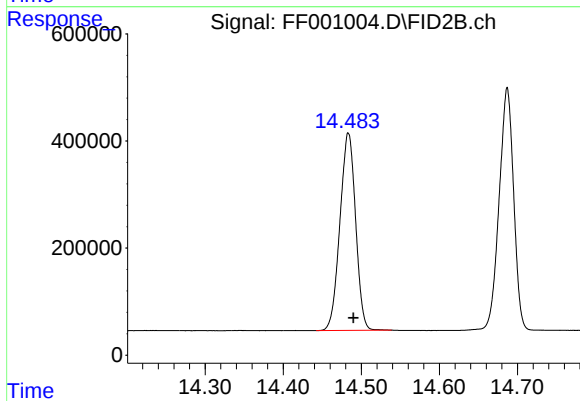

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.484 min
Delta R.T.: -0.006 min
Response: 5144951
Conc: 44.61 ug/ml

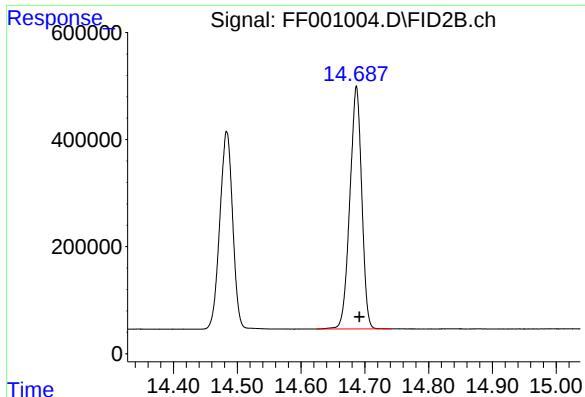

#10 N-TETRACOSANE


R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 5865755
Conc: 45.22 ug/ml

Instrument :
FID_F
ClientSampleId :

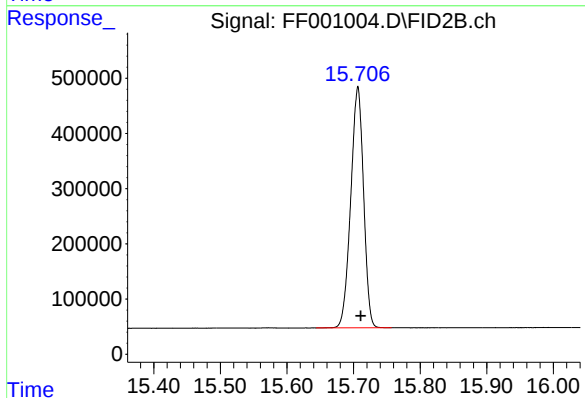

#11 N-HEXACOSANE

R.T.: 15.707 min
Delta R.T.: -0.004 min
Response: 5839281
Conc: 45.46 ug/ml

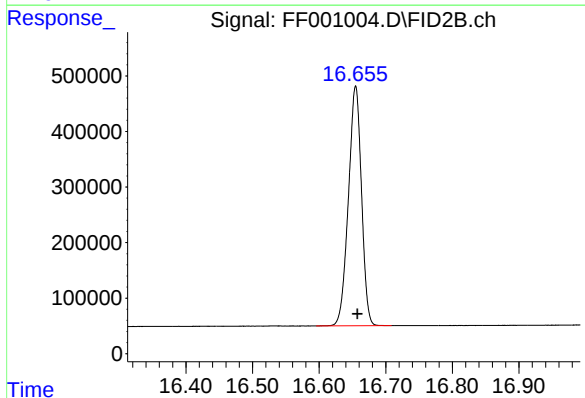

#12 N-OCTACOSANE

R.T.: 16.655 min
Delta R.T.: -0.003 min
Response: 5885267
Conc: 46.28 ug/ml