

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061819\
 Data File : FF004826.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2019 17:21
 Operator : DD\AJ
 Sample : K3158-03 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 19 01:08:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.704	217461	1.781 ug/ml
Target Compounds			
7) N-EICOSANE	12.654	457804	3.161 ug/ml
10) N-TETRACOSANE	14.883	271636	1.960 ug/ml
11) N-HEXACOSANE	15.937	83515	0.613 ug/ml
12) N-OCTACOSANE	16.892	104081	0.766 ug/ml
13) N-TRIACONTANE	17.781	241213	1.744 ug/ml
14) N-DOTRIACONTANE	18.621	163718	1.184 ug/ml
15) N-TETRATRIACONTANE	19.418	131187	0.960 ug/ml
16) N-HEXATRIACONTANE	20.154	276720	2.102 ug/ml
17) N-OCTATRIACONTANE	20.875	405754	3.374 ug/ml
18) N-TETRACONTANE	21.855	46793	0.380 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061819\
Data File : FF004826.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2019 17:21
Operator : DD\AJ
Sample : K3158-03 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 19 01:08:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

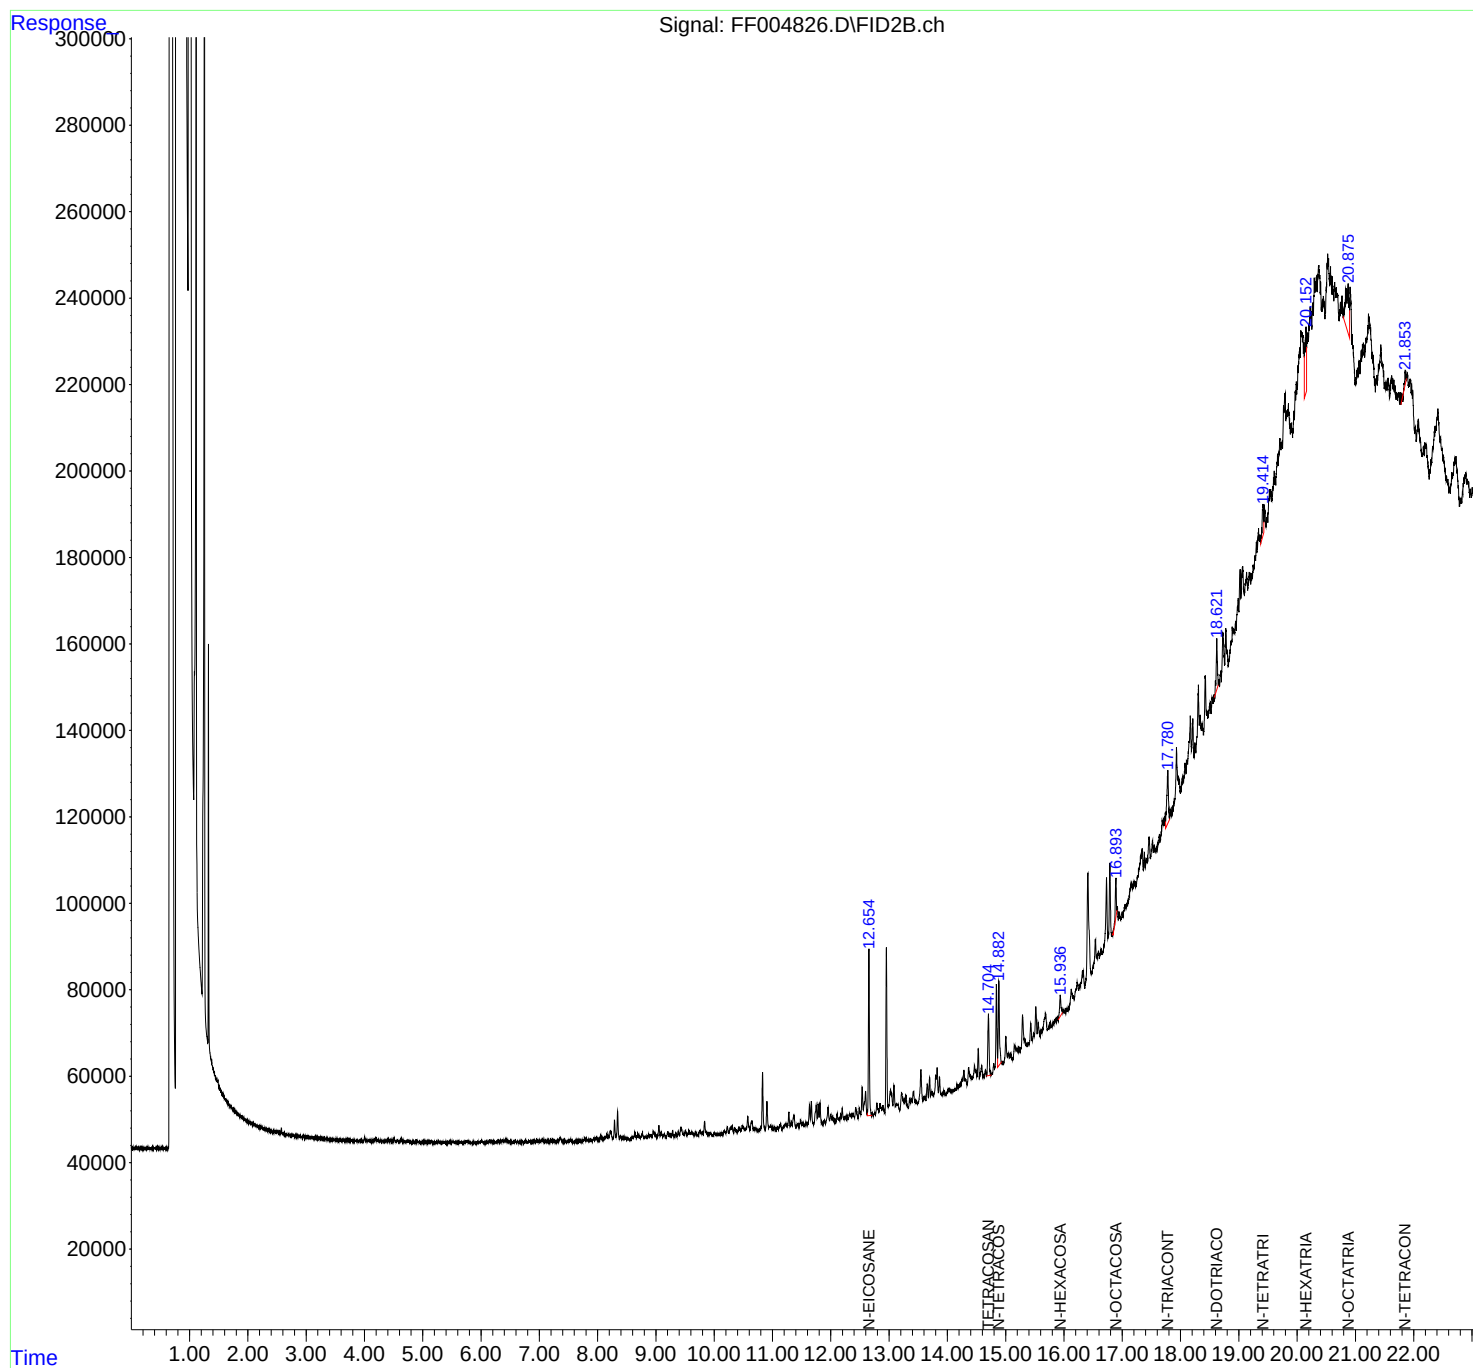

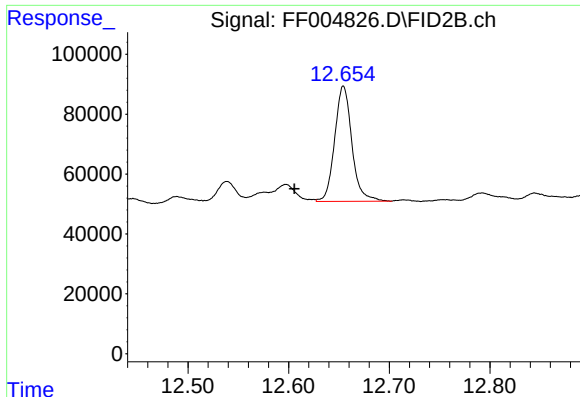


#7 N-EICOSANE

R.T.: 12.654 min
Delta R.T.: 0.049 min
Response: 457804
Conc: 3.16 ug/ml

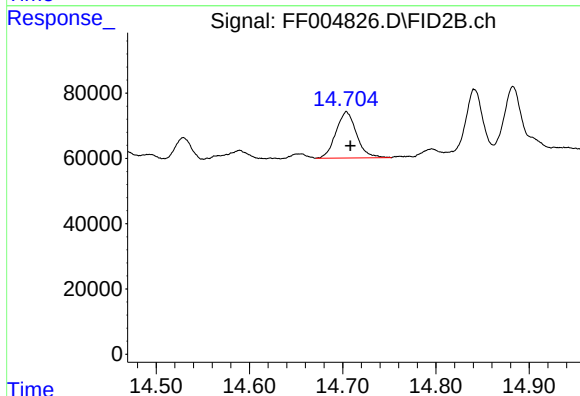


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.704 min
Delta R.T.: -0.004 min
Response: 217461
Conc: 1.78 ug/ml

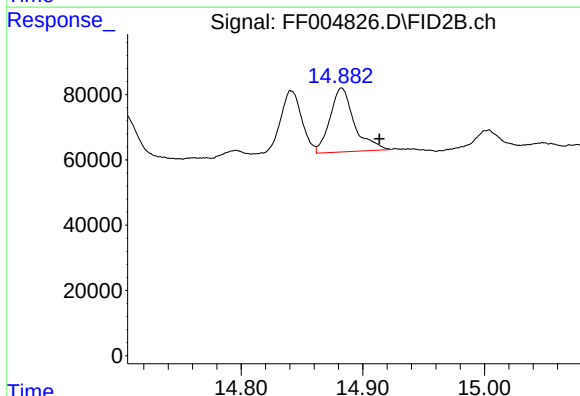


#10 N-TETRACOSANE

R.T.: 14.883 min
Delta R.T.: -0.031 min
Response: 271636
Conc: 1.96 ug/ml

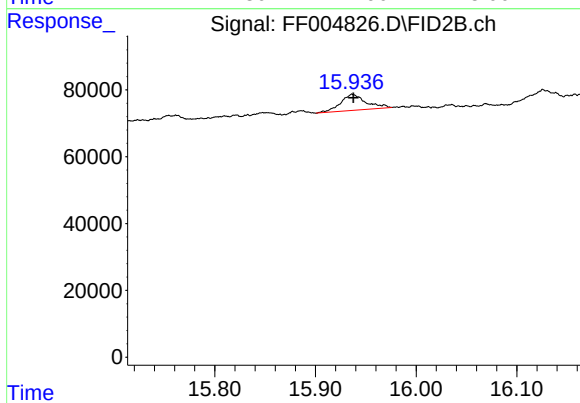


#11 N-HEXACOSANE

R.T.: 15.937 min
Delta R.T.: 0.000 min
Response: 83515
Conc: 0.61 ug/ml

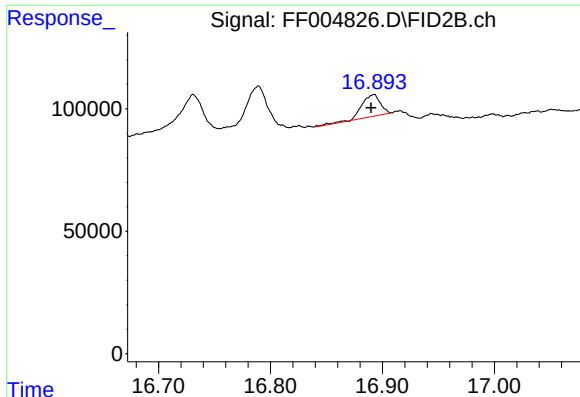


#12 N-OCTACOSANE

R.T.: 16.892 min
Delta R.T.: 0.002 min
Response: 104081
Conc: 0.77 ug/ml

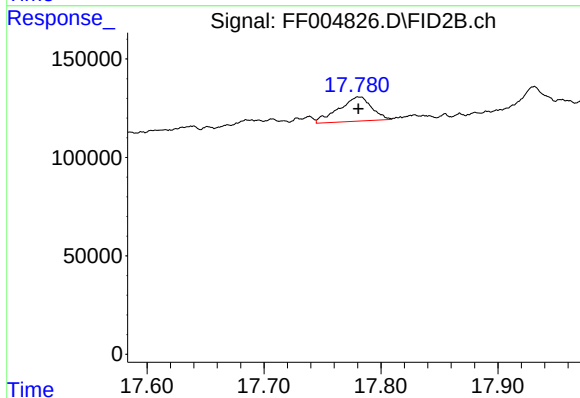


#13 N-TRIACONTANE

R.T.: 17.781 min
Delta R.T.: 0.000 min
Response: 241213
Conc: 1.74 ug/ml

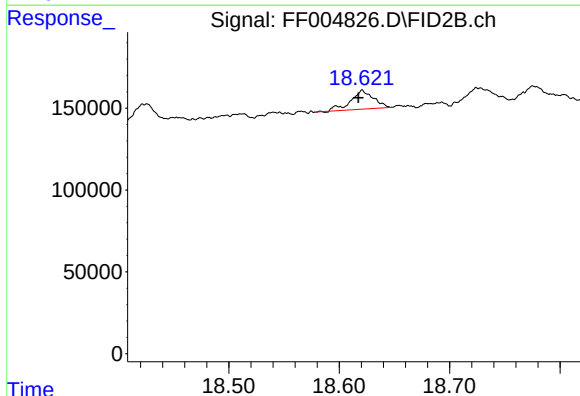


#14 N-DOTRIACONTANE

R.T.: 18.621 min
Delta R.T.: 0.004 min
Response: 163718
Conc: 1.18 ug/ml

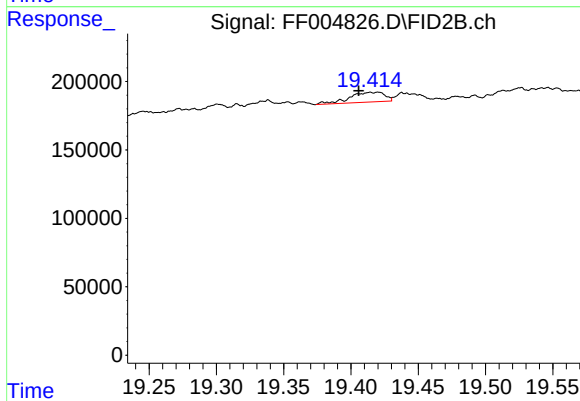


#15 N-TETRATRIACONTANE

R.T.: 19.418 min
Delta R.T.: 0.012 min
Response: 131187
Conc: 0.96 ug/ml

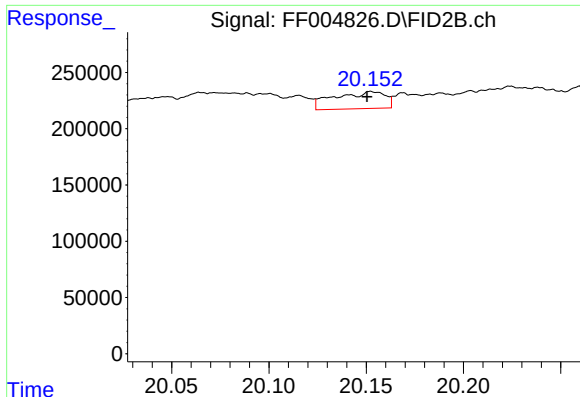


#16 N-HEXATRIACONTANE

R.T.: 20.154 min
Delta R.T.: 0.003 min
Response: 276720
Conc: 2.10 ug/ml

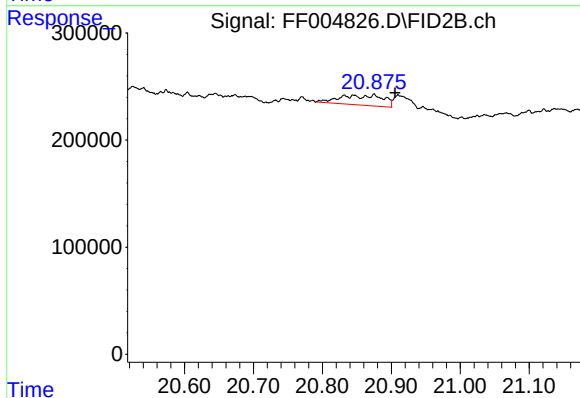

#17 N-OCTATRIACONTANE

R.T.: 20.875 min
Delta R.T.: -0.030 min
Response: 405754
Conc: 3.37 ug/ml

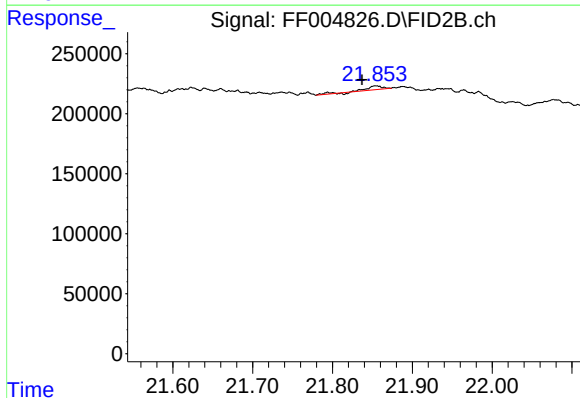

#18 N-TETRACONTANE

R.T.: 21.855 min
Delta R.T.: 0.018 min
Response: 46793
Conc: 0.38 ug/ml