

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061820\
 Data File : FF007056.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2020 11:46
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Jun 19 01:56:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
 Quant Title :
 QLast Update : Tue Jun 16 04:06:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.475	2915952	21.249 ug/ml
12) N-OCTACOSANE	16.910	2927723	19.638 ug/ml
13) N-TRIACONTANE	17.795	246870	1.645 ug/ml
14) N-DOTRIACONTANE	18.629	266328	1.928 ug/ml
15) N-TETRATRIACONTANE	19.414	192689	1.737 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061820\
Data File : FF007056.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2020 11:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 19 01:56:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

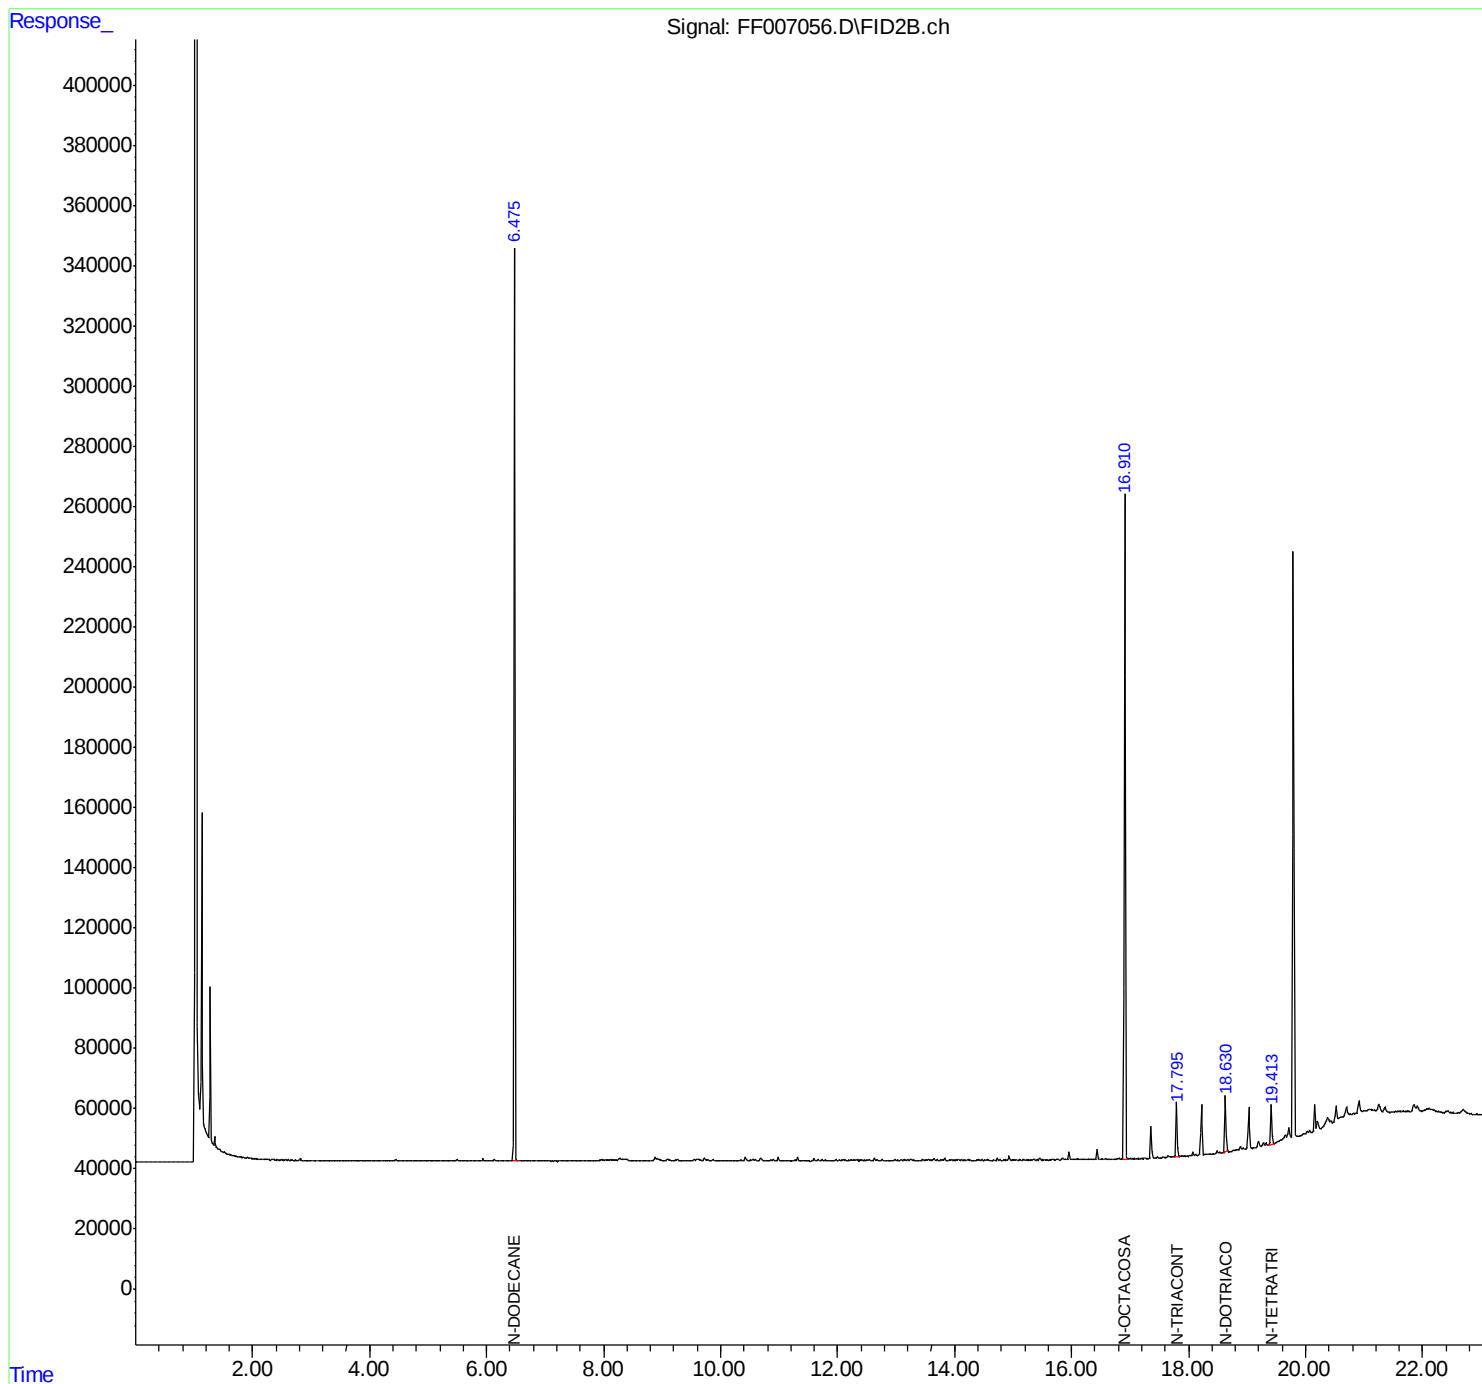


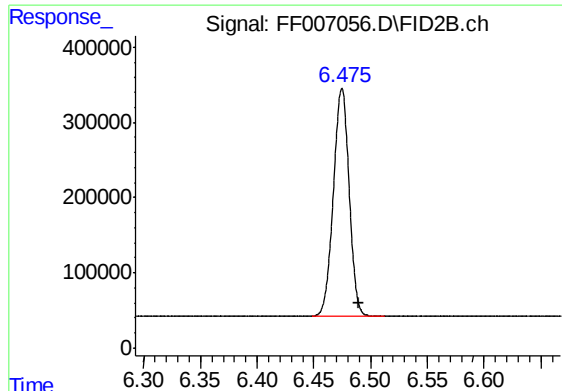

#3 N-DODECANE


R.T.: 6.475 min
Delta R.T.: -0.015 min
Response: 2915952
Conc: 21.25 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

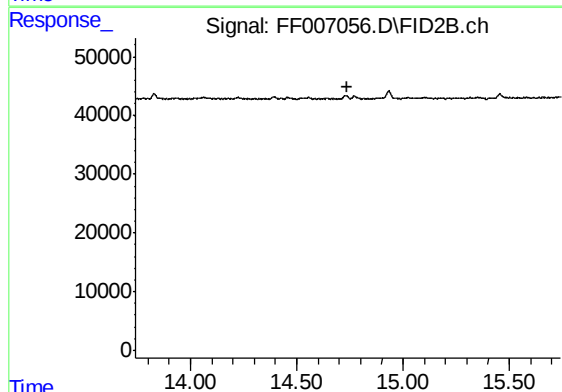


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.741 min
Response: 0
Conc: N.D.

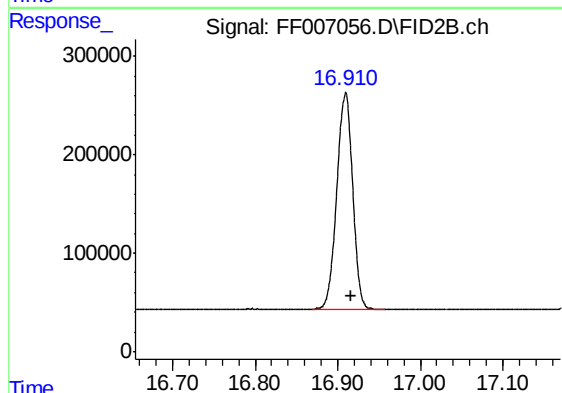


#12 N-OCTACOSANE

R.T.: 16.910 min
Delta R.T.: -0.006 min
Response: 2927723
Conc: 19.64 ug/ml

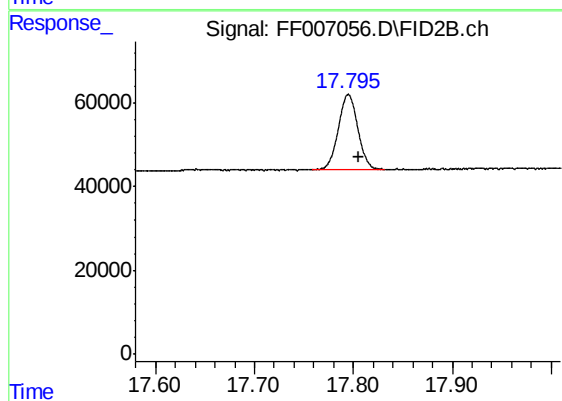

#13 N-TRIACONTANE


R.T.: 17.795 min
Delta R.T.: -0.010 min
Response: 246870
Conc: 1.65 ug/ml

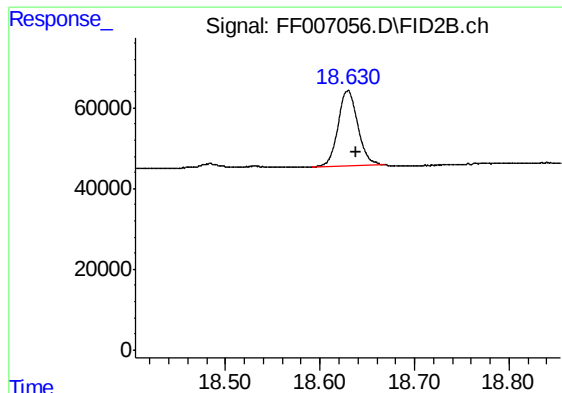

#14 N-DOTRIACONTANE

R.T.: 18.629 min
Delta R.T.: -0.009 min
Response: 266328
Conc: 1.93 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

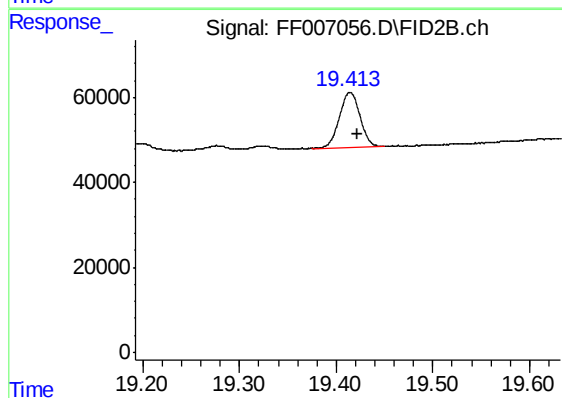

#15 N-TETRATRIACONTANE

R.T.: 19.414 min
Delta R.T.: -0.008 min
Response: 192689
Conc: 1.74 ug/ml