

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061820\
 Data File : FF007059.D
 Signal(s) : FID2B.ch
 Acq On : 18 Jun 2020 15:13
 Operator : DD\AJ
 Sample : L3031-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 LOT-11

Integration File: autoint1.e
 Quant Time: Jun 19 01:57:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
 Quant Title :
 QLast Update : Tue Jun 16 04:06:59 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	3245802	27.572 ug/ml
Target Compounds			
4) N-TETRADECANE	8.336f	376912	2.757 ug/ml
7) N-EICOSANE	12.698f	4192906	30.695 ug/ml
8) N-DOCOSANE	13.859	562657	4.129 ug/ml
10) N-TETRACOSANE	14.917	2179109	13.251 ug/ml
12) N-OCTACOSANE	16.913	624181	4.187 ug/ml
13) N-TRIACONTANE	17.800	335197	2.234 ug/ml
14) N-DOTRIACONTANE	18.622	233226	1.688 ug/ml
15) N-TETRATRIACONTANE	19.485f	209495	1.888 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF061820\
Data File : FF007059.D
Signal(s) : FID2B.ch
Acq On : 18 Jun 2020 15:13
Operator : DD\AJ
Sample : L3031-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
LOT-11

Integration File: autoint1.e
Quant Time: Jun 19 01:57:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF061520.M
Quant Title :
QLast Update : Tue Jun 16 04:06:59 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

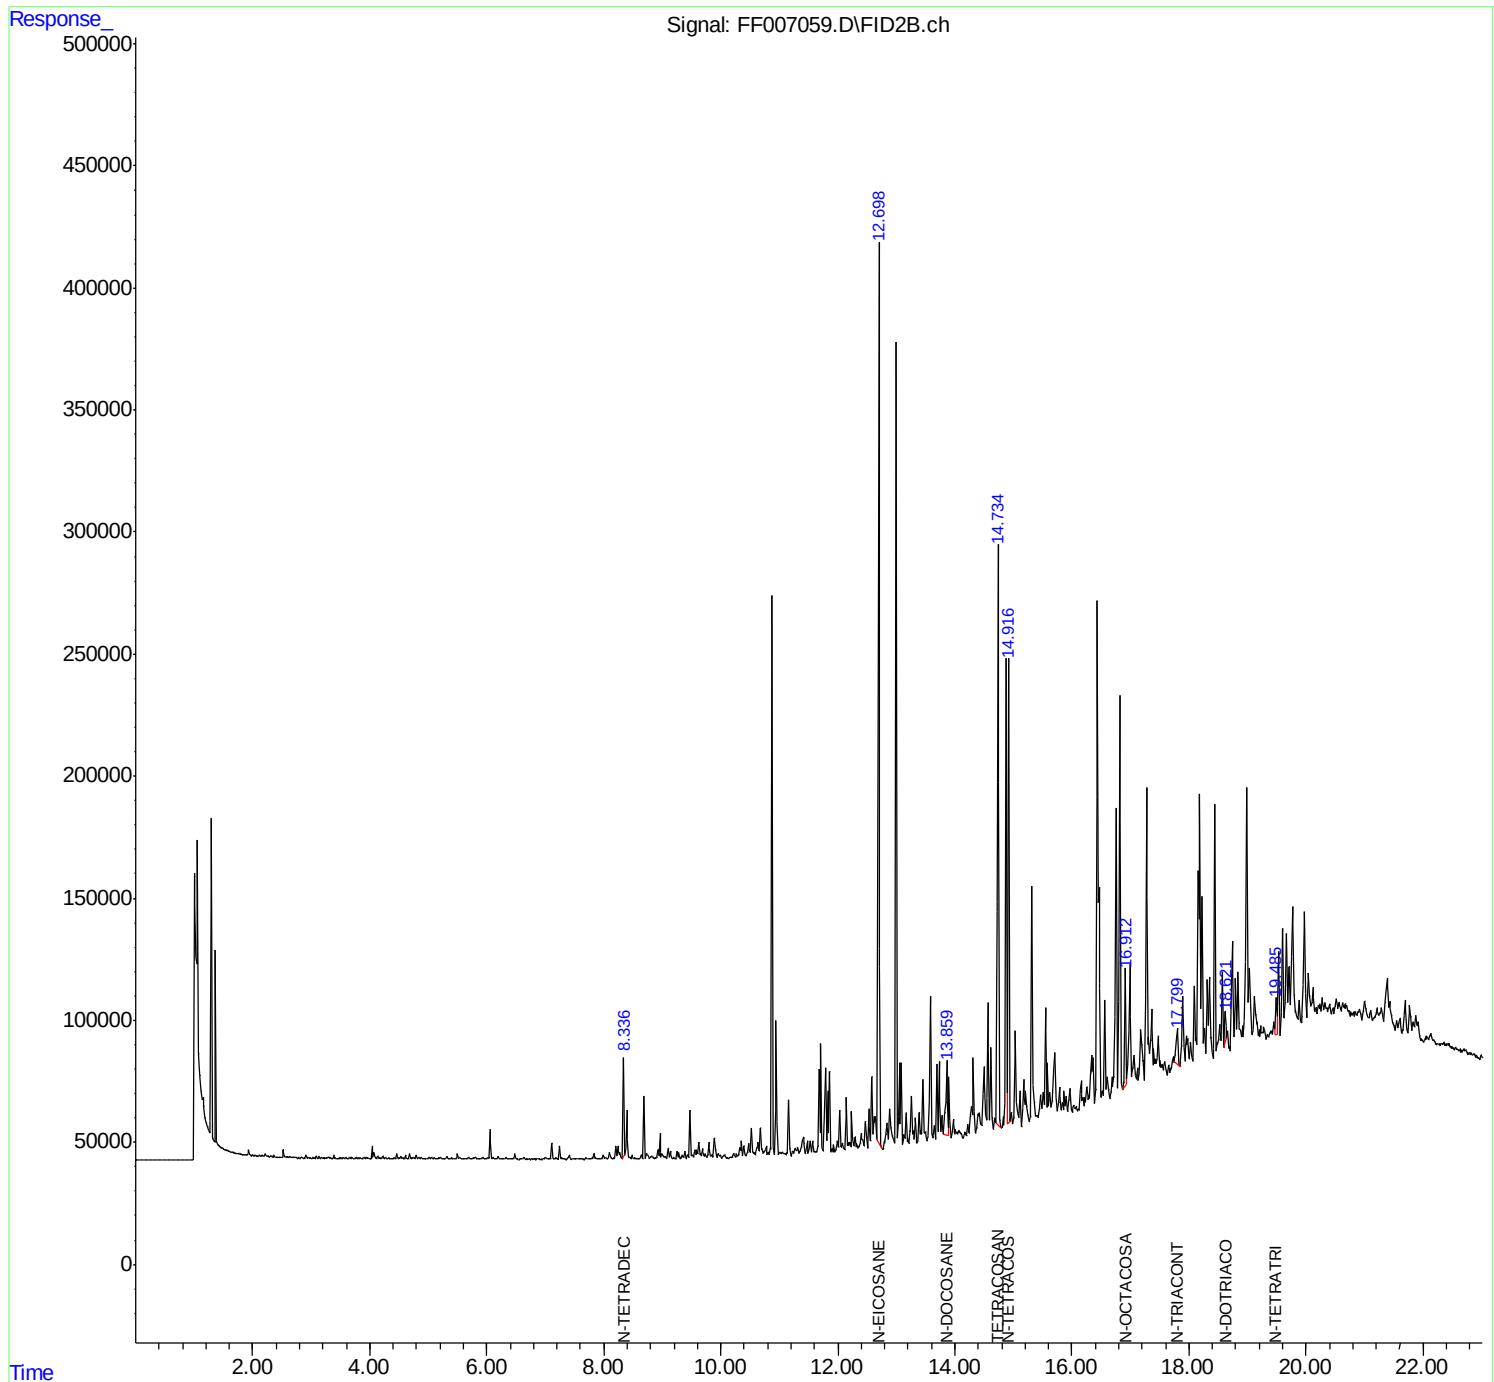


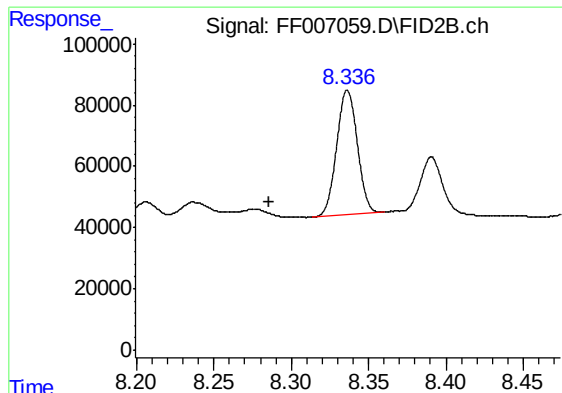

#4 N-TETRADECANE


R.T.: 8.336 min
Delta R.T.: 0.050 min
Response: 376912
Conc: 2.76 ug/ml

Instrument :
FID_F
ClientSampleId :
LOT-11

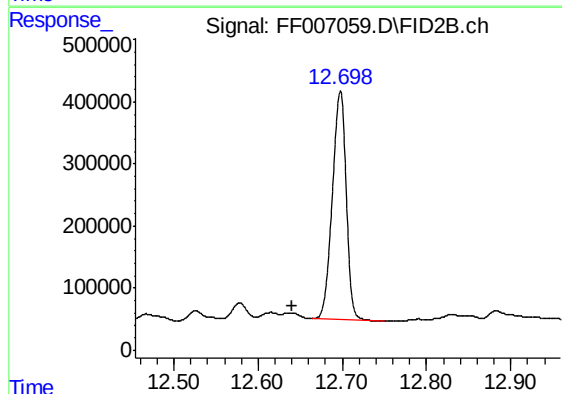


#7 N-EICOSANE

R.T.: 12.698 min
Delta R.T.: 0.057 min
Response: 4192906
Conc: 30.69 ug/ml

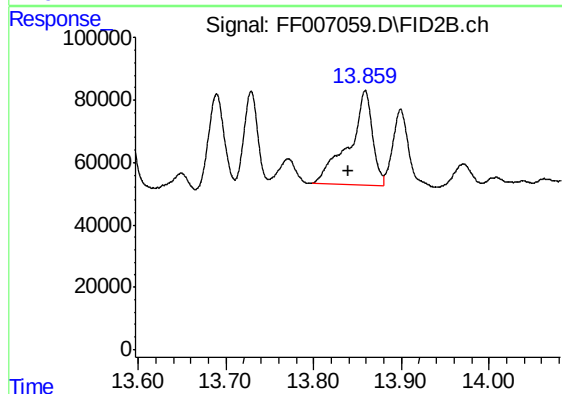


#8 N-DOCOSANE

R.T.: 13.859 min
Delta R.T.: 0.019 min
Response: 562657
Conc: 4.13 ug/ml

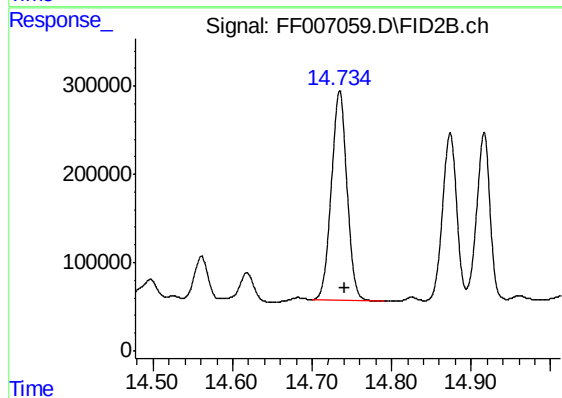

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.735 min
Delta R.T.: -0.006 min
Response: 3245802
Conc: 27.57 ug/ml

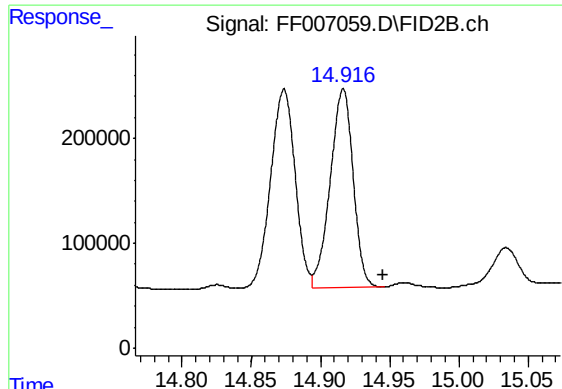

#10 N-TETRACOSANE


R.T.: 14.917 min
Delta R.T.: -0.029 min
Response: 2179109
Conc: 13.25 ug/ml

Instrument :
FID_F
ClientSampleId :
LOT-11

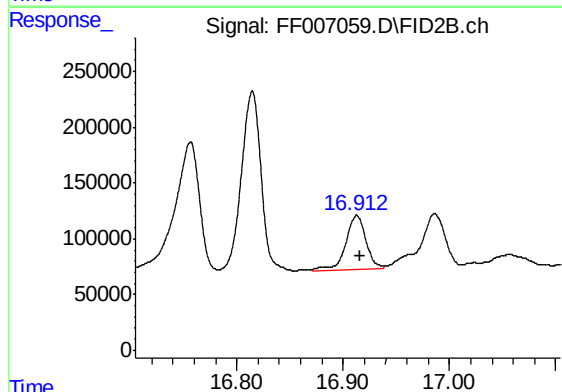


#12 N-OCTACOSANE

R.T.: 16.913 min
Delta R.T.: -0.004 min
Response: 624181
Conc: 4.19 ug/ml

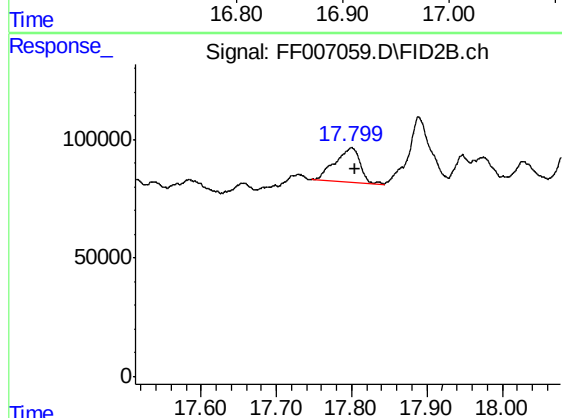


#13 N-TRIACONTANE

R.T.: 17.800 min
Delta R.T.: -0.006 min
Response: 335197
Conc: 2.23 ug/ml

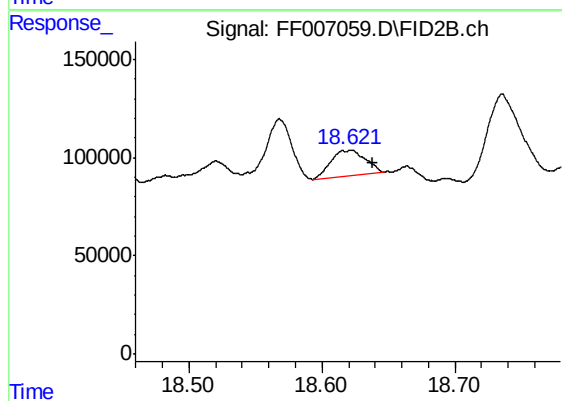

#14 N-DOTRIACONTANE

R.T.: 18.622 min
Delta R.T.: -0.016 min
Response: 233226
Conc: 1.69 ug/ml

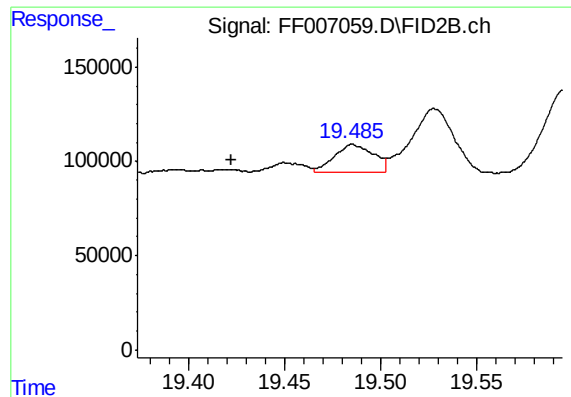

#15 N-TETRATRIACONTANE

R.T.: 19.485 min

Delta R.T.: 0.063 min

Response: 209495

Conc: 1.89 ug/ml

Instrument :
FID_F
ClientSampleId :
LOT-11